
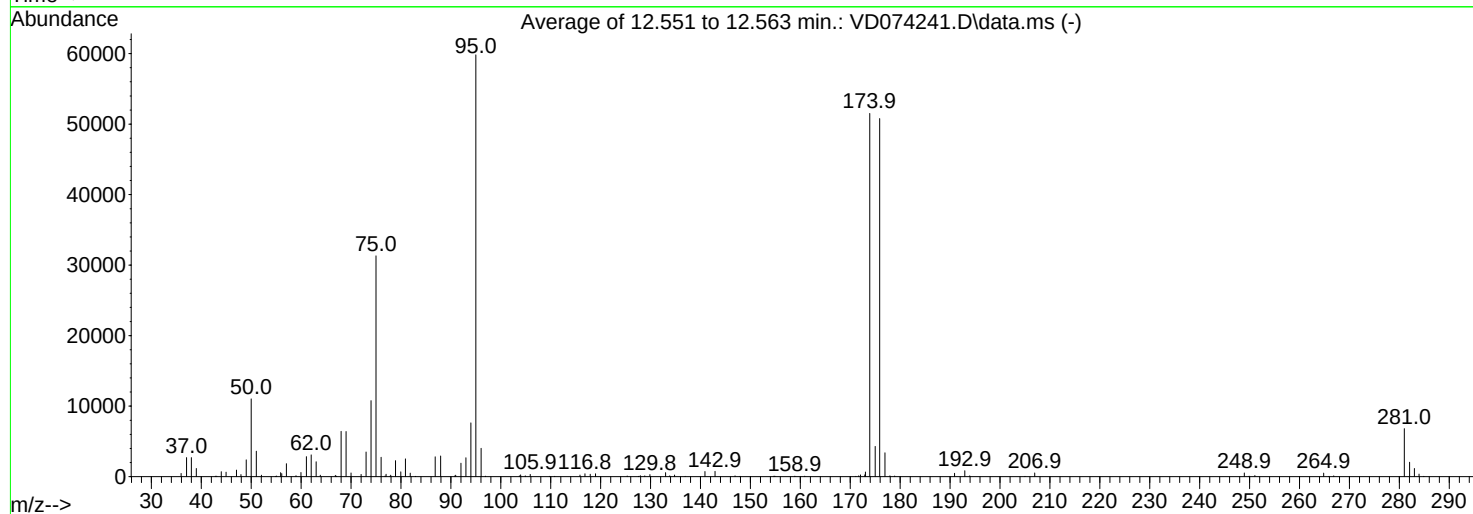


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD090922\
Data File : VD074241.D
Acq On : 09 Sep 2022 14:02
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090922S.M
Title : SW846 8260
Last Update : Sat Sep 10 04:45:19 2022

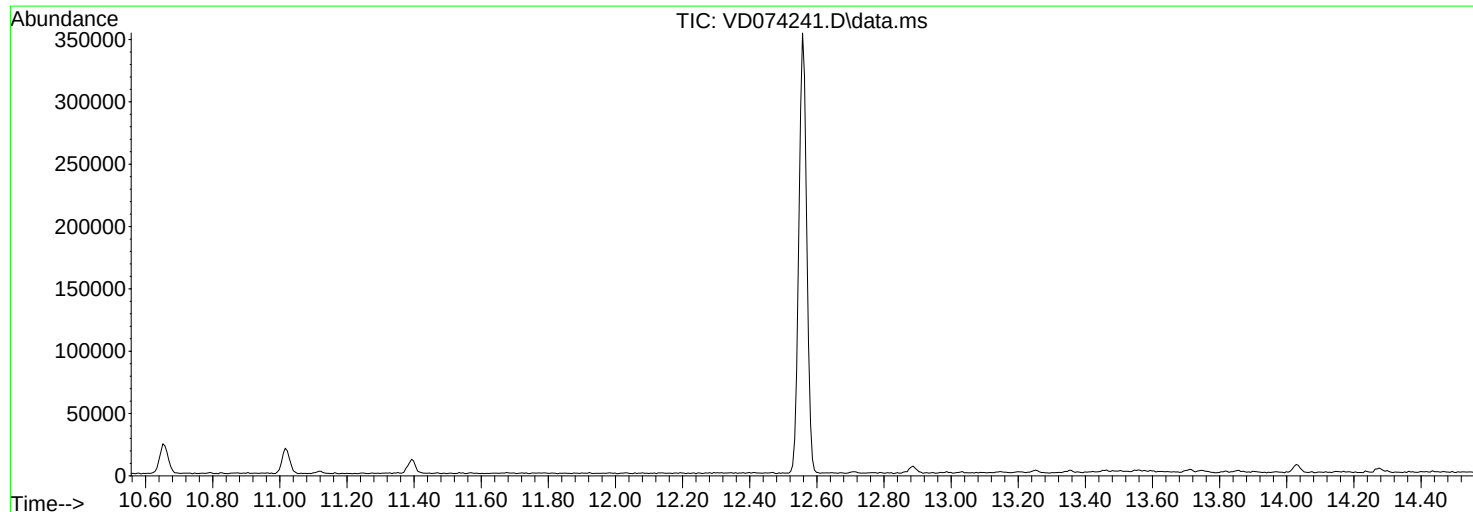

AutoFind: Scans 1864, 1865, 1866; Background Corrected with Scan 1856

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	11020	PASS
75	95	30	60	52.4	31331	PASS
95	95	100	100	100.0	59827	PASS
96	95	5	9	6.7	4019	PASS
173	174	0.00	2	1.3	669	PASS
174	95	50	100	86.1	51525	PASS
175	174	5	9	8.3	4281	PASS
176	174	95	101	98.6	50784	PASS
177	176	5	9	6.7	3384	PASS