


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD091018\
 Data File : VD059984.D
 Acq On : 10 Sep 2018 9:50
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampled :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
 Title : SW846 8260
 Last Update : Thu Aug 23 03:03:08 2018

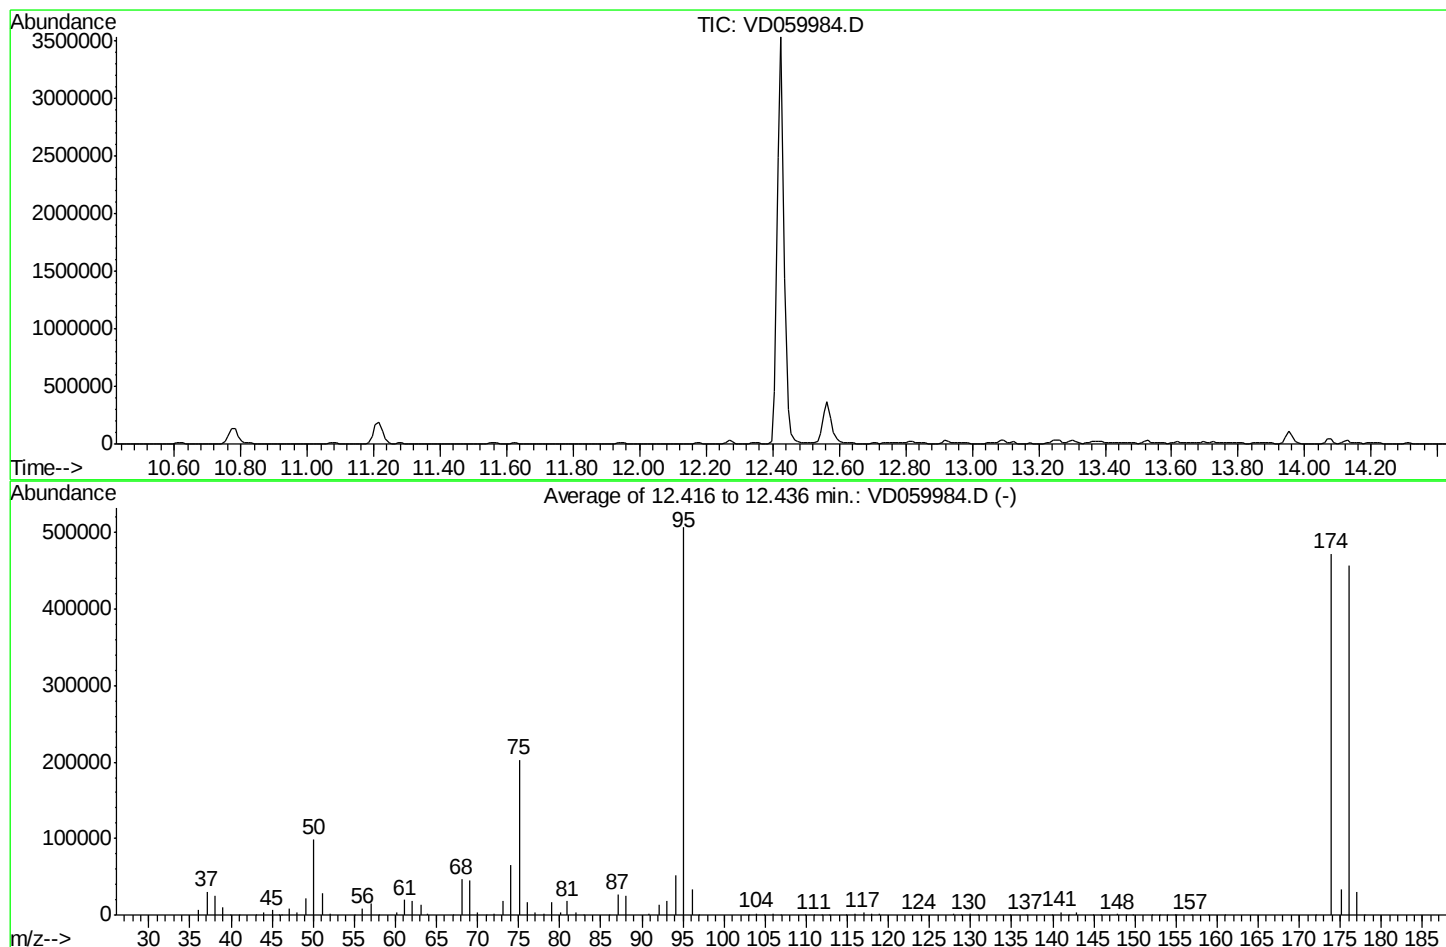

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	98693	PASS
75	95	30	60	40.0	202645	PASS
95	95	100	100	100.0	507050	PASS
96	95	5	9	6.5	32959	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.1	472170	PASS
175	174	5	9	7.1	33314	PASS
176	174	95	101	96.8	457258	PASS
177	176	5	9	6.6	30152	PASS