

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD091020\
 Data File : VD066616.D
 Acq On : 10 Sep 2020 15:15
 Operator : VA/SY
 Sample : L3931-01
 Misc : 5.39G/5.00ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SP-1-1

Quant Time: Sep 11 02:41:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 04 01:57:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.98
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.86
63) Chlorobenzene-d5	0.00	117	0m	50.00	ug/l	-11.64
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.58

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD091020\
Data File : VD066616.D
Acq On : 10 Sep 2020 15:15
Operator : VA/SY
Sample : L3931-01
Misc : 5.39G/5.00ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SP-1-1

Quant Time: Sep 11 02:41:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 04 01:57:04 2020
Response via : Initial Calibration

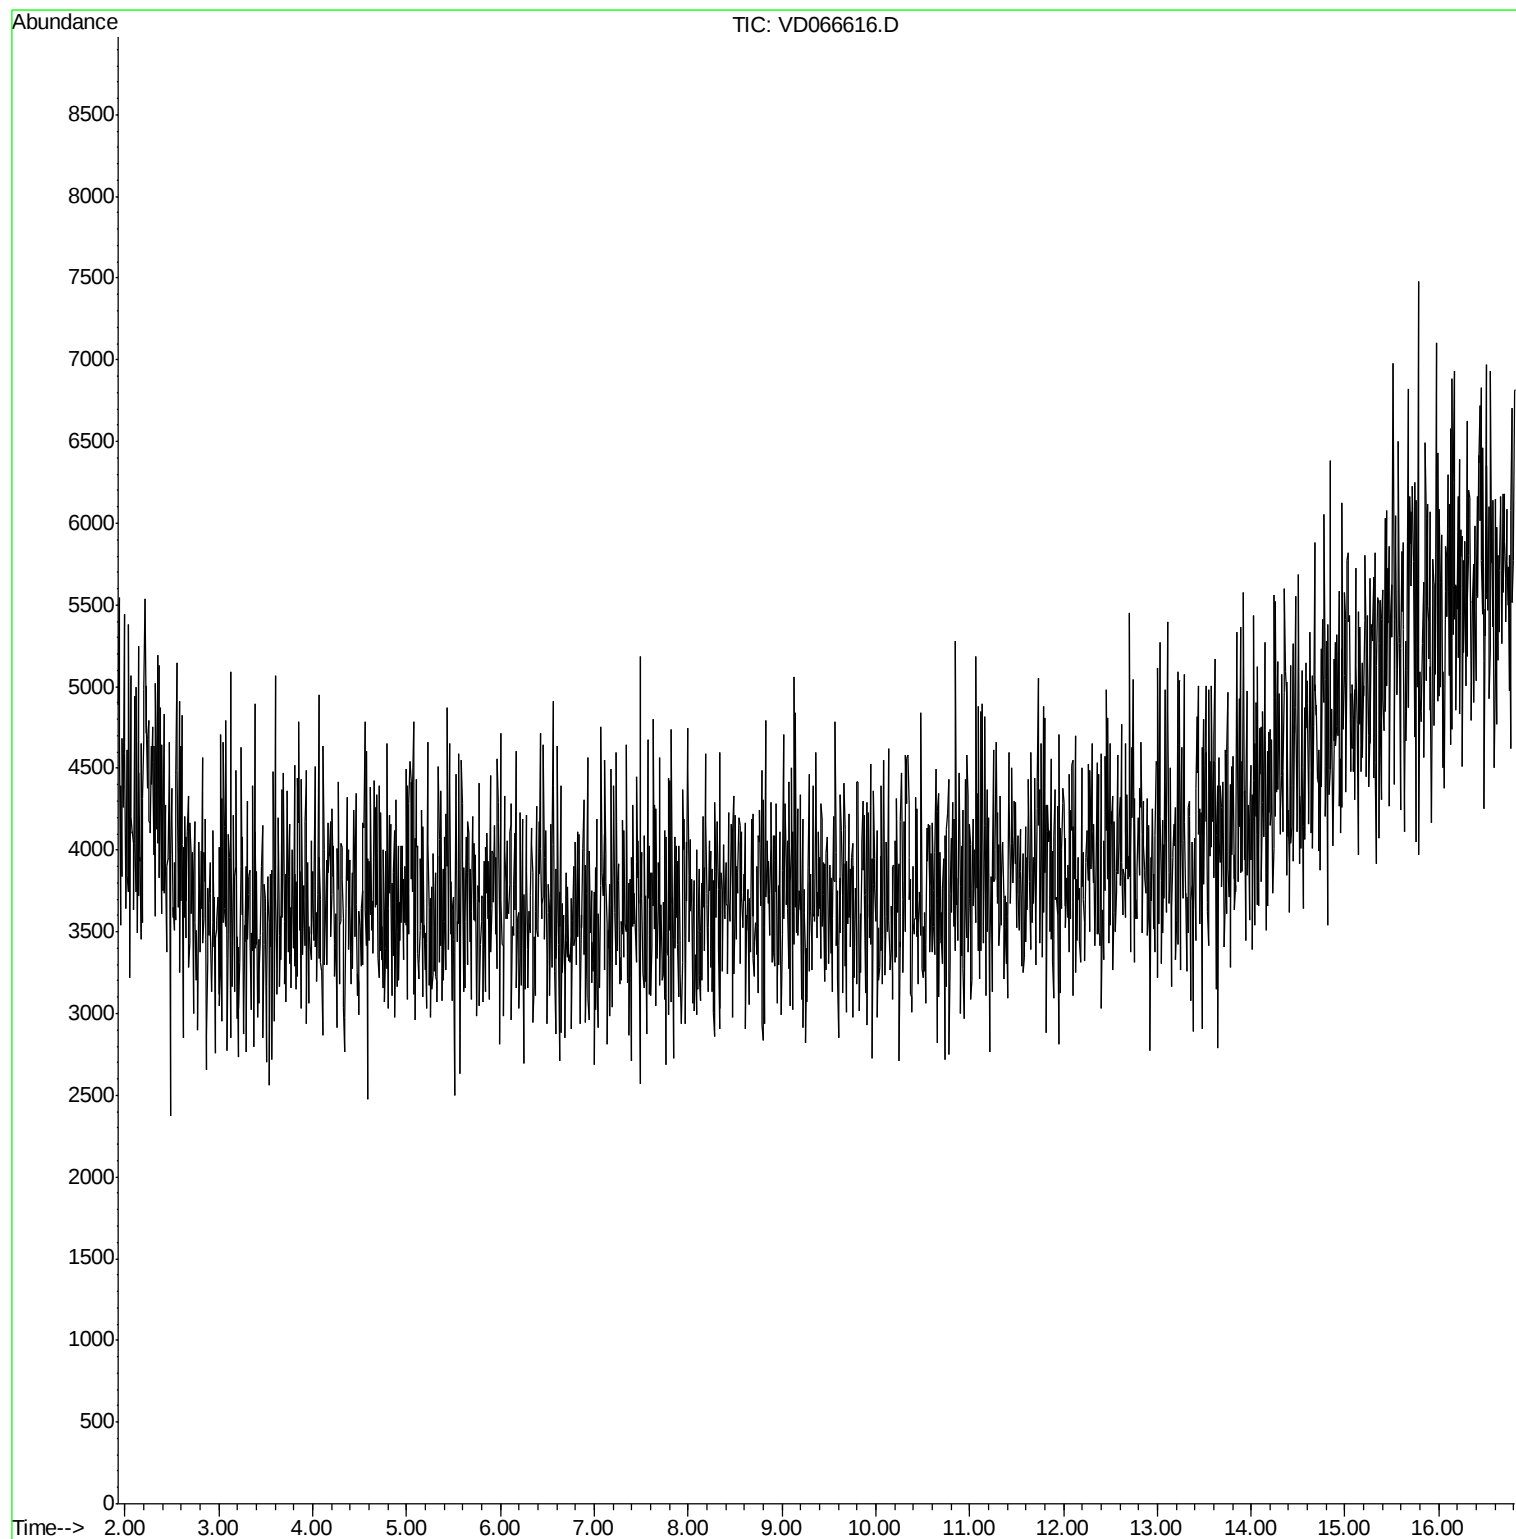

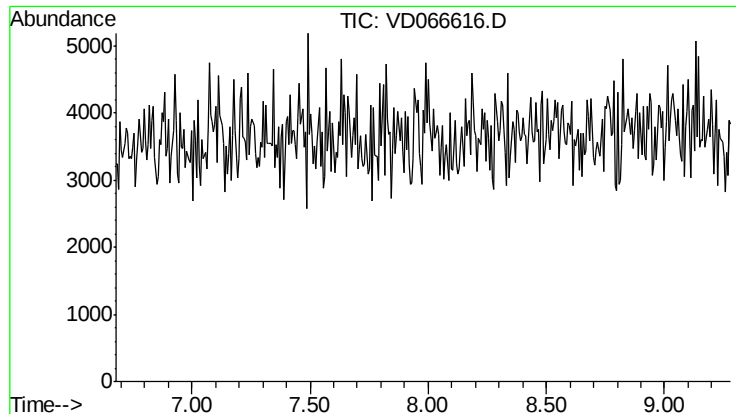

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.98 min

Lab File: VD066616.D

Acq: 10 Sep 2020 15:15

Tot Ion: 168

Sig Exp Ratio

168 100



99 63.1

Instrument :

MSVOA_D

ClientSampleId :

SP-1-1

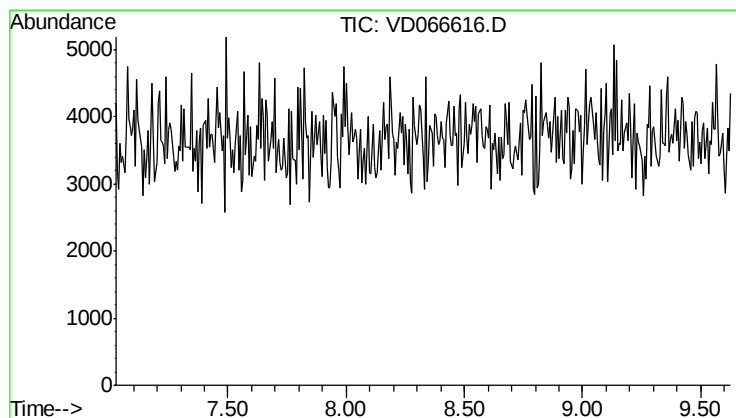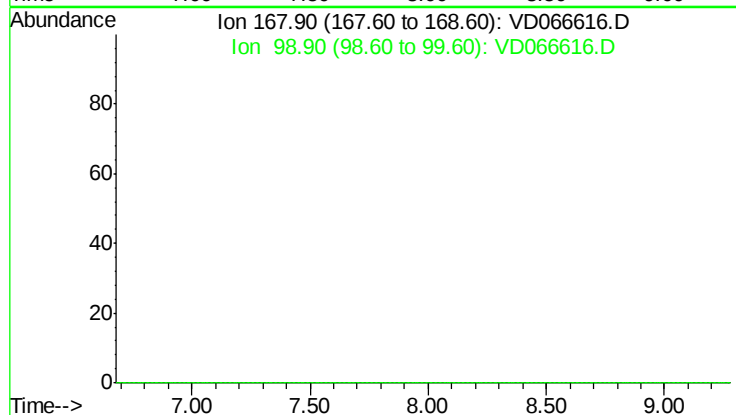

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.33 min

Lab File: VD066616.D


Acq: 10 Sep 2020 15:15


Tgt Ion: 65

Sig Exp Ratio

65 100

67 51.4


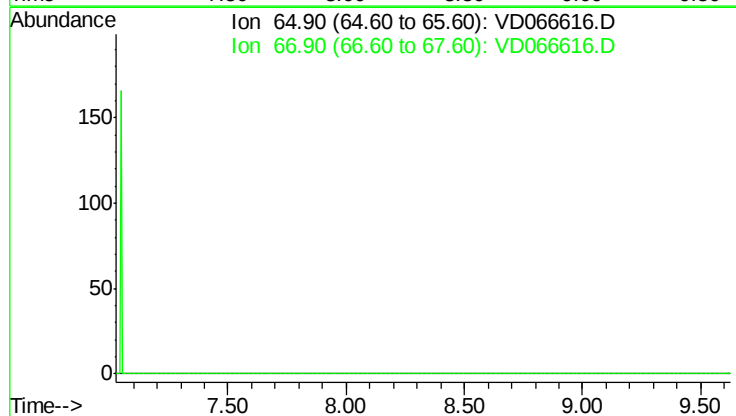


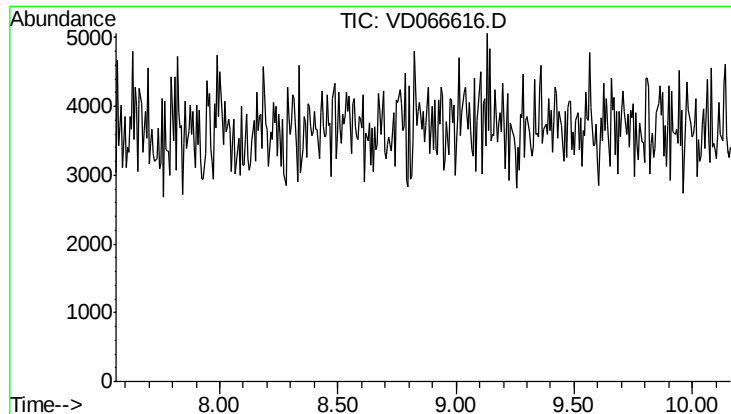

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.86 min
 Lab File: VD066616.D
 Acq: 10 Sep 2020 15:15


Instrument :
 MSVOA_D
 ClientSampleId :
 SP-1-1


Tot Ion	114
Sig	Exp Ratio
114	100
63	21.6
88	16.6

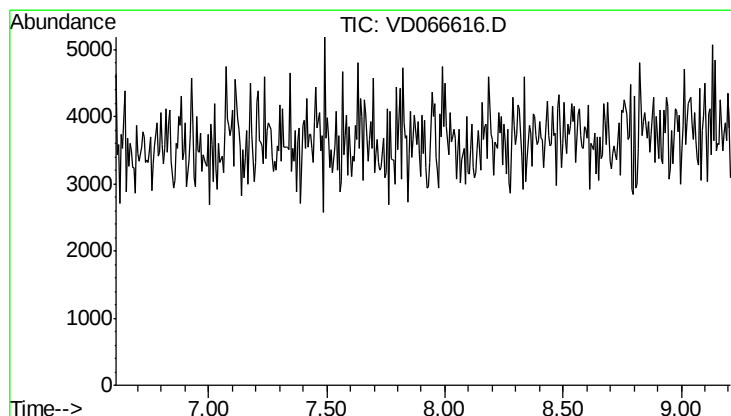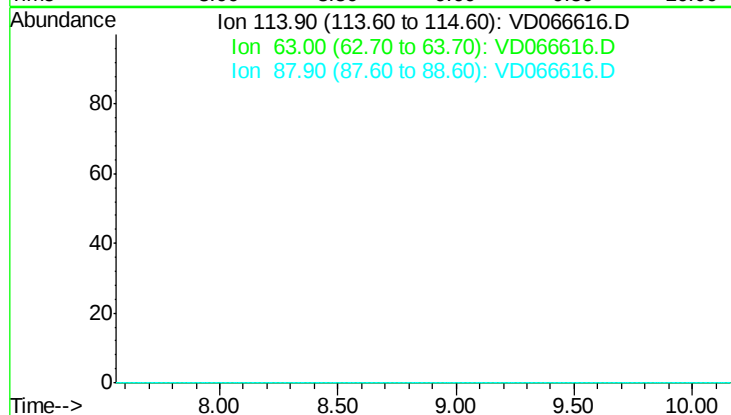

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.91 min
 Lab File: VD066616.D
 Acq: 10 Sep 2020 15:15

Tgt Ion	113
Sig	Exp Ratio
113	100
111	104.0
192	17.1

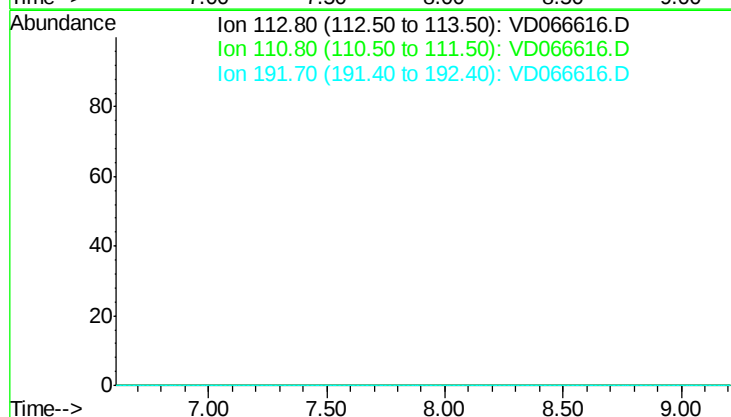


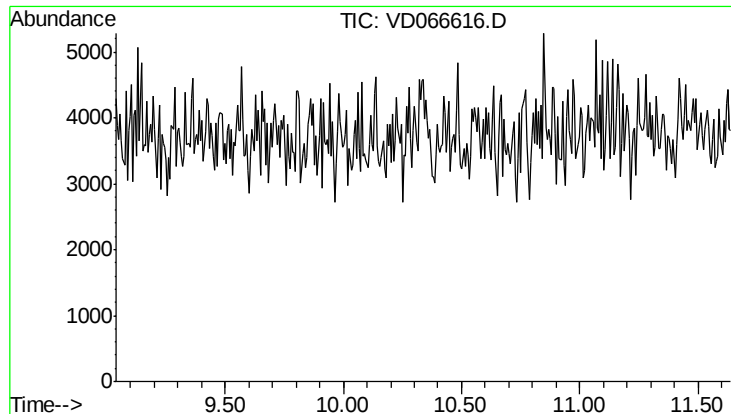


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.34 min

Lab File: VD066616.D
Acq: 10 Sep 2020 15:15

Instrument :
MSVOA_D
ClientSampleId :
SP-1-1


Tot Ion	98
Sig	Exp Ratio
98	100
100	66.1

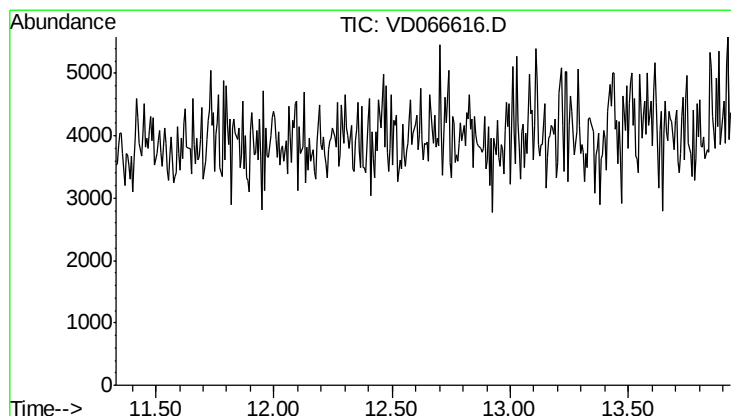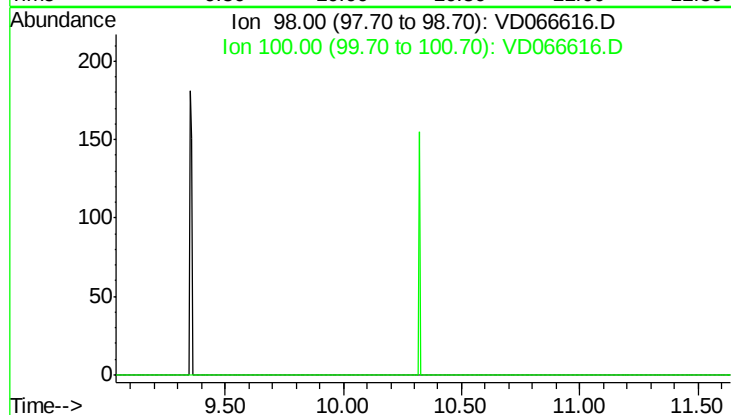


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.63 min

Lab File: VD066616.D
Acq: 10 Sep 2020 15:15

Tgt Ion	95
Sig	Exp Ratio
95	100
174	77.9
176	74.3

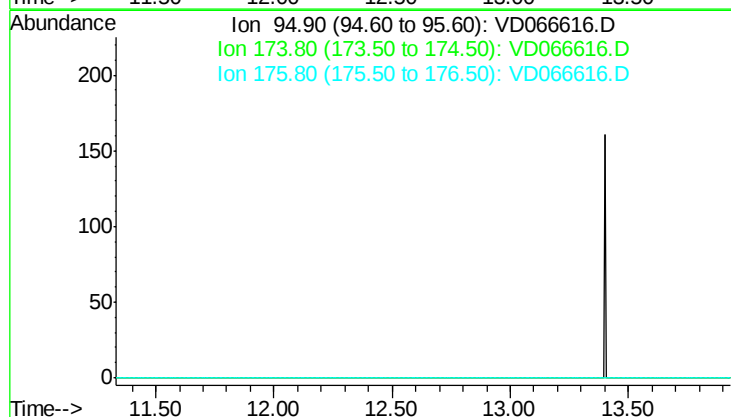


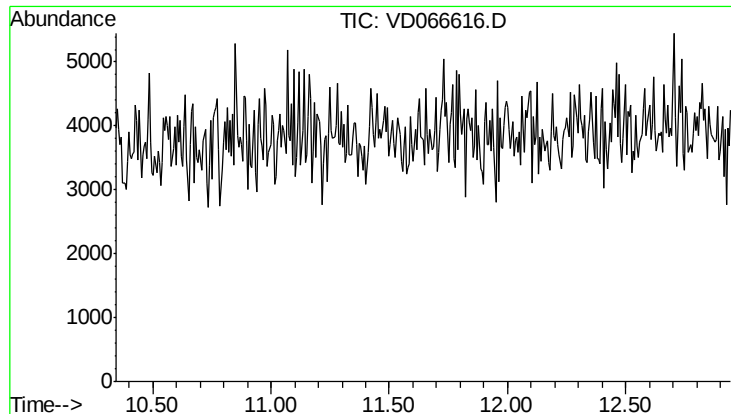


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.64 min

Lab File: VD066616.D
 Acq: 10 Sep 2020 15:15

Instrument :
 MSVOA_D
 ClientSampleId :
 SP-1-1

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 57.7
 119 32.3

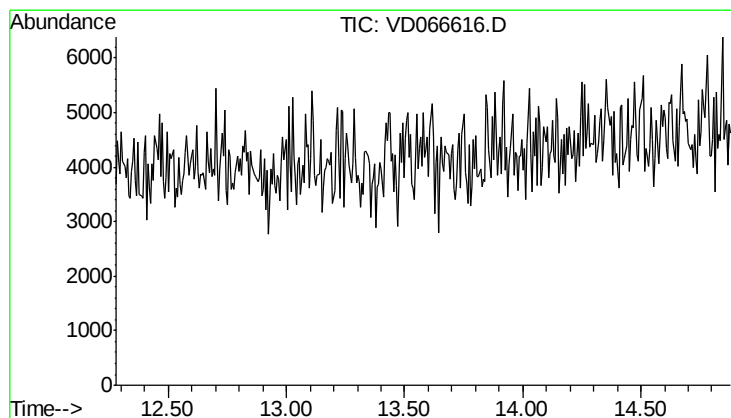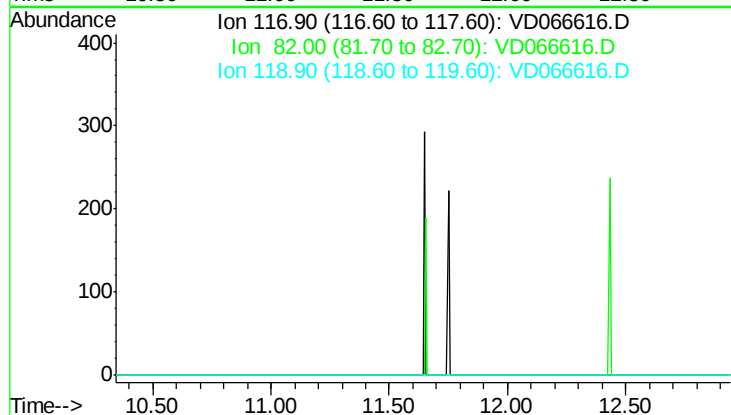

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.58 min

Lab File: VD066616.D
 Acq: 10 Sep 2020 15:15

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 60.8
 150 172.9

