


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD091020\
Data File : VD066607.D
Acq On : 10 Sep 2020 09:27
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Title : SW846 8260
Last Update : Fri Sep 04 01:57:04 2020

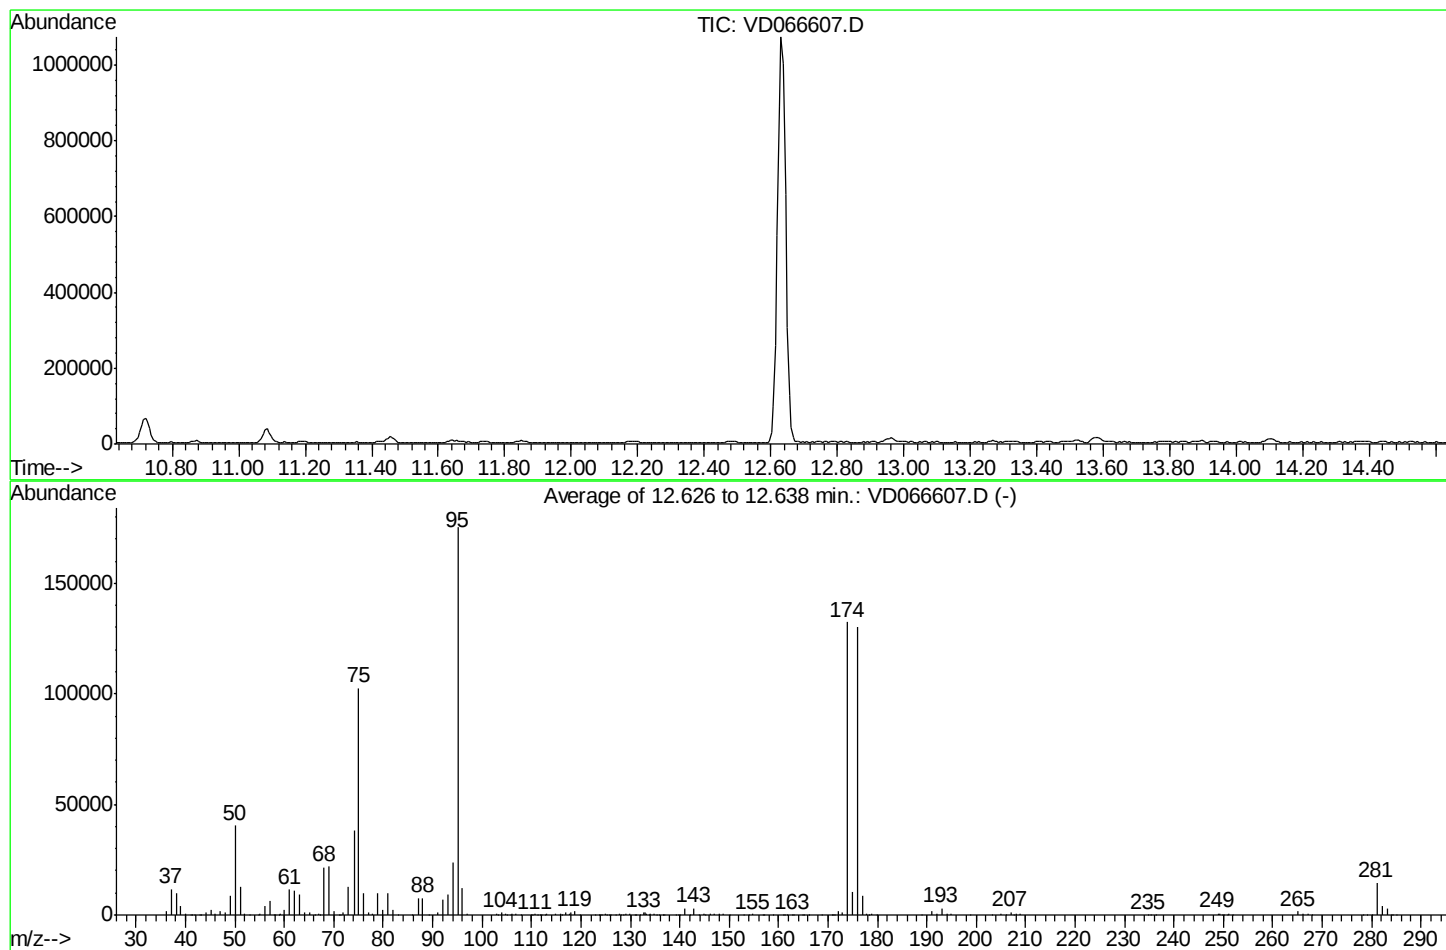

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	40261	PASS
75	95	30	60	58.5	102488	PASS
95	95	100	100	100.0	175296	PASS
96	95	5	9	7.0	12248	PASS
173	174	0.00	2	1.0	1298	PASS
174	95	50	100	75.5	132280	PASS
175	174	5	9	7.9	10444	PASS
176	174	95	101	98.4	130165	PASS
177	176	5	9	6.6	8592	PASS