

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091021\
 Data File : VD070311.D
 Acq On : 10 Sep 2021 20:36
 Operator : VA/SY
 Sample : M3684-12
 Misc : 5.91G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 F005130

Quant Time: Sep 11 02:29:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 09 03:07:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	248389	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	606801	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	720374	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	300894	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	219404	68.792	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	137.580%
35) Dibromofluoromethane	7.914	113	232866	53.913	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.820%
50) Toluene-d8	10.338	98	852785	54.379	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.760%
62) 4-Bromofluorobenzene	12.626	95	311044	56.752	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	113.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091021\
Data File : VD070311.D
Acq On : 10 Sep 2021 20:36
Operator : VA/SY
Sample : M3684-12
Misc : 5.91G/5.00ml/MSVOA_D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
F005130

Quant Time: Sep 11 02:29:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Quant Title : SW846 8260
QLast Update : Thu Sep 09 03:07:09 2021
Response via : Initial Calibration




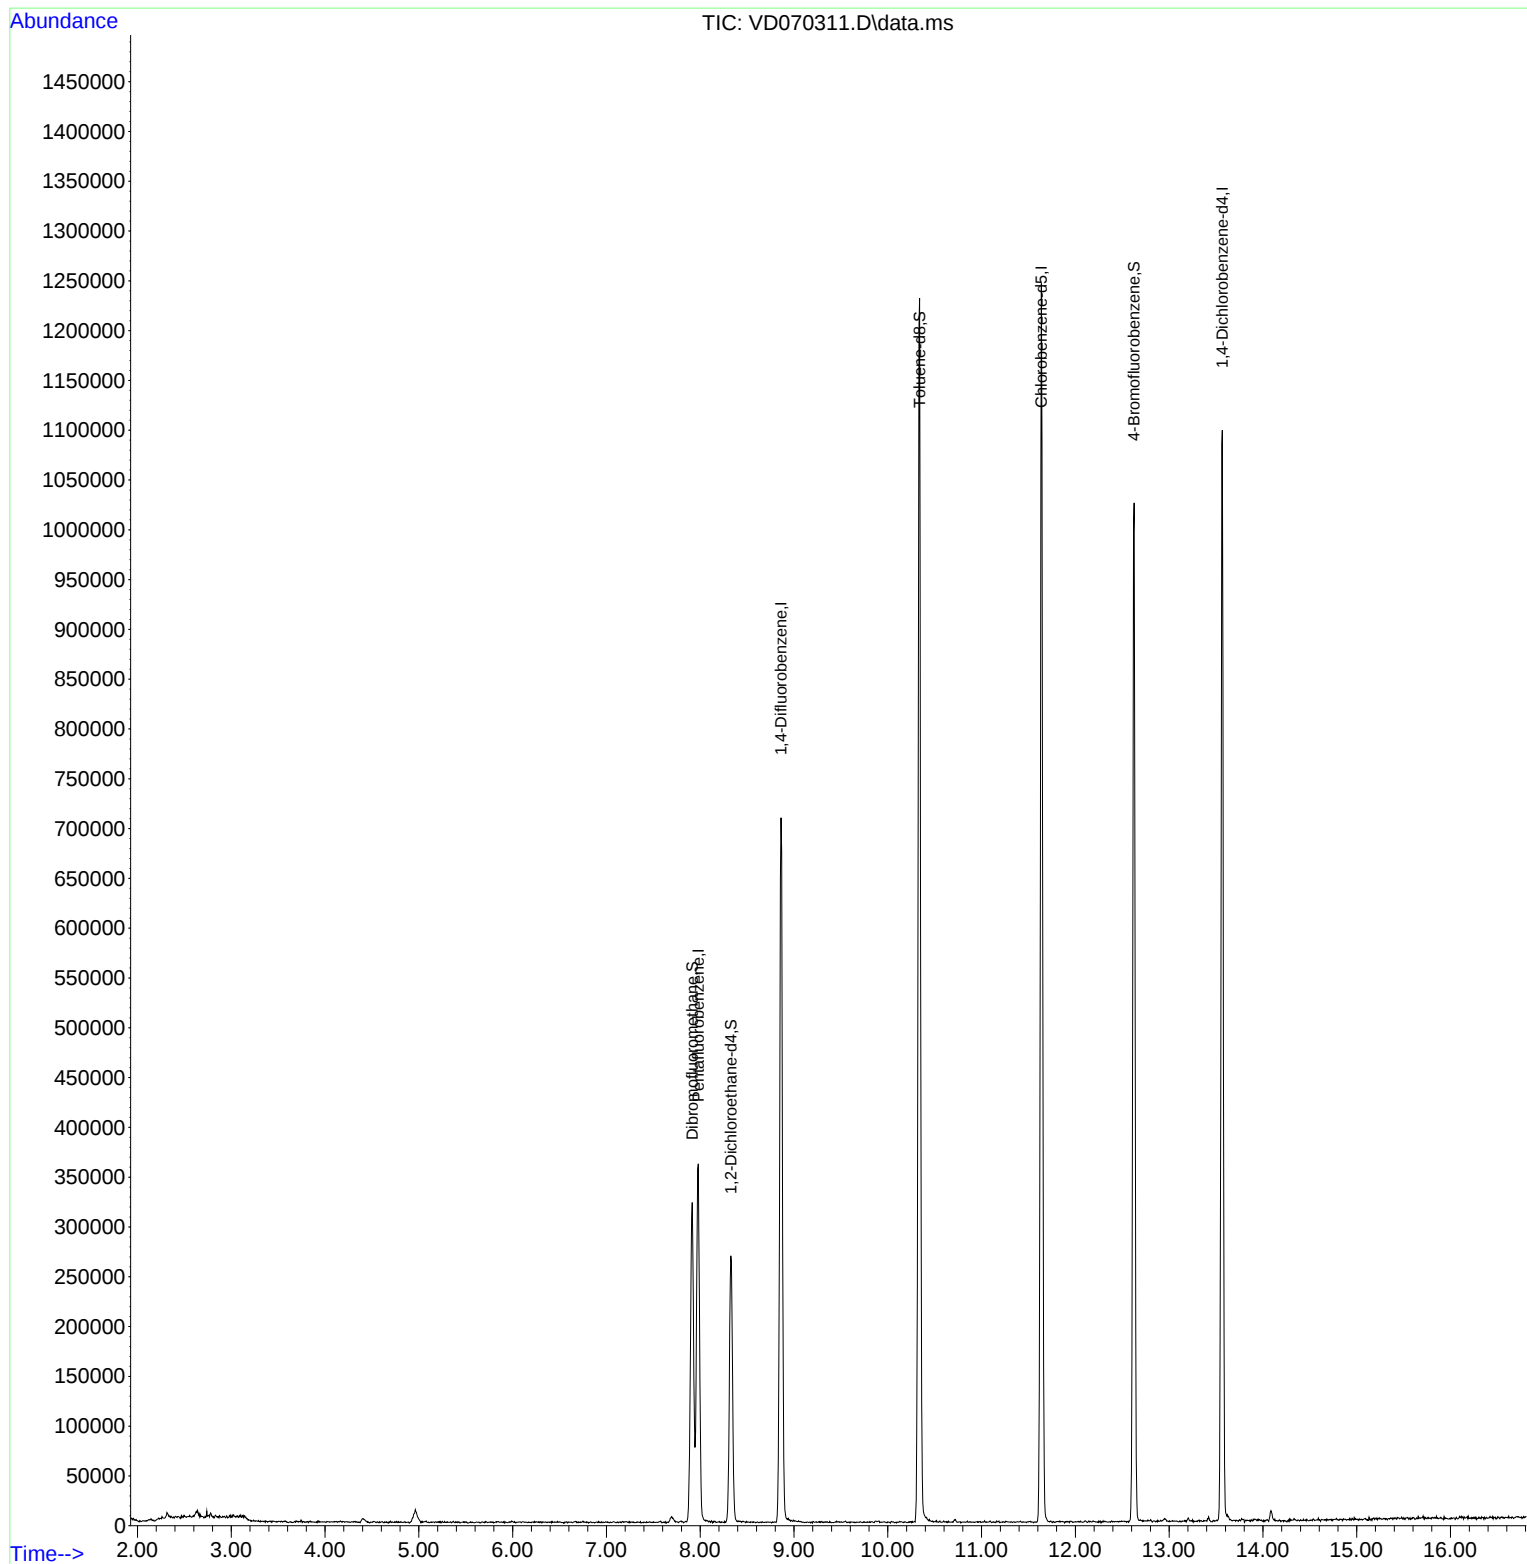


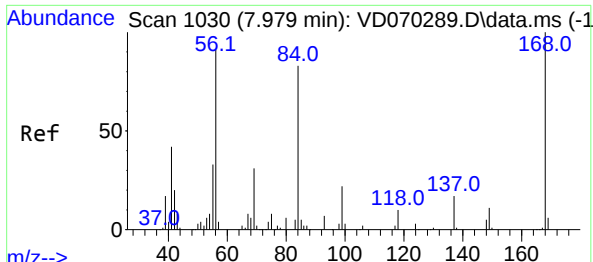

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36




Instrument :
MSVOA_D
ClientSampleId :
F005130


Tgt Ion:168 Resp: 248389
Ion Ratio Lower Upper
168 100
99 62.3 50.8 76.2

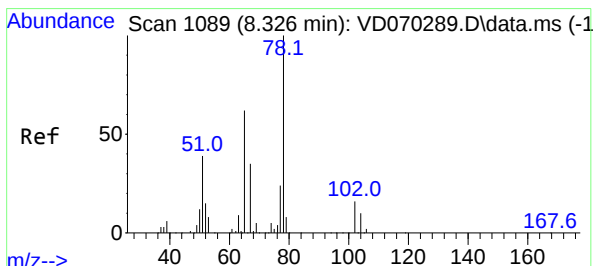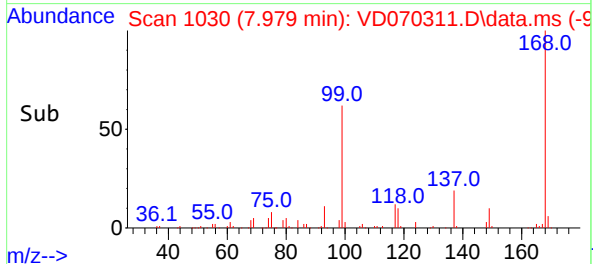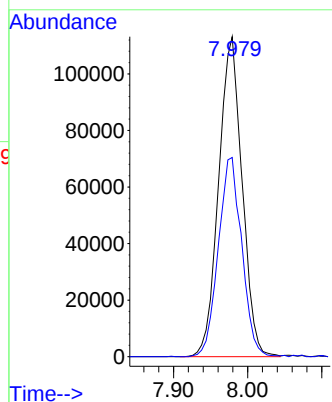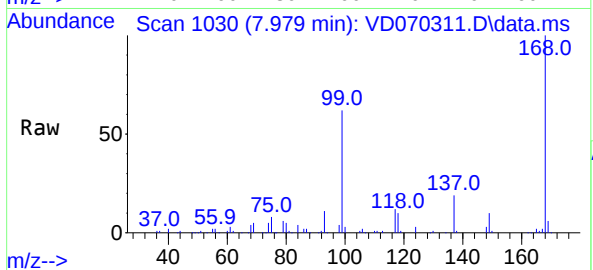

#33
1,2-Dichloroethane-d4
Concen: 68.792 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36

Tgt Ion: 65 Resp: 219404
Ion Ratio Lower Upper
65 100
67 55.1 0.0 111.4

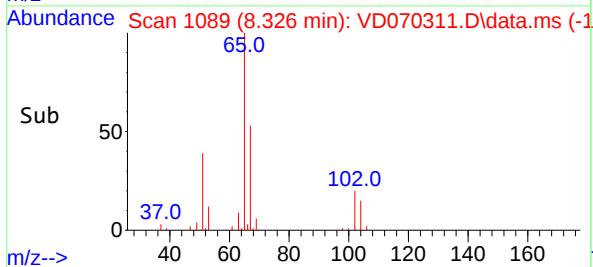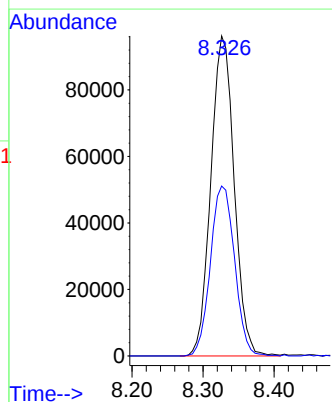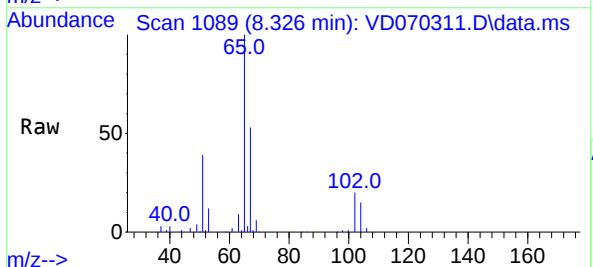

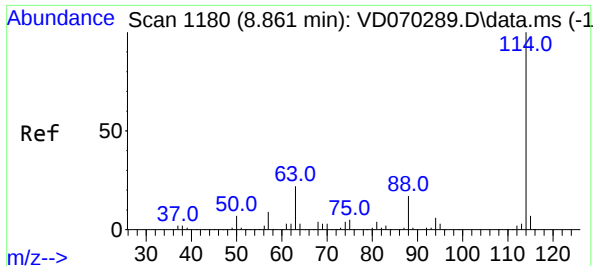





#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36

Instrument :
MSVOA_D
ClientSampleId :
F005130

Tgt Ion:114 Resp: 606801

Ion	Ratio	Lower	Upper
114	100		
63	20.6	0.0	43.4
88	16.4	0.0	33.4

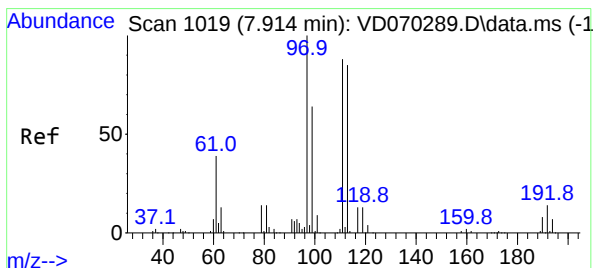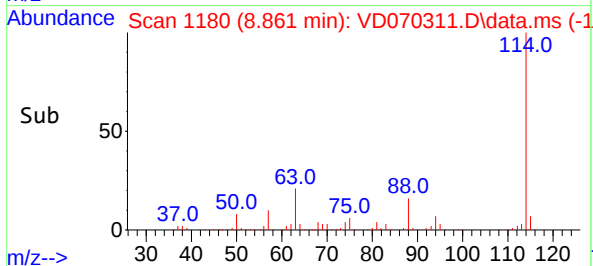
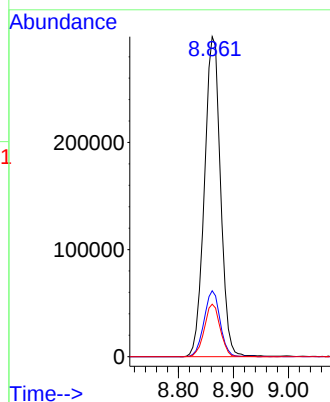
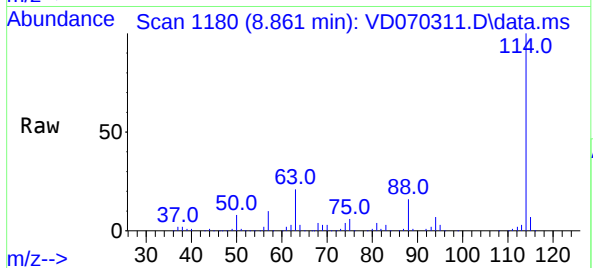



#35

Dibromofluoromethane
Concen: 53.913 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36

Tgt Ion:113 Resp: 232866

Ion	Ratio	Lower	Upper
113	100		
111	102.9	81.4	122.2
192	17.1	13.0	19.6


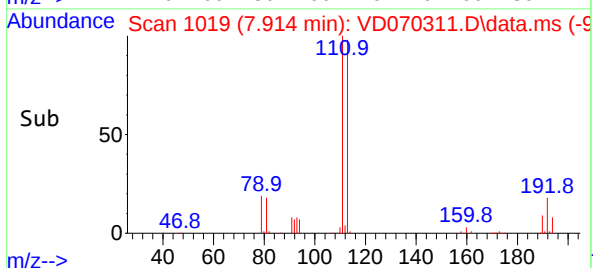
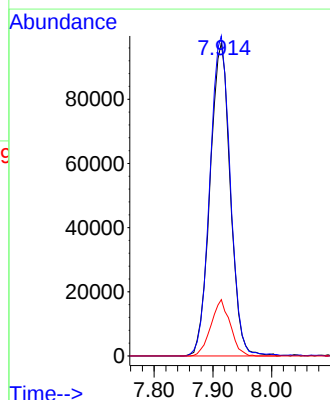
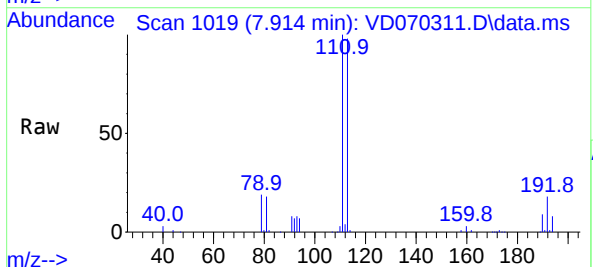


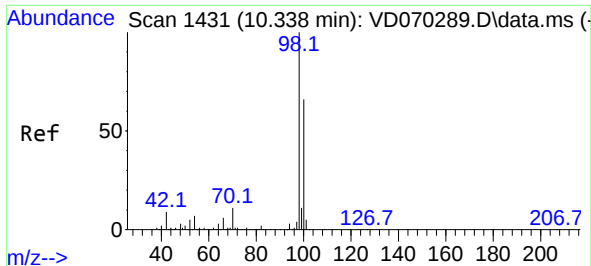

#50
Toluene-d8
Concen: 54.379 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36




Instrument :
MSVOA_D
ClientSampleId :
F005130


Tgt Ion: 98 Resp: 852785
Ion Ratio Lower Upper
98 100
100 63.3 52.0 78.0

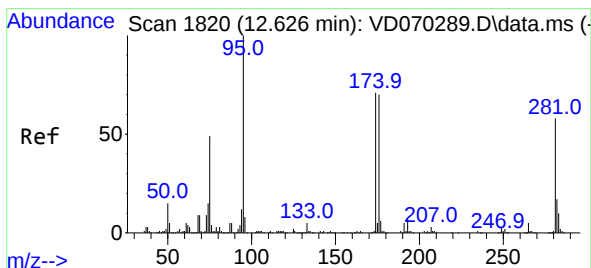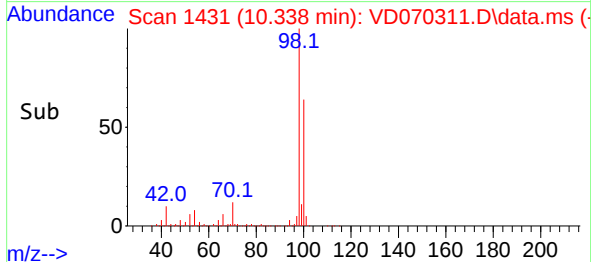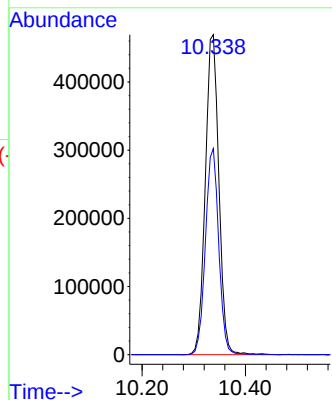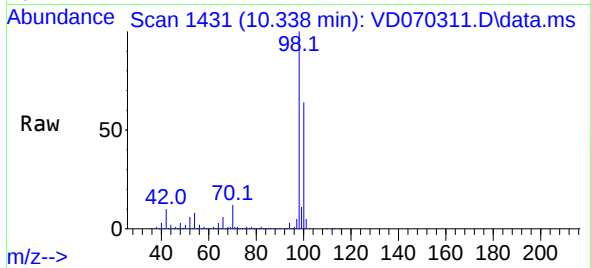

#62
4-Bromofluorobenzene
Concen: 56.752 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36

Tgt Ion: 95 Resp: 311044
Ion Ratio Lower Upper
95 100
174 72.3 0.0 140.6
176 70.1 0.0 137.4


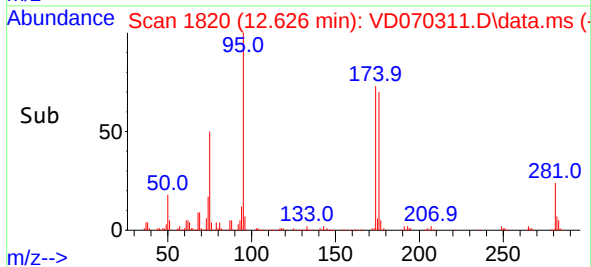
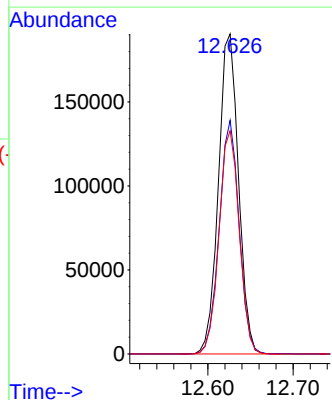
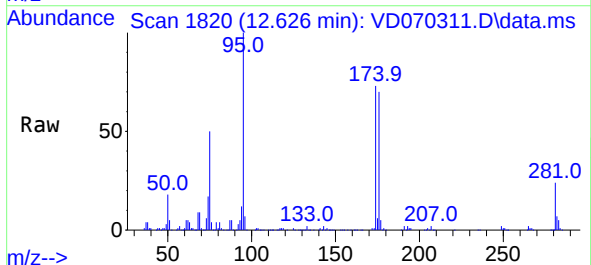


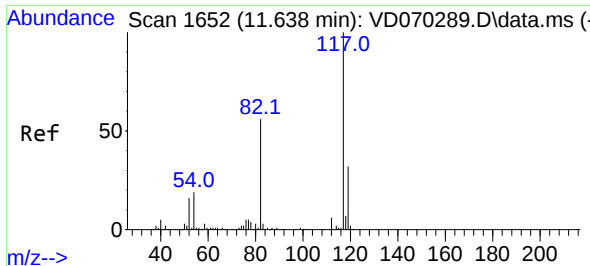

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36

Instrument :
MSVOA_D
ClientSampleId :
F005130

Tgt Ion:	117	Resp:	720374
Ion	Ratio	Lower	Upper
117	100		
82	56.3	45.0	67.4
119	31.9	25.2	37.8

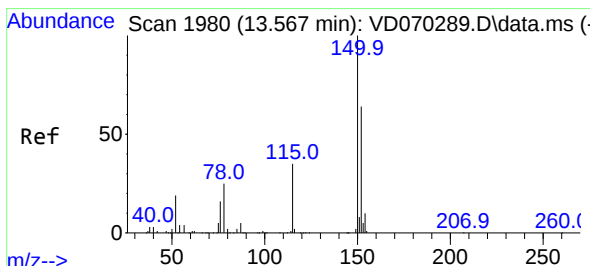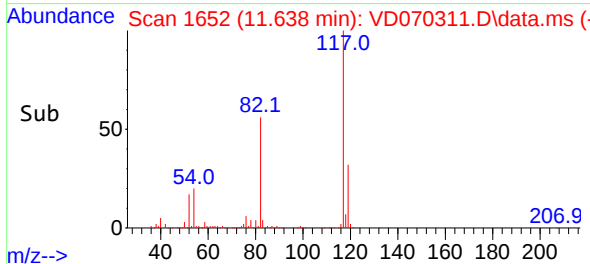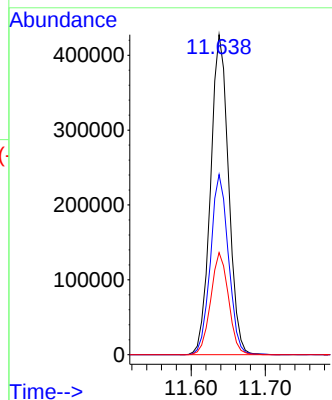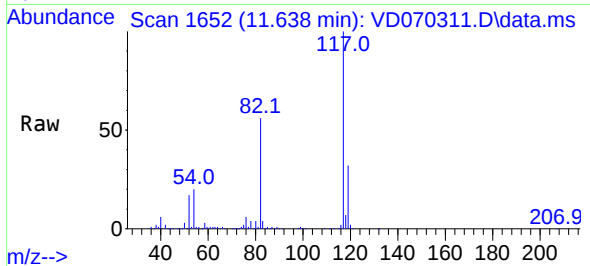

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD070311.D
Acq: 10 Sep 2021 20:36

Tgt Ion:	152	Resp:	300894
Ion	Ratio	Lower	Upper
152	100		
115	62.0	32.1	96.3
150	156.0	0.0	350.6

