
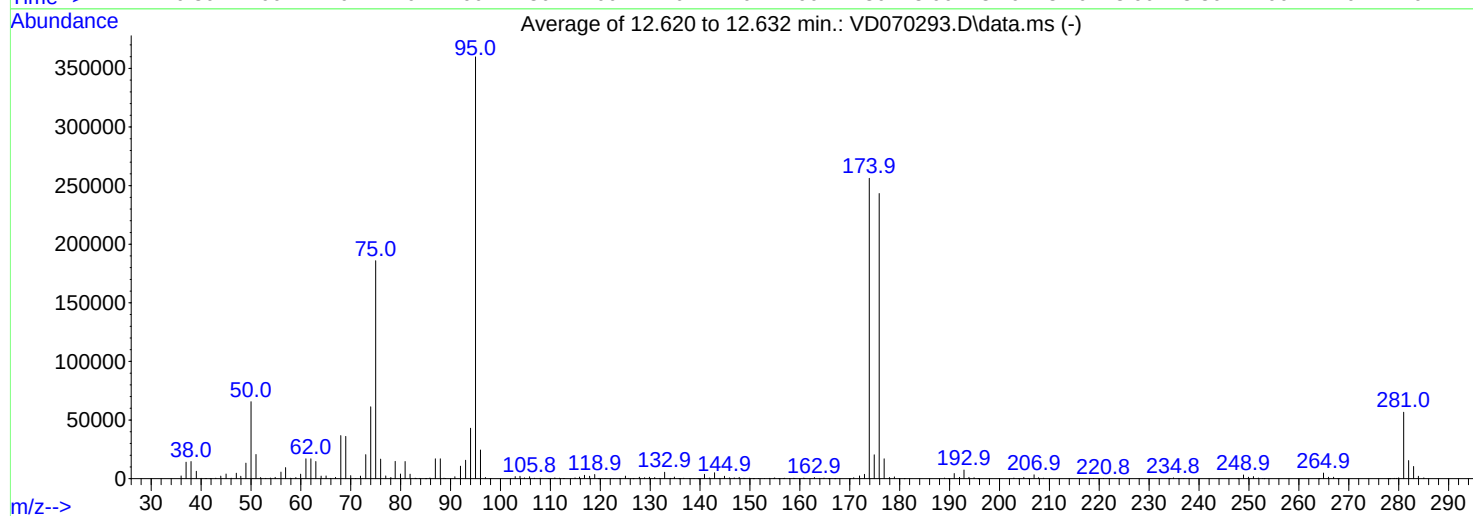


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD091021\  
 Data File : VD070293.D  
 Acq On : 10 Sep 2021 11:49  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D090821S.M  
 Title : SW846 8260  
 Last Update : Thu Sep 09 03:07:09 2021

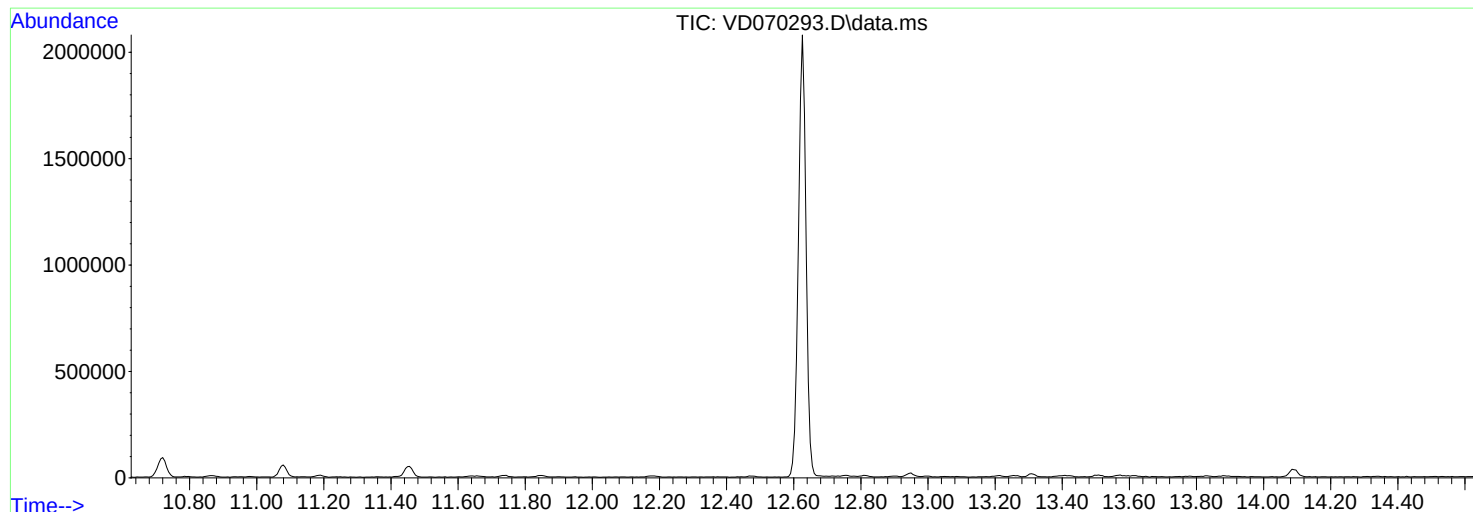

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.2         | 65619      | PASS                |
| 75             | 95              | 30              | 60              | 51.7         | 185941     | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 359851     | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 24499      | PASS                |
| 173            | 174             | 0.00            | 2               | 1.5          | 3744       | PASS                |
| 174            | 95              | 50              | 100             | 71.2         | 256256     | PASS                |
| 175            | 174             | 5               | 9               | 7.9          | 20315      | PASS                |
| 176            | 174             | 95              | 101             | 94.9         | 243285     | PASS                |
| 177            | 176             | 5               | 9               | 6.9          | 16882      | PASS                |