


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD091120\
Data File : VD066641.D
Acq On : 11 Sep 2020 10:55
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Title : SW846 8260
Last Update : Fri Sep 04 01:57:04 2020

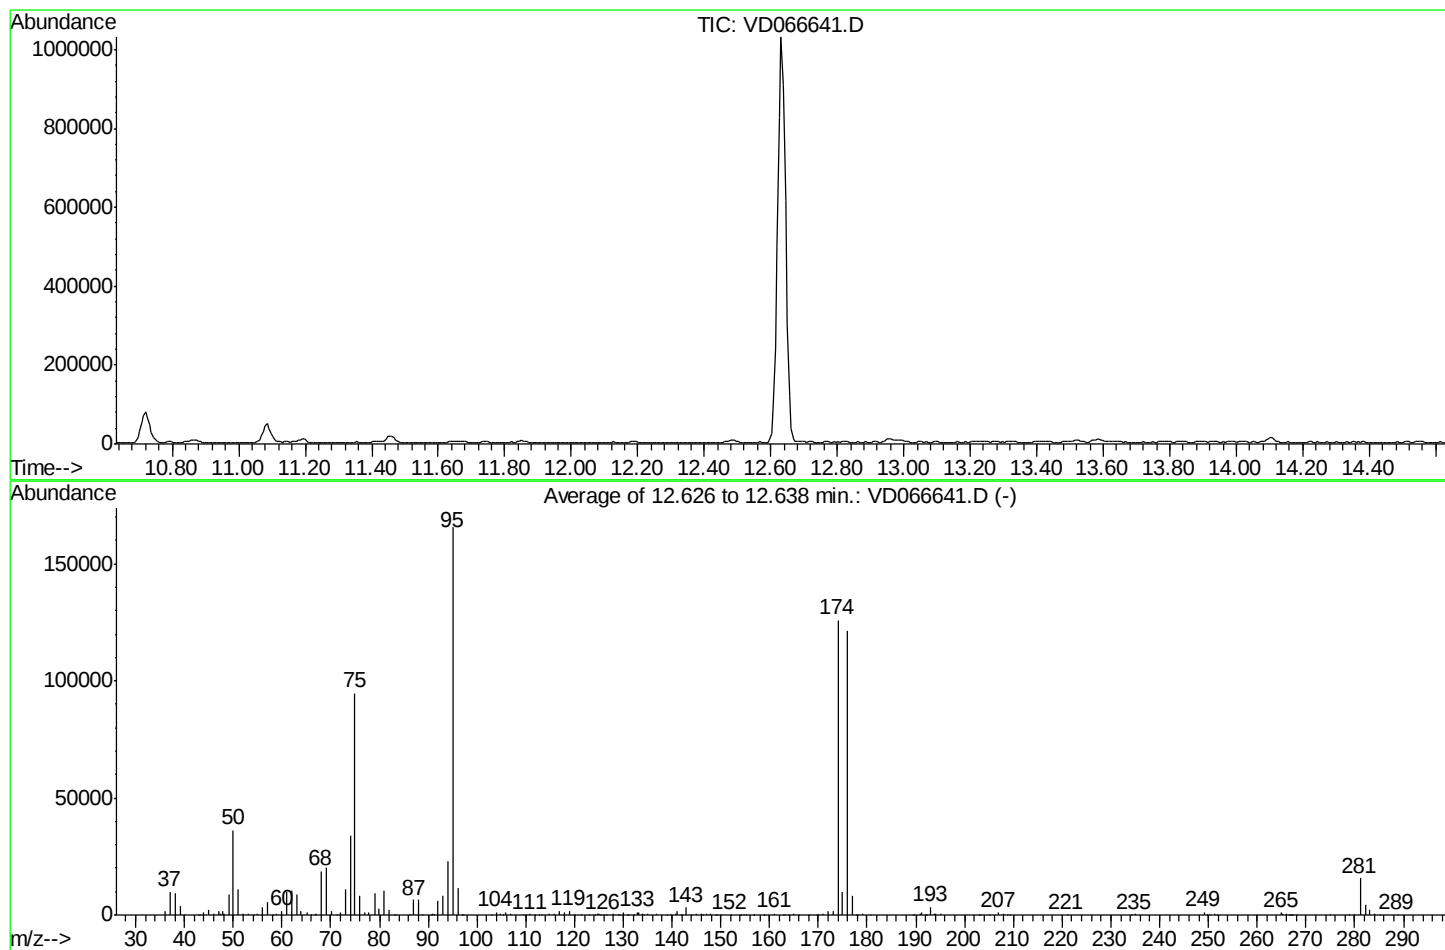

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	36093	PASS
75	95	30	60	57.2	94693	PASS
95	95	100	100	100.0	165568	PASS
96	95	5	9	7.0	11588	PASS
173	174	0.00	2	1.4	1823	PASS
174	95	50	100	76.1	126018	PASS
175	174	5	9	7.7	9721	PASS
176	174	95	101	96.2	121272	PASS
177	176	5	9	6.6	7992	PASS