
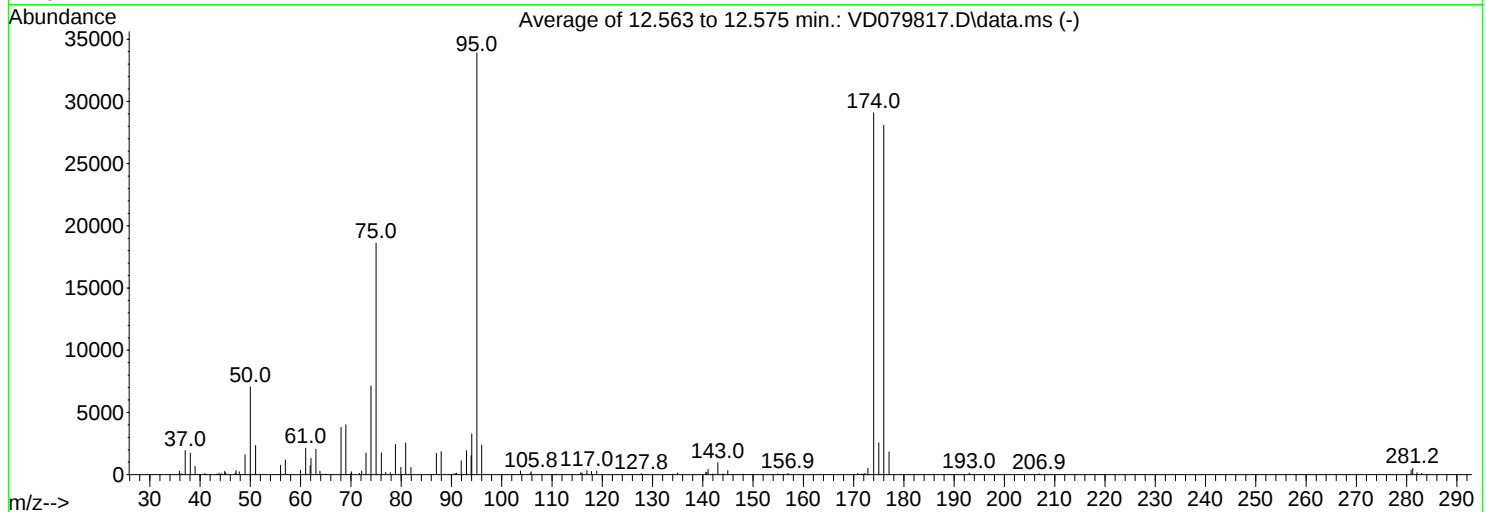


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091124\
Data File : VD079817.D
Acq On : 11 Sep 2024 09:12
Operator : RP/MD
Sample : BFB826
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB826

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Thu Sep 12 01:25:24 2024

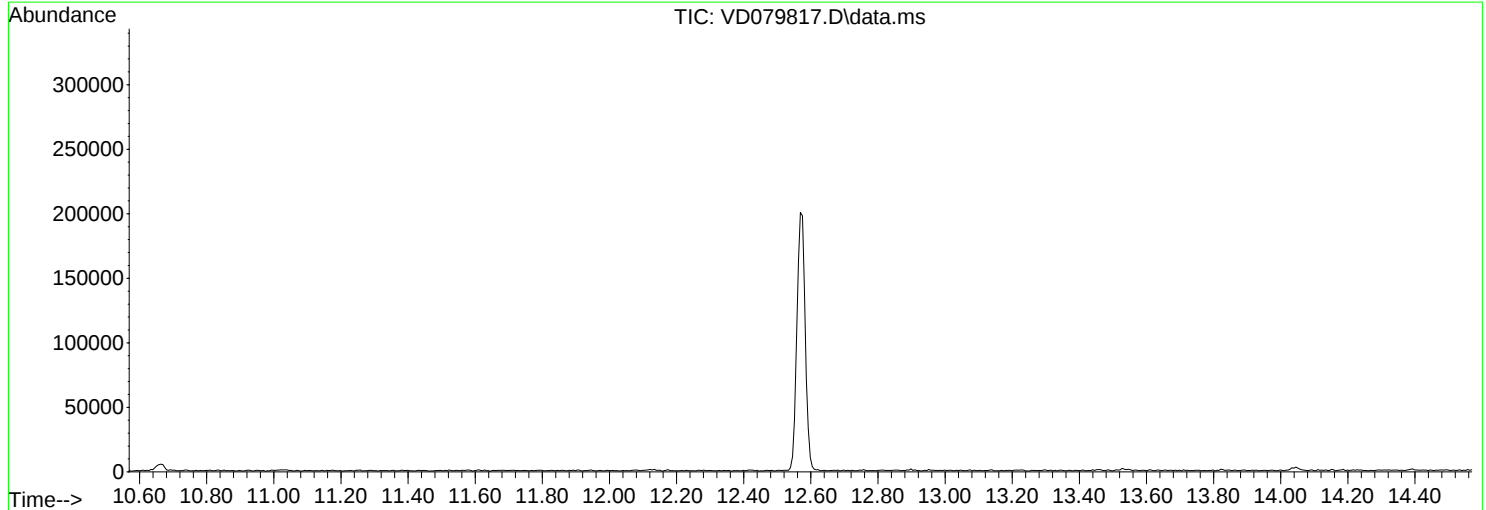

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.8	7065	PASS
75	95	30	80	54.9	18605	PASS
95	95	100	100	100.0	33904	PASS
96	95	5	9	7.0	2378	PASS
173	174	0.00	2	1.7	502	PASS
174	95	50	120	85.8	29088	PASS
175	174	5	9	8.8	2565	PASS
176	174	95	105	96.5	28075	PASS
177	176	5	10	6.5	1831	PASS

m/z	Abundance
35.50	177.0
39.90	655.0
43.70	206.0
44.10	188.0

Instrument :
MSVOA_D
ClientSampleId :
BFB826

m/z	Abundance
36.20	248.0
37.00	1309.0
38.00	1681.0
39.00	480.0
39.90	716.0
40.90	155.0
43.90	484.0
44.90	293.0
47.00	375.0
47.90	165.0
48.90	1400.0
50.00	5985.0
51.10	1993.0
52.00	173.0
56.00	653.0
57.00	667.0
60.00	361.0
61.00	1863.0
61.90	2169.0
63.10	2035.0
63.80	410.0
68.00	3212.0
69.00	3504.0
71.70	307.0
72.20	285.0
73.00	1714.0
74.00	6231.0
75.00	17096.0
76.10	1495.0
77.90	300.0
78.80	2017.0
79.90	365.0
80.90	1914.0
81.90	701.0
87.00	1185.0
88.00	1424.0
90.80	218.0
92.00	1094.0
93.00	1568.0
93.90	4538.0
95.00	30736.0
96.00	1991.0
103.80	348.0
105.70	256.0
115.80	244.0
117.00	338.0
117.80	276.0
118.90	245.0
134.90	154.0
140.60	576.0
141.10	411.0
141.90	171.0
142.90	808.0
144.90	364.0
172.10	255.0
173.00	534.0
174.00	24528.0
175.00	2289.0
176.00	23632.0
177.00	1441.0
280.90	573.0
283.00	156.0

Instrument :
MSVOA_D
ClientSampleId :
BFB826

m/z	Abundance
35.90	487.0
37.10	2353.0
38.00	1875.0
39.10	786.0
39.90	670.0
41.10	186.0
43.30	154.0
44.10	530.0
45.10	451.0
47.20	291.0
49.00	1832.0
50.00	7763.0
51.00	2880.0
56.00	985.0
57.00	1424.0
60.00	284.0
61.00	2209.0
62.10	2050.0
63.00	1819.0
63.90	447.0
68.00	4215.0
69.00	4522.0
69.90	245.0
70.20	241.0
72.10	260.0
73.00	1886.0
74.00	7023.0
75.00	19616.0
76.00	1947.0
76.90	216.0
78.90	2884.0
80.00	606.0
80.90	3038.0
82.00	546.0
87.00	2155.0
87.90	2064.0
91.00	333.0
91.90	1227.0
93.00	2401.0
94.10	5351.0
95.00	35816.0
96.00	2768.0
103.80	304.0
105.90	390.0
110.80	167.0
116.00	375.0
117.00	382.0
117.90	181.0
118.90	458.0
140.80	542.0
143.00	1111.0
145.00	289.0
156.90	169.0
170.80	296.0
171.60	153.0
172.30	227.0
174.00	32520.0
175.00	2577.0
176.00	28680.0
177.00	1951.0
193.00	208.0
280.90	556.0
281.20	495.0
282.00	307.0

Instrument :
MSVOA_D
ClientSampleId :
BFB826

m/z	Abundance
35.90	367.0
37.00	2146.0
38.10	1648.0
38.90	743.0
40.00	601.0
43.80	494.0
44.30	263.0
44.90	515.0
47.10	720.0
47.80	525.0
49.00	1585.0
50.00	7448.0
51.00	2148.0
56.00	653.0
56.90	1446.0
60.00	385.0
61.00	2313.0
62.00	1899.0
63.00	2277.0
64.10	175.0
65.00	153.0
68.10	3979.0
69.00	4008.0
70.10	454.0
72.10	307.0
73.00	1648.0
74.00	8140.0
75.00	19104.0
76.00	1776.0
76.90	367.0
77.80	174.0
78.90	2347.0
80.00	799.0
80.90	2682.0
81.90	508.0
87.00	1789.0
88.00	2063.0
90.50	192.0
92.00	1036.0
93.00	1813.0
94.00	4453.0
95.10	35160.0
96.00	2376.0
103.60	258.0
105.80	353.0
115.70	235.0
116.80	277.0
117.90	302.0
119.00	159.0
127.80	241.0
135.00	220.0
141.00	871.0
143.10	985.0
144.00	181.0
144.90	302.0
148.00	169.0
154.90	197.0
157.00	155.0
172.80	971.0
174.00	30216.0
175.00	2828.0
176.00	31912.0
177.10	2101.0
193.00	184.0
206.90	236.0
281.20	1043.0
282.10	192.0
282.90	152.0

Instrument :
MSVOA_D
ClientSampleId :
BFB826