




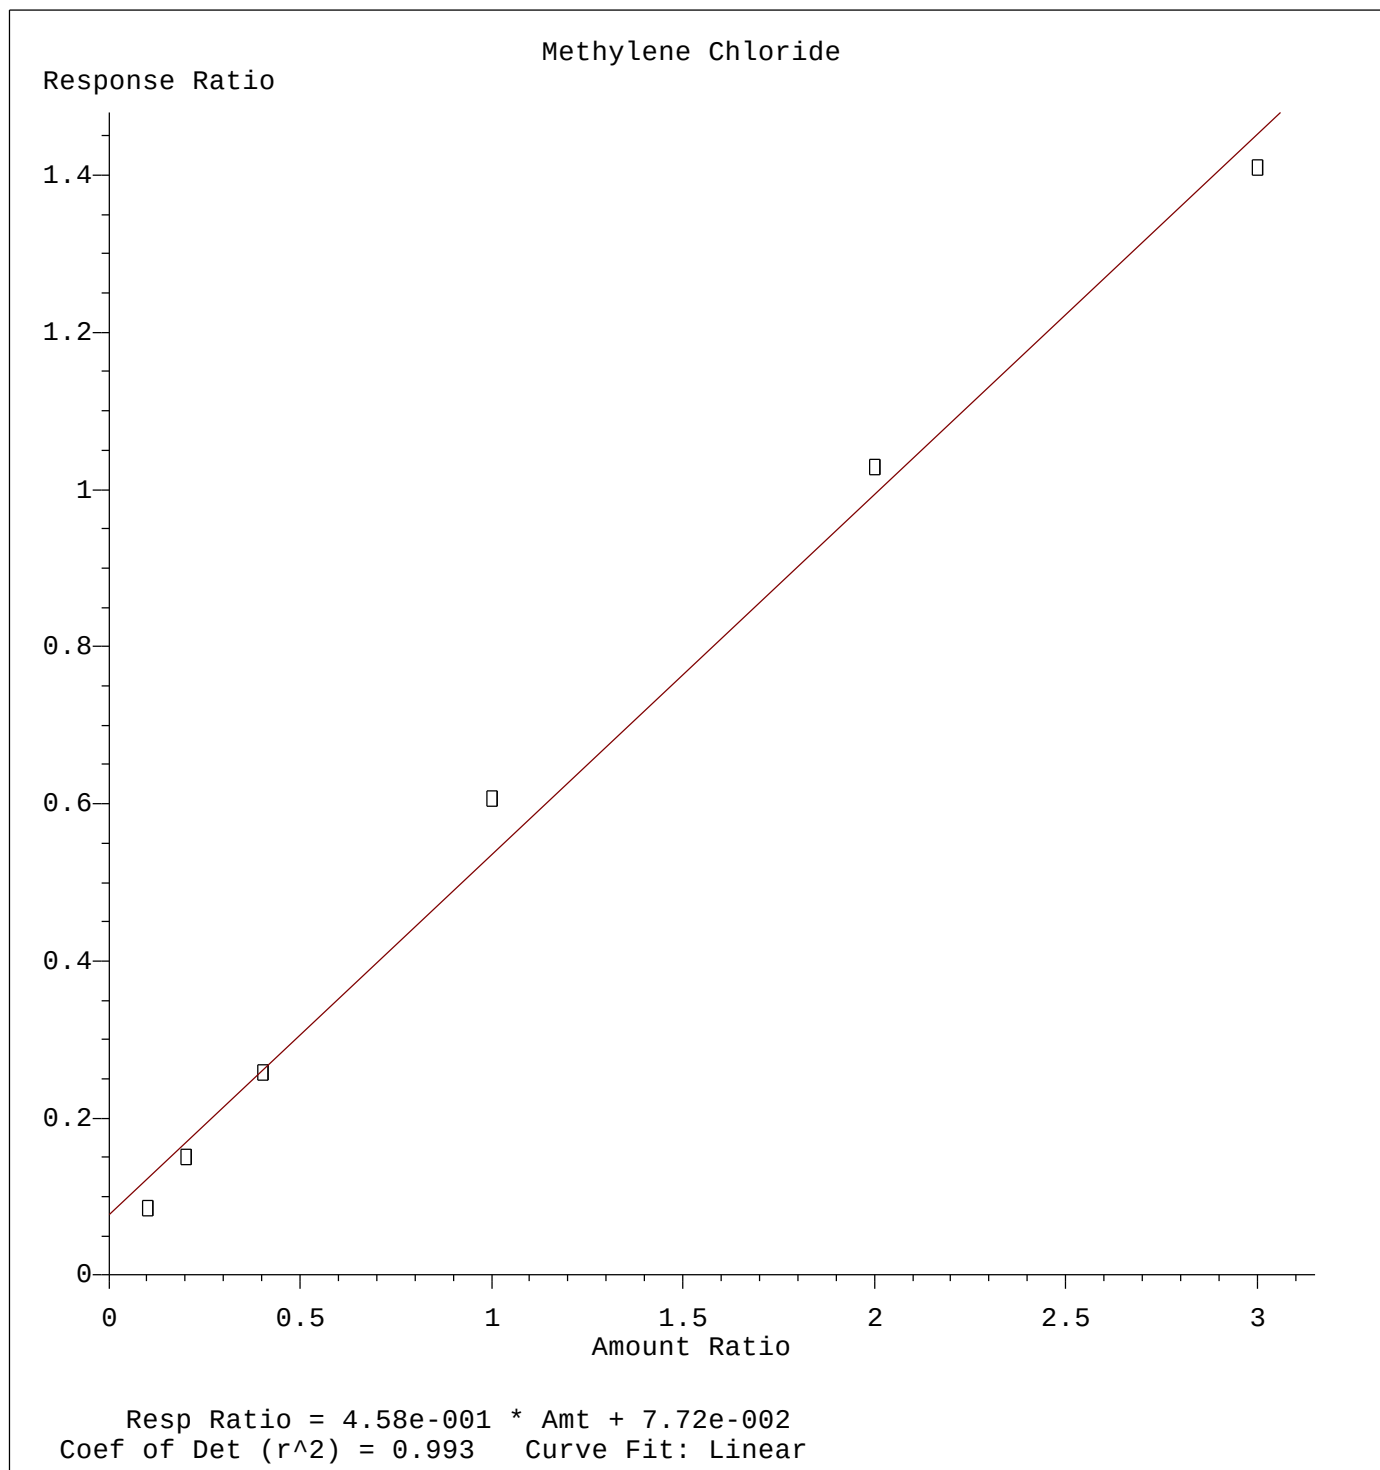

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D091318S.M  
Calibration Table Last Updated: Fri Sep 14 14:53:27 2018

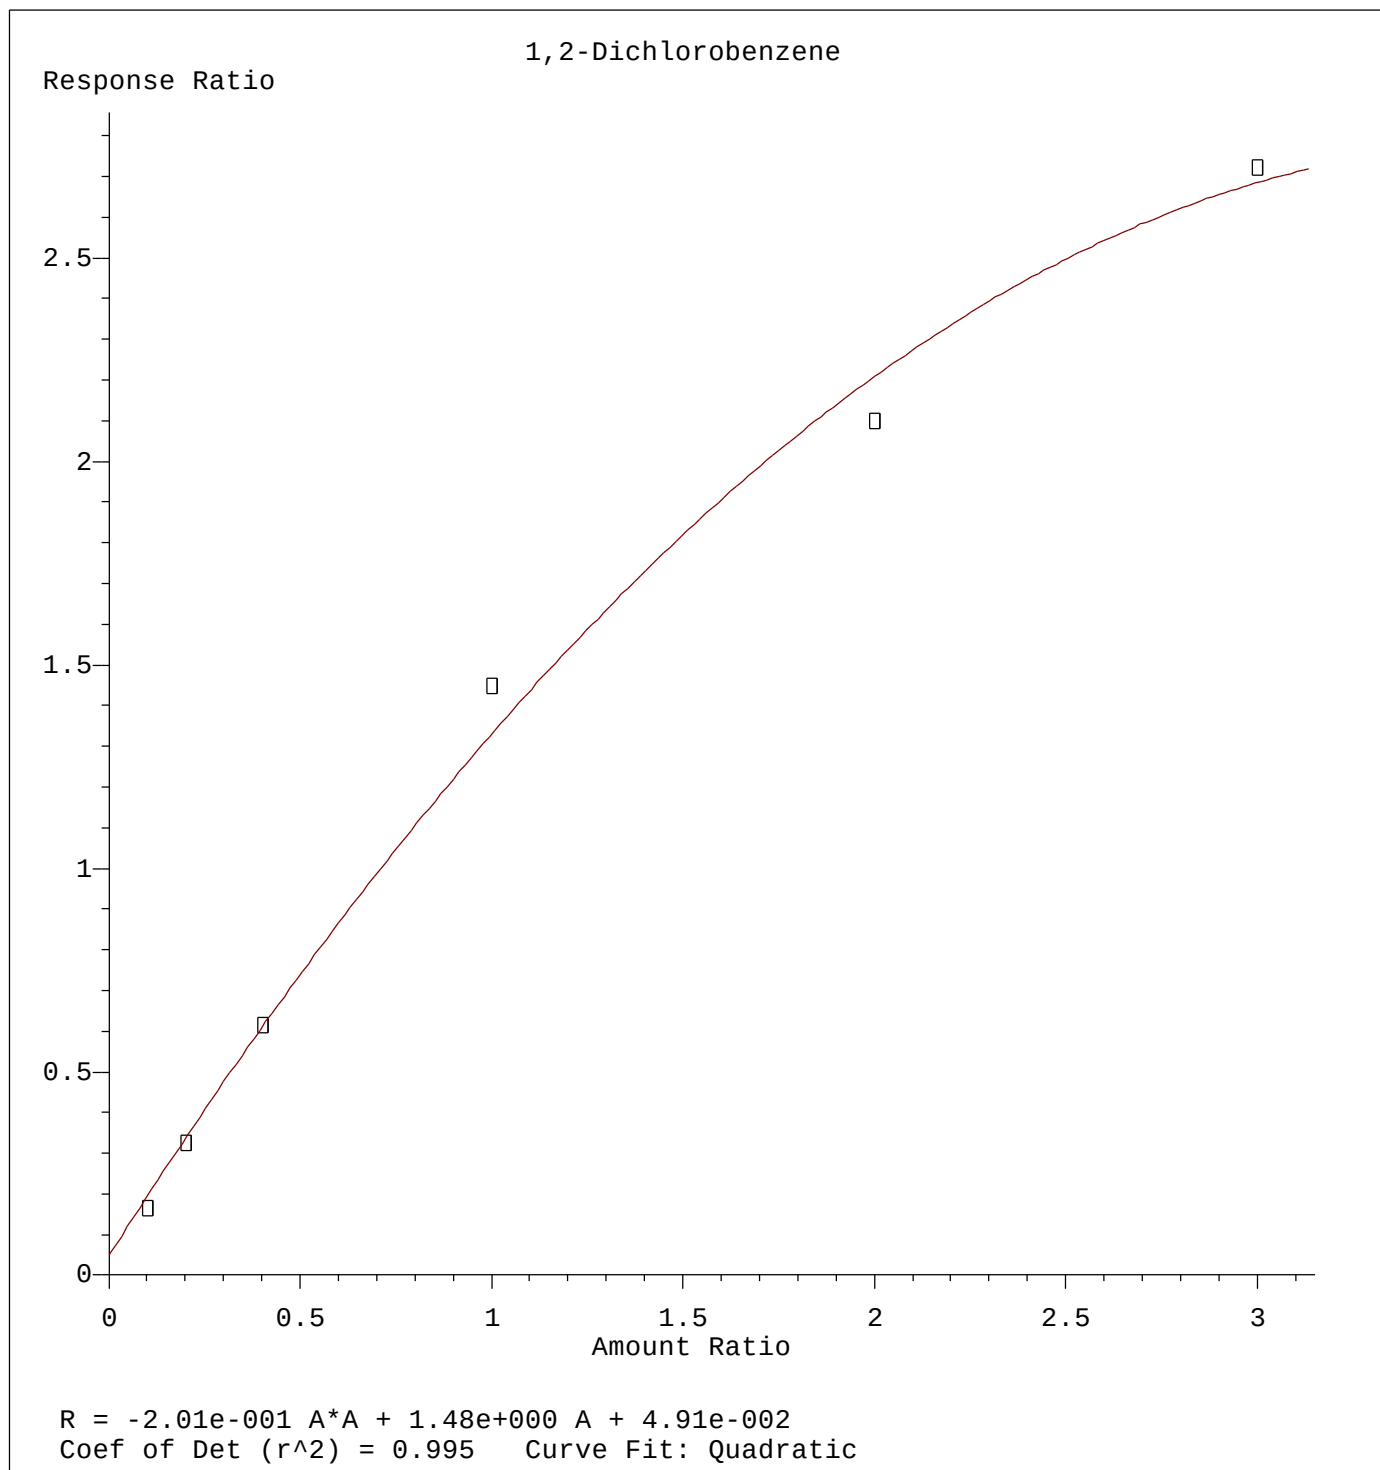


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D091318S.M  
Calibration Table Last Updated: Fri Sep 14 14:53:27 2018

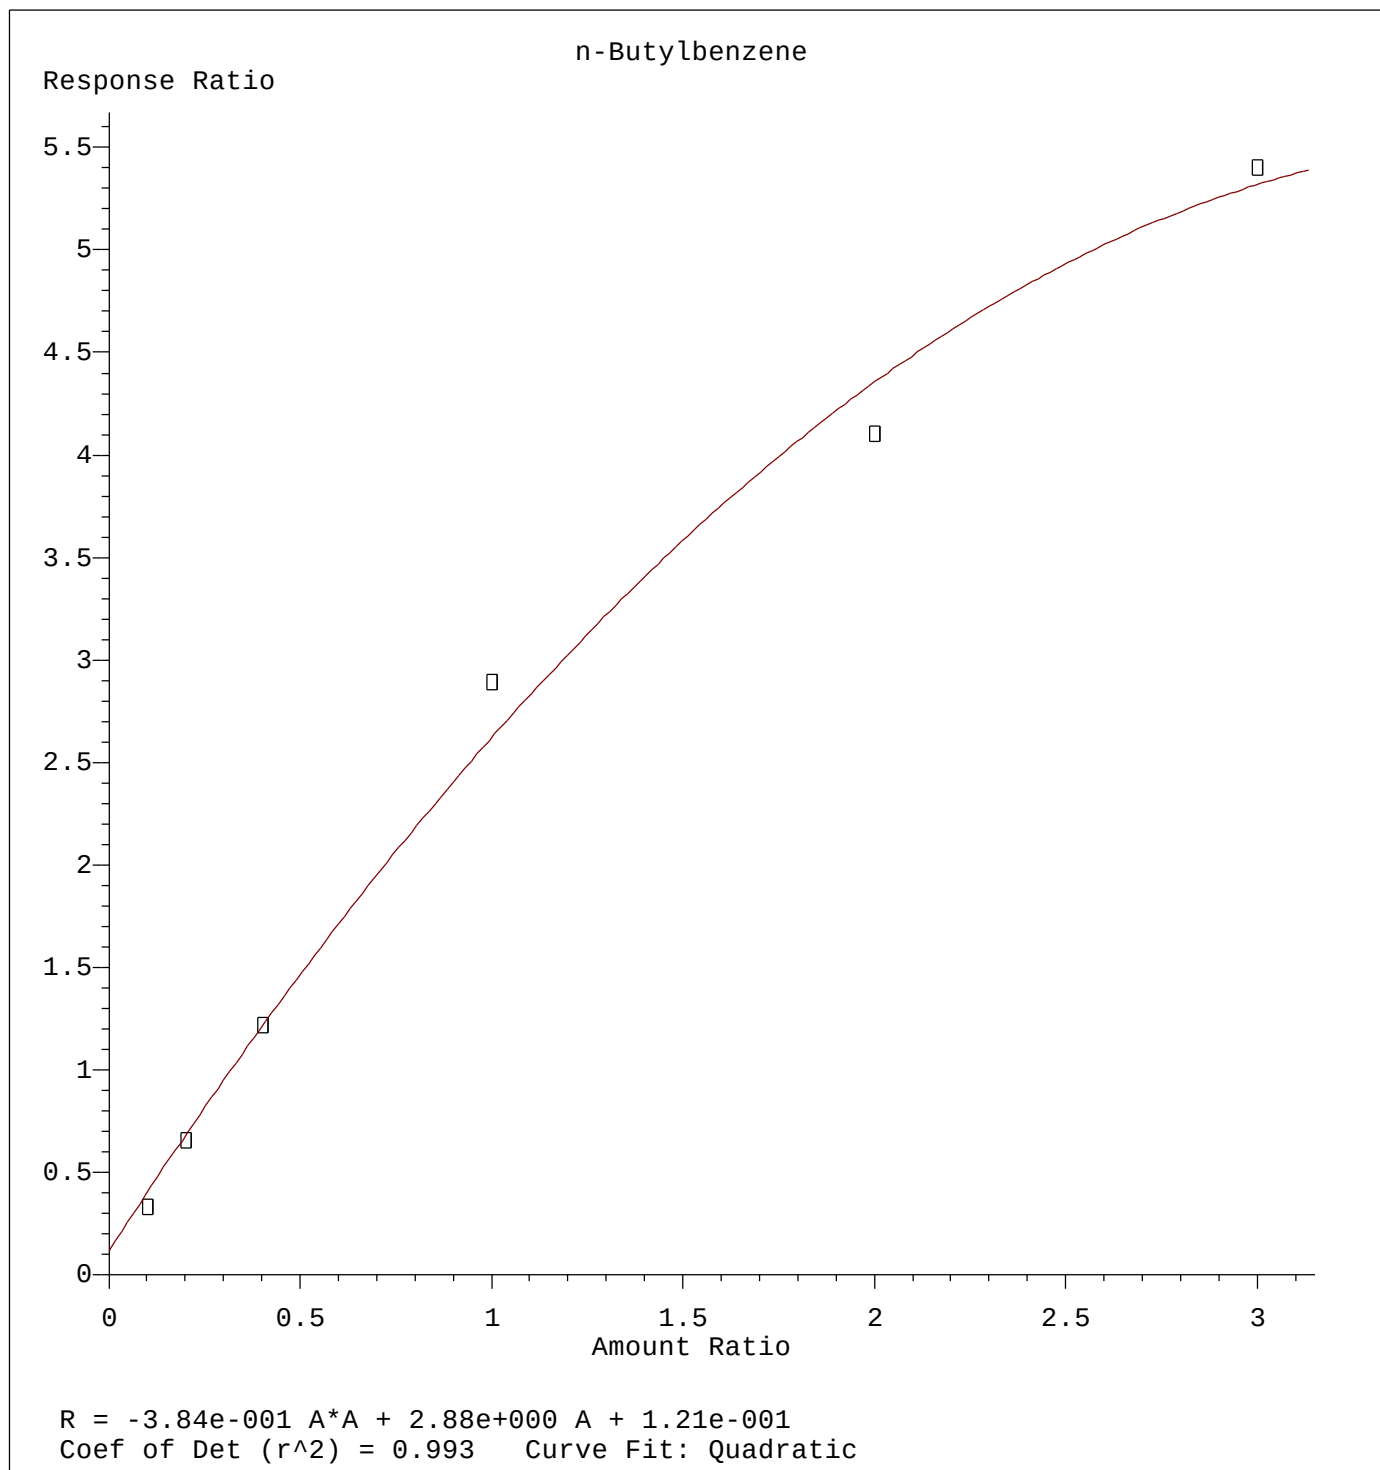

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D091318S.M  
Calibration Table Last Updated: Fri Sep 14 14:53:27 2018

# 2-Hexanone

Response Ratio

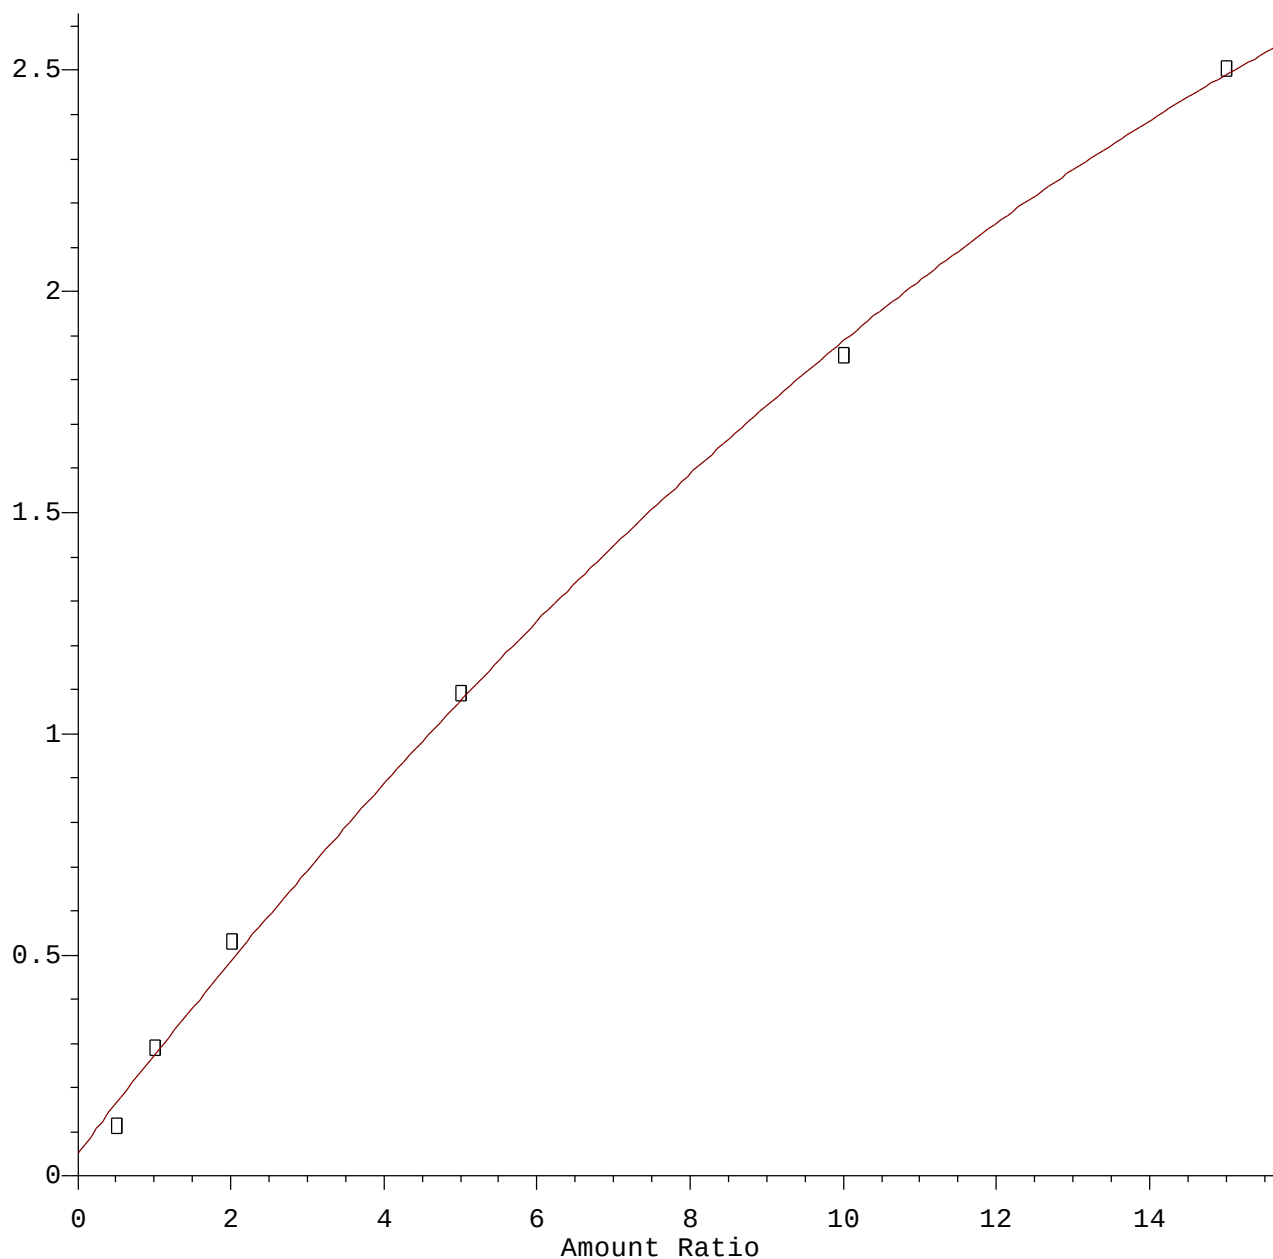


$R = -4.21e-003 A^2 + 2.26e-001 A + 5.27e-002$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D091318S.M  
Calibration Table Last Updated: Fri Sep 14 14:53:27 2018

# 4-Methyl-2-Pentanone

Response Ratio

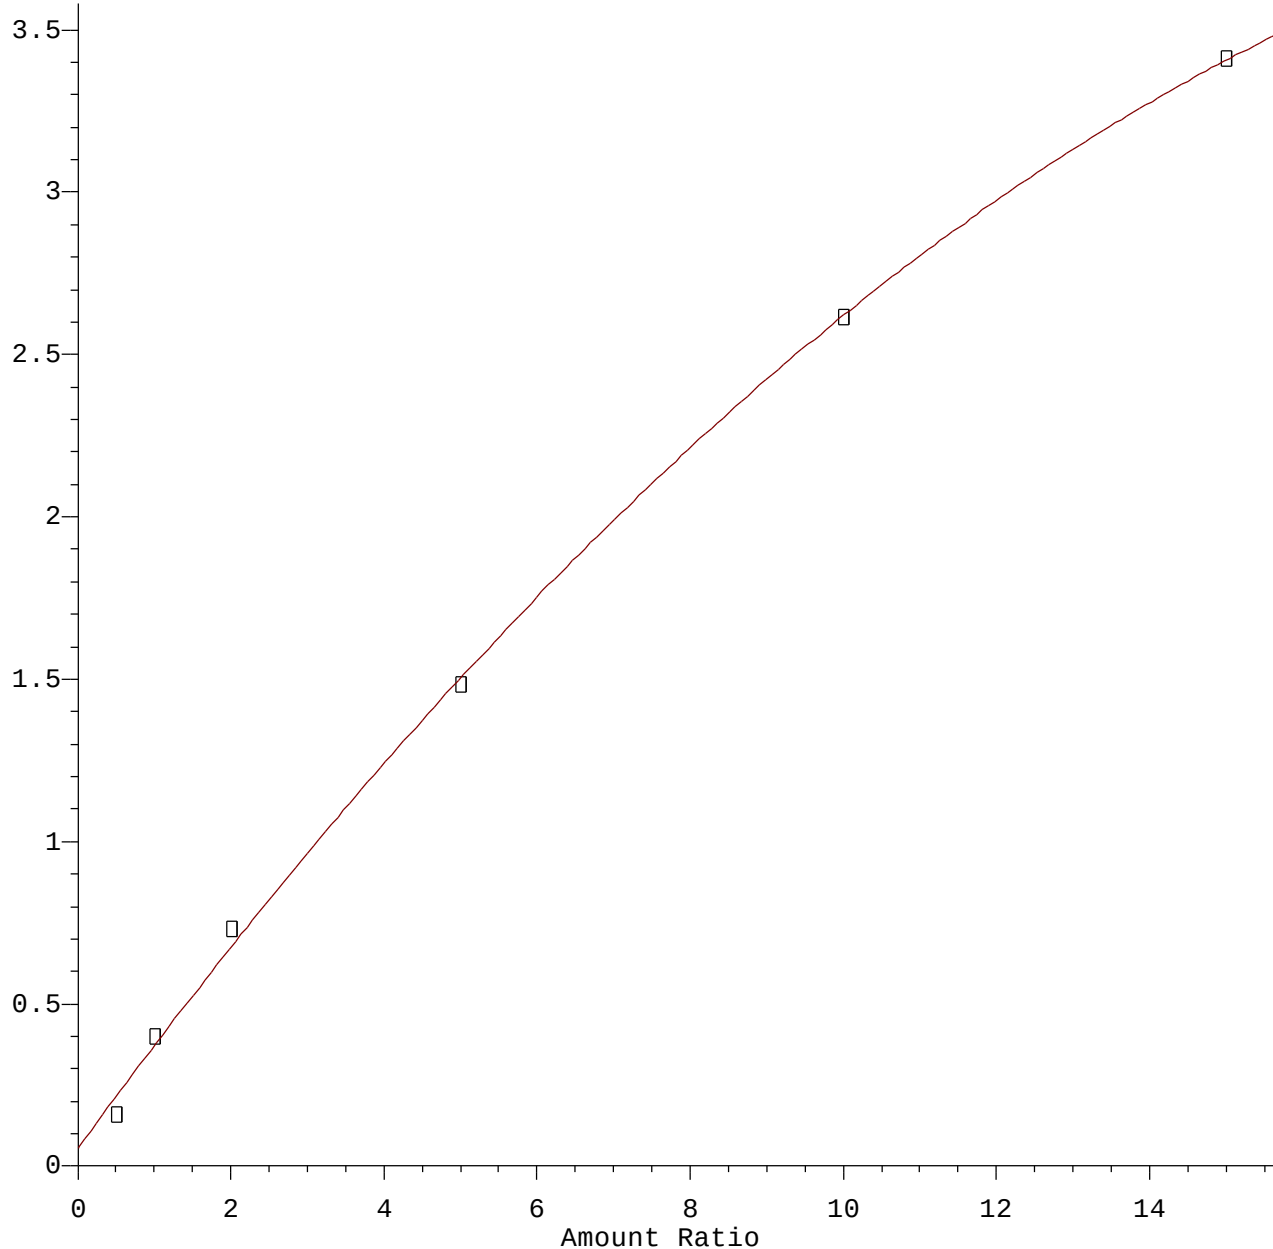

$R = -6.62e-003 A^2 + 3.23e-001 A + 5.61e-002$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D091318S.M  
Calibration Table Last Updated: Fri Sep 14 14:53:27 2018