


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD091318\
 Data File : VD059991.D
 Acq On : 13 Sep 2018 10:08
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091318S.M
 Title : SW846 8260
 Last Update : Thu Sep 13 16:17:40 2018

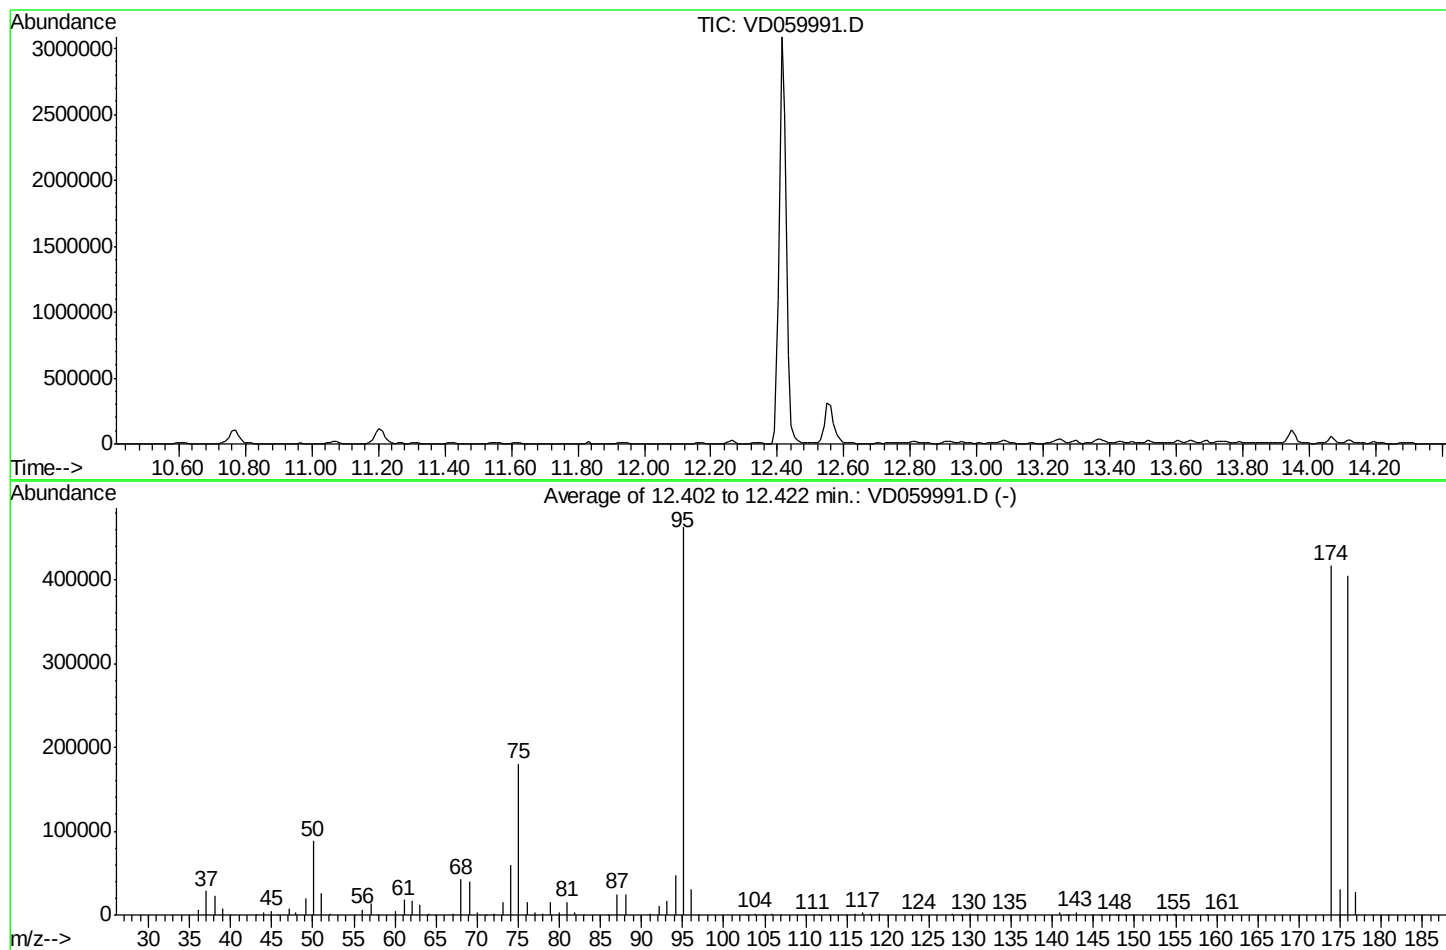

AutoFind: Scans 1105, 1106, 1107; Background Corrected with Scan 1100

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	88168	PASS
75	95	30	60	39.1	180645	PASS
95	95	100	100	100.0	462314	PASS
96	95	5	9	6.8	31266	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.0	416064	PASS
175	174	5	9	7.2	30031	PASS
176	174	95	101	97.4	405120	PASS
177	176	5	9	6.8	27409	PASS