
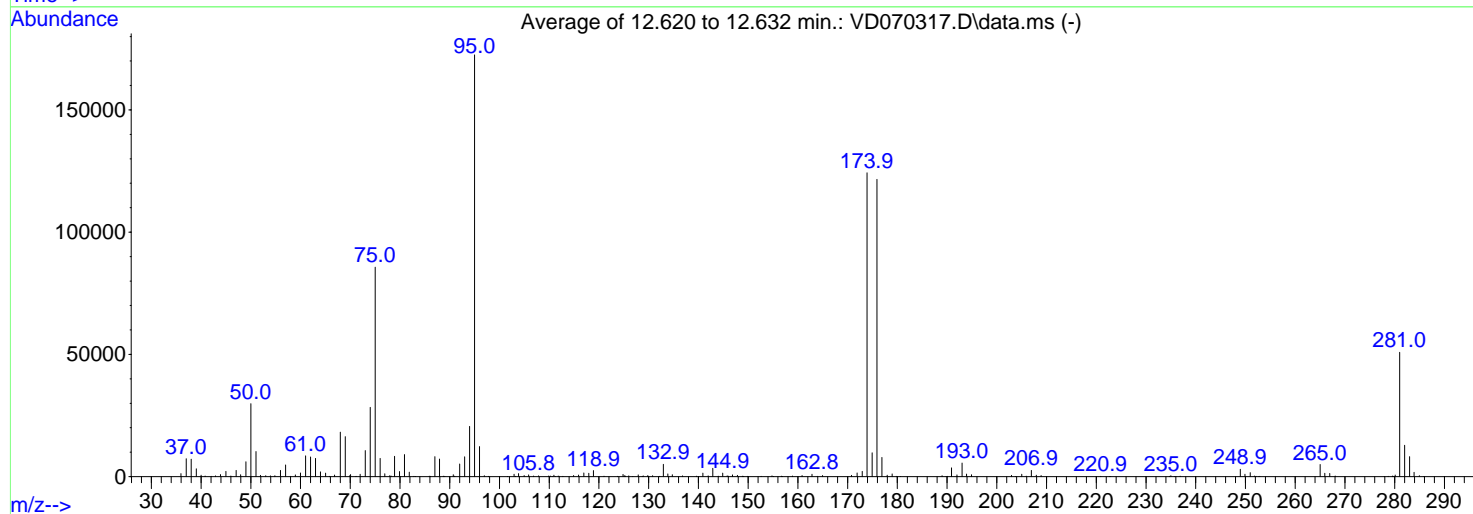


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD091321\  
 Data File : VD070317.D  
 Acq On : 13 Sep 2021 10:40  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D090821S.M  
 Title : SW846 8260  
 Last Update : Thu Sep 09 03:07:09 2021

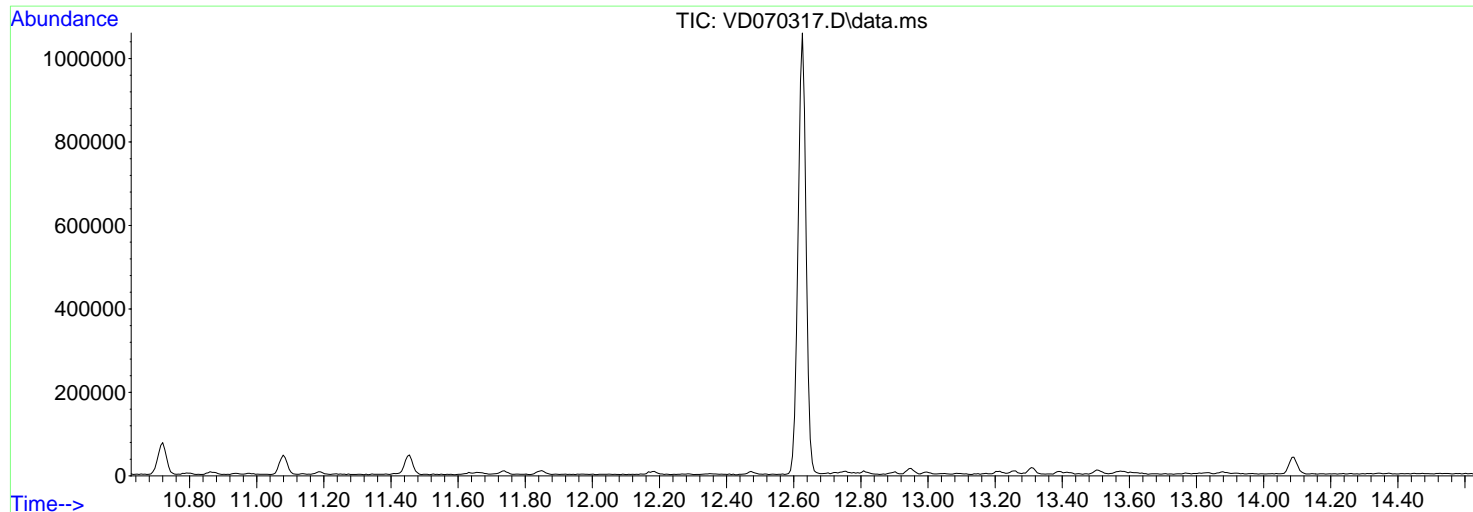

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	29856	PASS
75	95	30	60	49.7	85659	PASS
95	95	100	100	100.0	172523	PASS
96	95	5	9	7.1	12327	PASS
173	174	0.00	2	1.7	2153	PASS
174	95	50	100	72.0	124285	PASS
175	174	5	9	7.8	9751	PASS
176	174	95	101	97.9	121619	PASS
177	176	5	9	6.5	7871	PASS