

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091322\
 Data File : VD074268.D
 Acq On : 13 Sep 2022 16:17
 Operator : VA/SY
 Sample : N4581-01
 Misc : 4.99G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CRUSHED-MASONRY-PILE-6

Quant Time: Sep 14 01:56:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090922S.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 10 04:45:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	110993	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	195220	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.575	117	172544	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.504	152	76912	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	59983	53.008	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	106.020%
35) Dibromofluoromethane	7.804	113	54066	40.776	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	81.560%
50) Toluene-d8	10.263	98	240209	50.196	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	100.400%
62) 4-Bromofluorobenzene	12.563	95	74550	43.739	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	87.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091322\
Data File : VD074268.D
Acq On : 13 Sep 2022 16:17
Operator : VA/SY
Sample : N4581-01
Misc : 4.99G/5.00ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CRUSHED-MASONRY-PILE-6

Quant Time: Sep 14 01:56:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090922S.M
Quant Title : SW846 8260
QLast Update : Sat Sep 10 04:45:19 2022
Response via : Initial Calibration




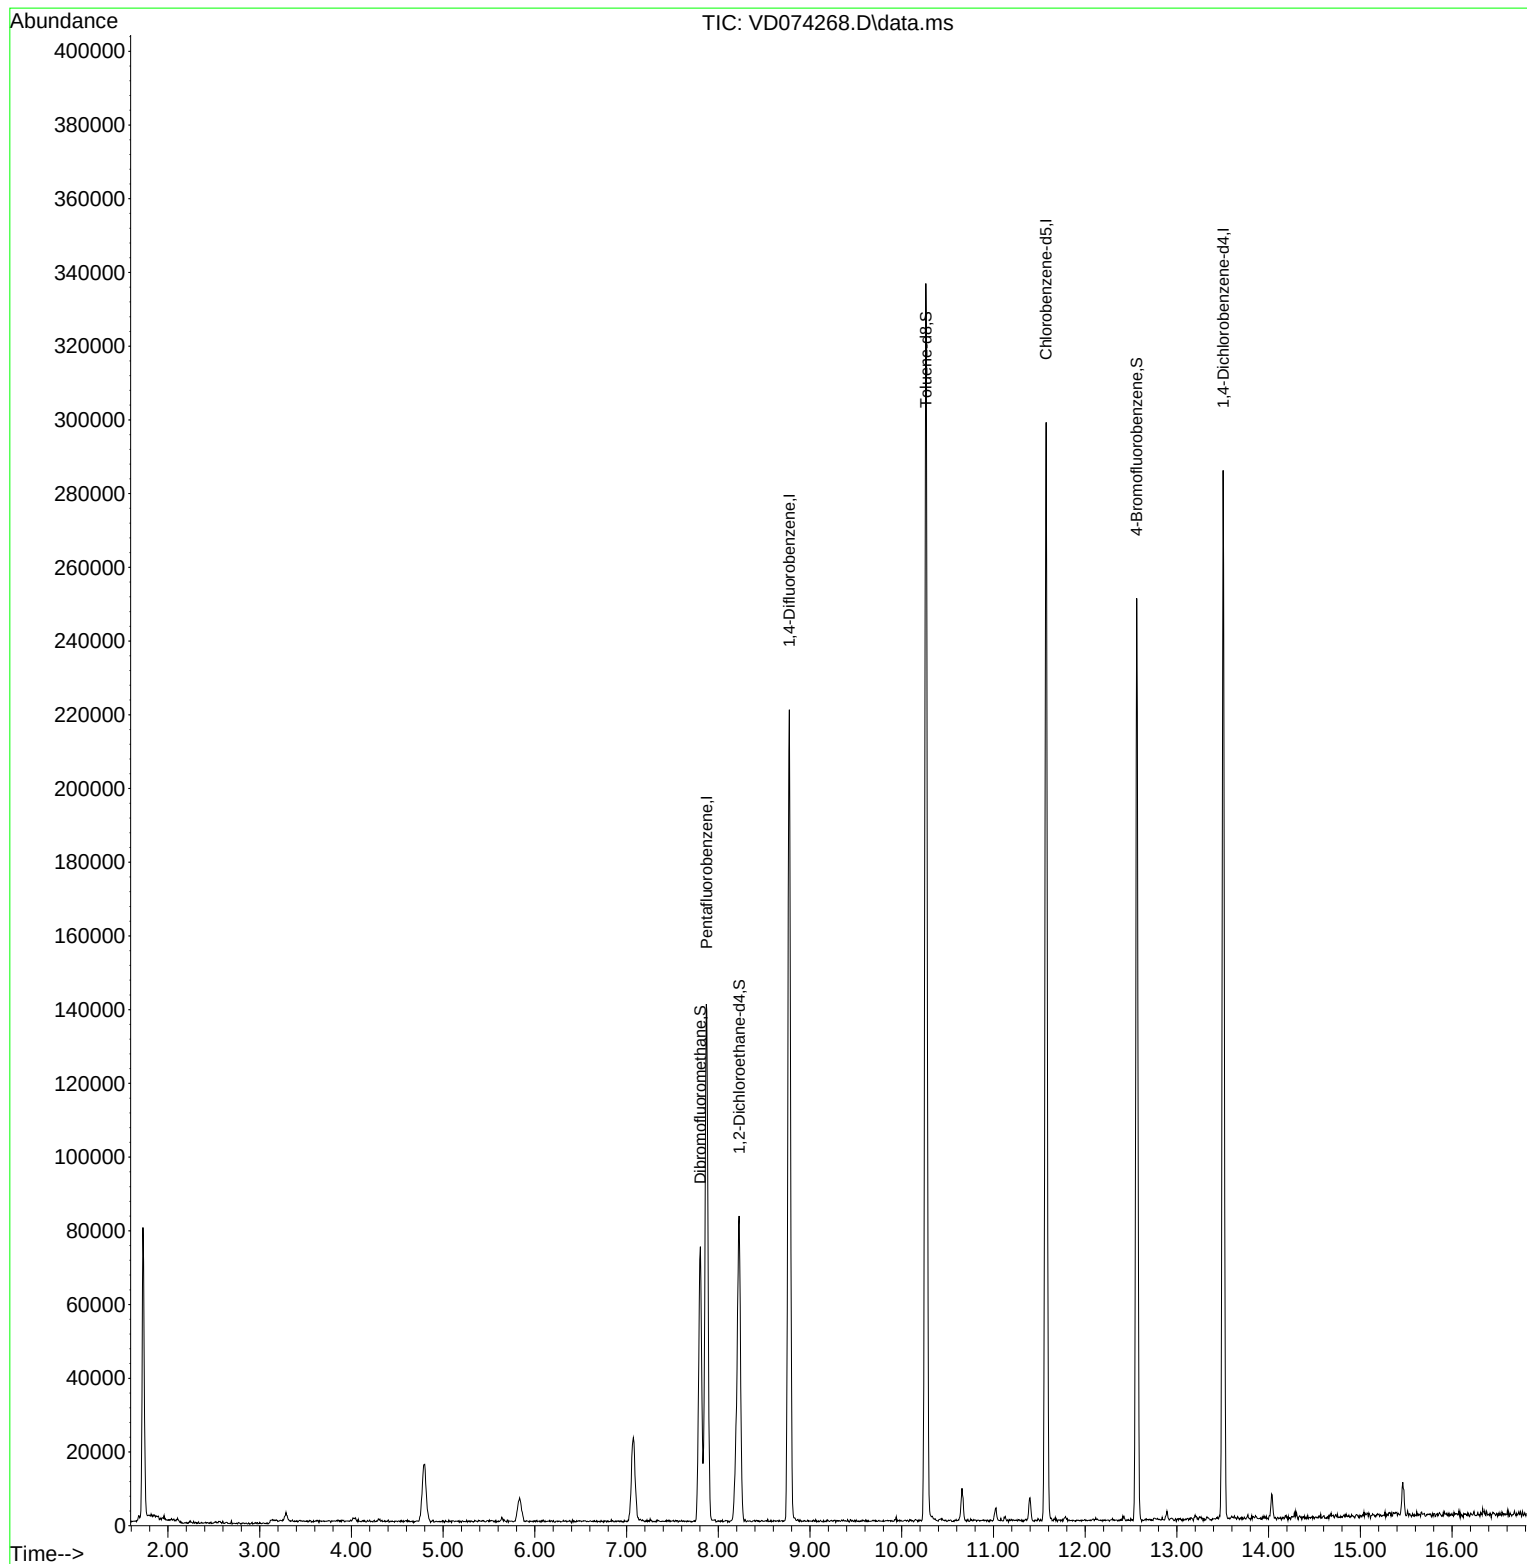


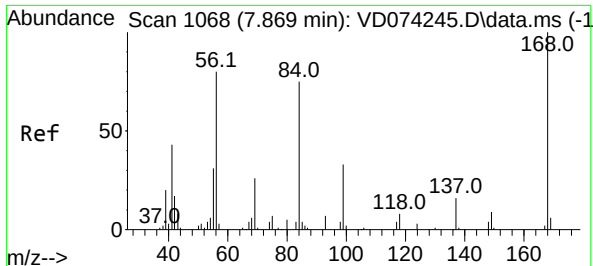

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1109
Delta R.T. 0.006 min
Lab File: VD074268.D
Acq: 13 Sep 2022 16:17




Instrument :
MSVOA_D
ClientSampleId :
CRUSHED-MASONRY-PILE-6


Tgt Ion:168 Resp: 110993
Ion Ratio Lower Upper
168 100
99 54.6 43.0 64.6

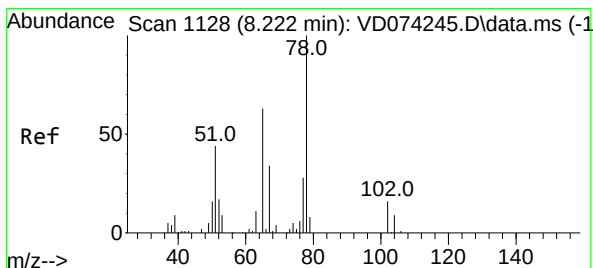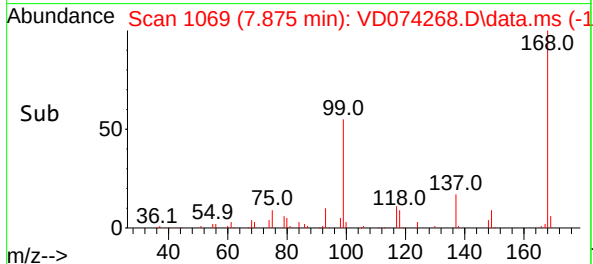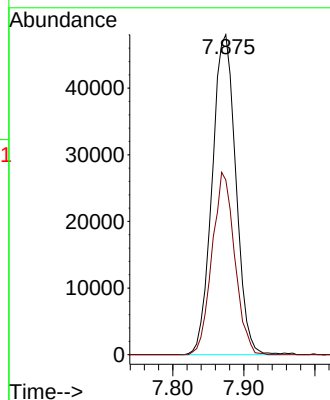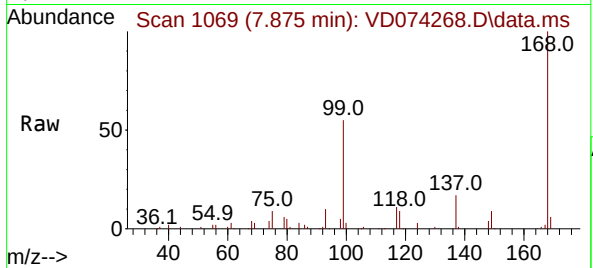

#33
1,2-Dichloroethane-d4
Concen: 53.008 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. 0.006 min
Lab File: VD074268.D
Acq: 13 Sep 2022 16:17

Tgt Ion: 65 Resp: 59983
Ion Ratio Lower Upper
65 100
67 56.3 0.0 110.6

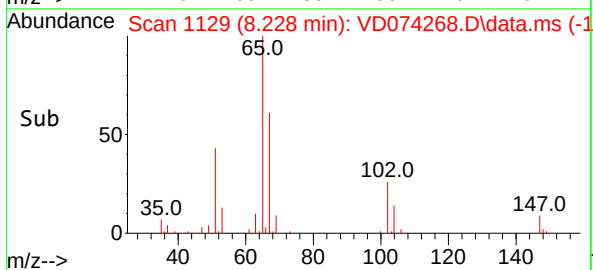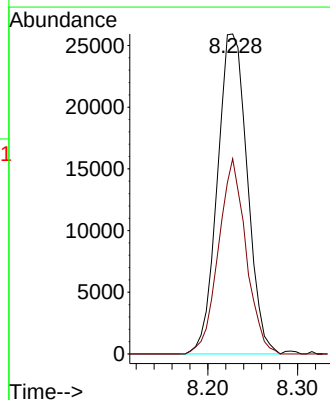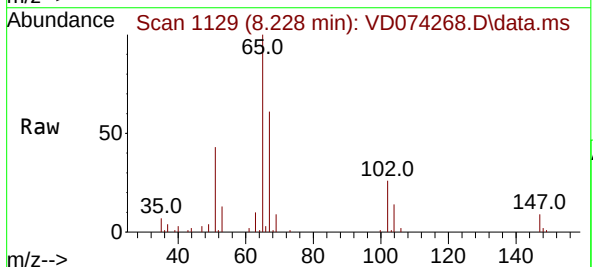

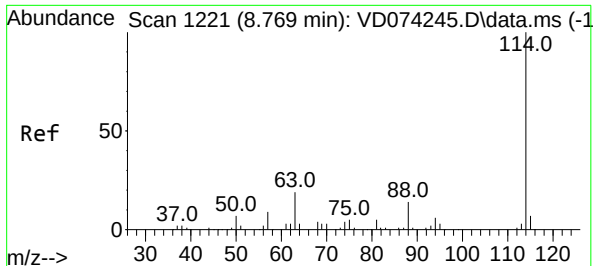

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. 0.005 min

Lab File: VD074268.D

Acq: 13 Sep 2022 16:17

Instrument :

MSVOA_D

ClientSampleId :

CRUSHED-MASONRY-PILE-6





Tgt Ion:114 Resp: 195220

Ion Ratio Lower Upper

114 100

63 19.1 0.0 37.6

88 14.1 0.0 28.4

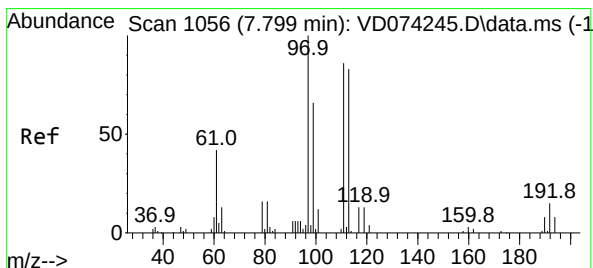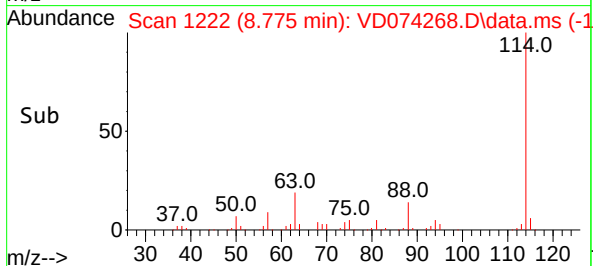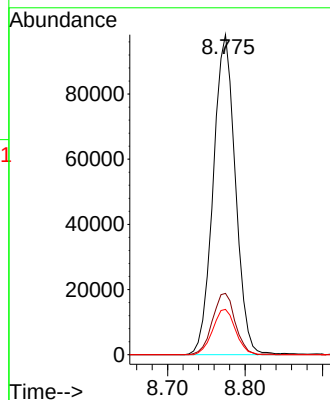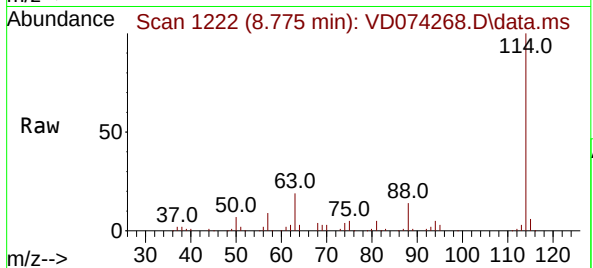

#35

Dibromofluoromethane

Concen: 40.776 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. 0.005 min

Lab File: VD074268.D

Acq: 13 Sep 2022 16:17




Tgt Ion:113 Resp: 54066


Ion Ratio Lower Upper

113 100

111 100.4 83.0 124.6

192 19.3 16.2 24.2


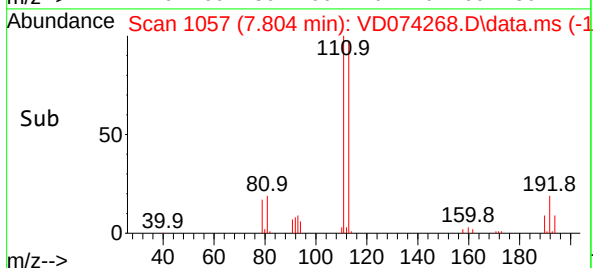
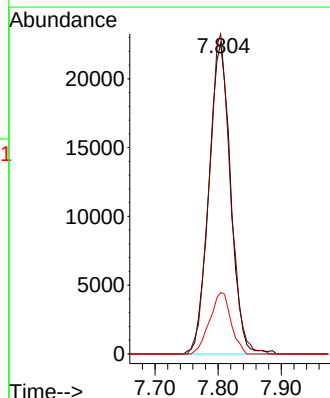
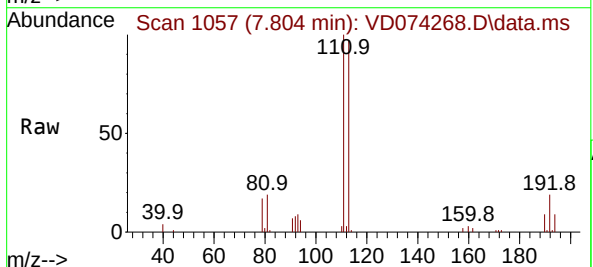


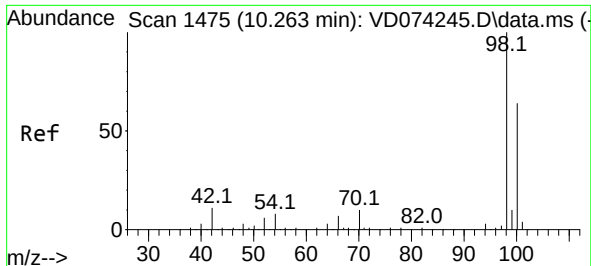

#50
Toluene-d8
Concen: 50.196 ug/l
RT: 10.263 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VD074268.D
Acq: 13 Sep 2022 16:17




Instrument :
MSVOA_D
ClientSampleId :
CRUSHED-MASONRY-PILE-6


Tgt Ion: 98 Resp: 240209
Ion Ratio Lower Upper
98 100
100 64.2 51.8 77.8

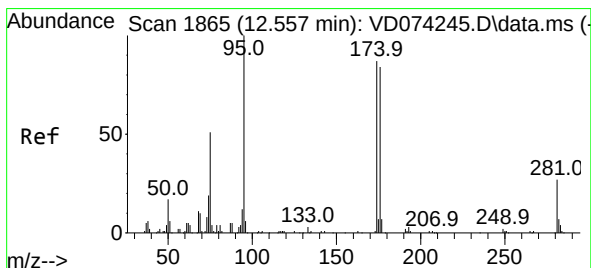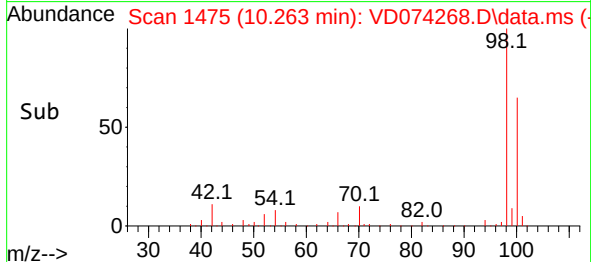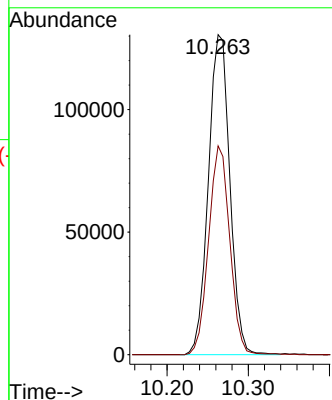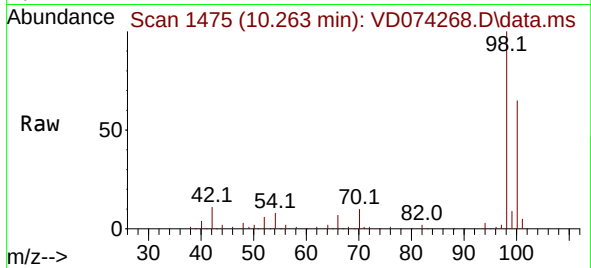

#62
4-Bromofluorobenzene
Concen: 43.739 ug/l
RT: 12.563 min Scan# 1866
Delta R.T. 0.006 min
Lab File: VD074268.D
Acq: 13 Sep 2022 16:17

Tgt Ion: 95 Resp: 74550
Ion Ratio Lower Upper
95 100
174 90.1 0.0 179.2
176 84.8 0.0 171.4


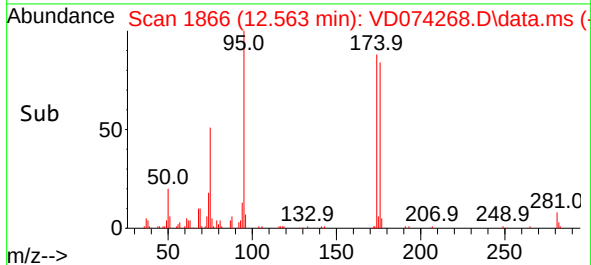
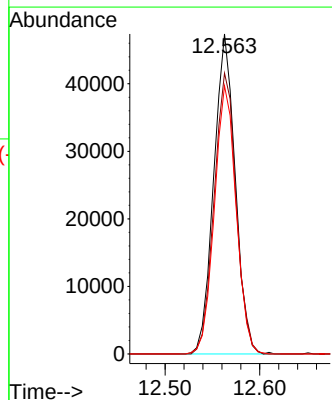
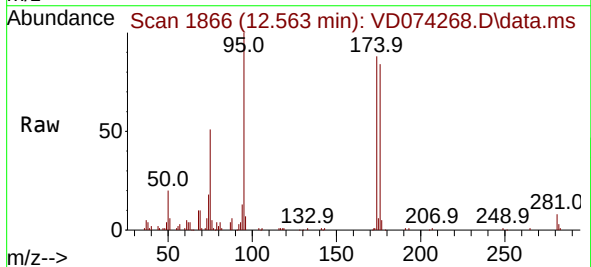


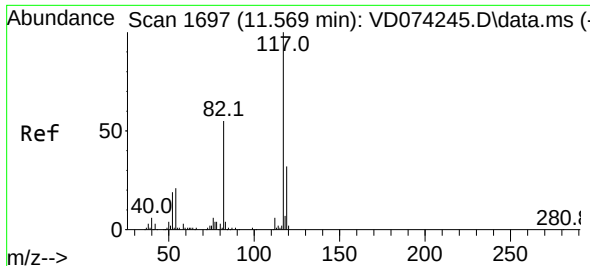

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.575 min Scan# 1
Delta R.T. 0.006 min
Lab File: VD074268.D
Acq: 13 Sep 2022 16:17

Instrument :
MSVOA_D
ClientSampleId :
CRUSHED-MASONRY-PILE-6

Tgt Ion:117 Resp: 172544
Ion Ratio Lower Upper
117 100
82 53.7 44.2 66.2
119 31.6 25.4 38.0

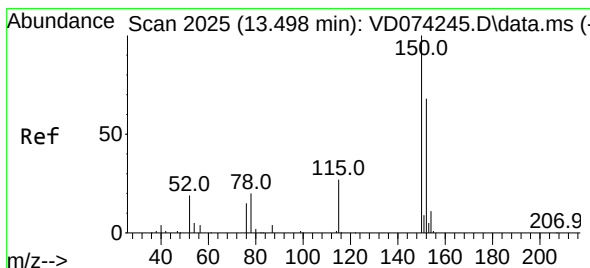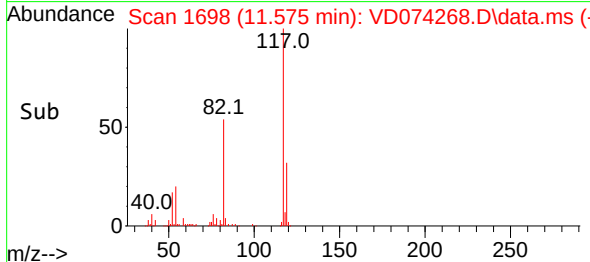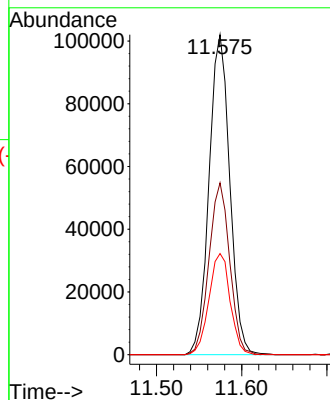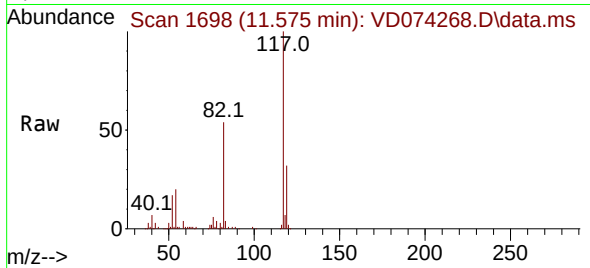

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.504 min Scan# 2026
Delta R.T. 0.006 min
Lab File: VD074268.D
Acq: 13 Sep 2022 16:17

Tgt Ion:152 Resp: 76912
Ion Ratio Lower Upper
152 100
115 55.6 28.4 85.2
150 155.5 0.0 351.0

