
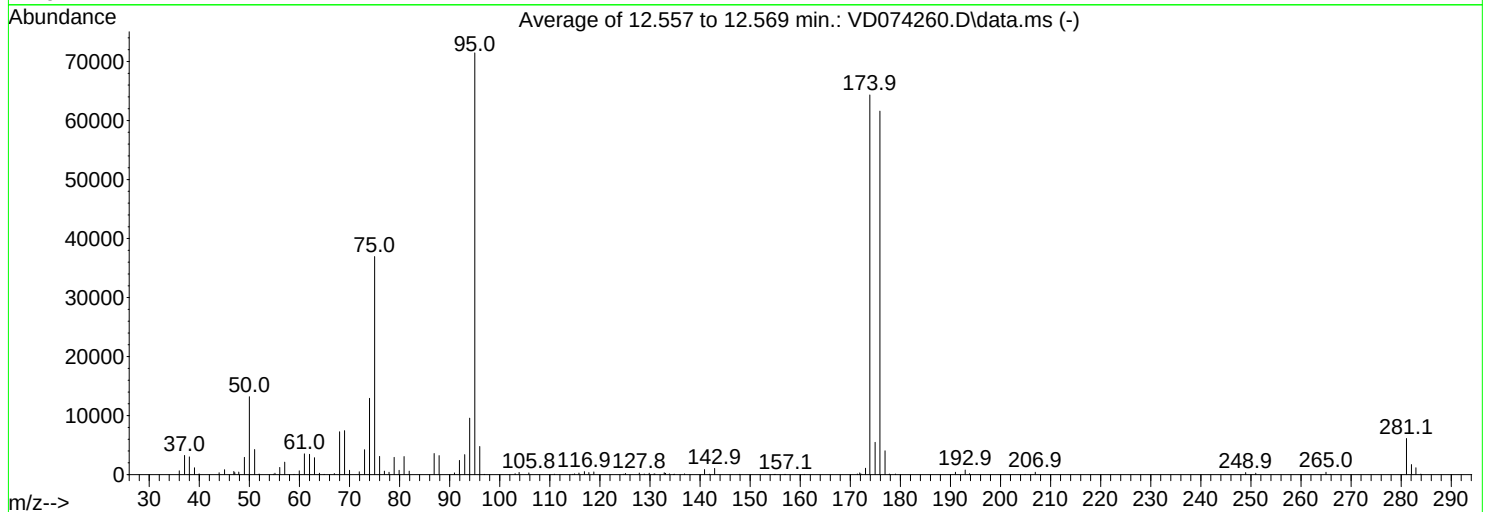


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091322\
Data File : VD074260.D
Acq On : 13 Sep 2022 10:03
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090922S.M
Title : SW846 8260
Last Update : Sat Sep 10 04:45:19 2022

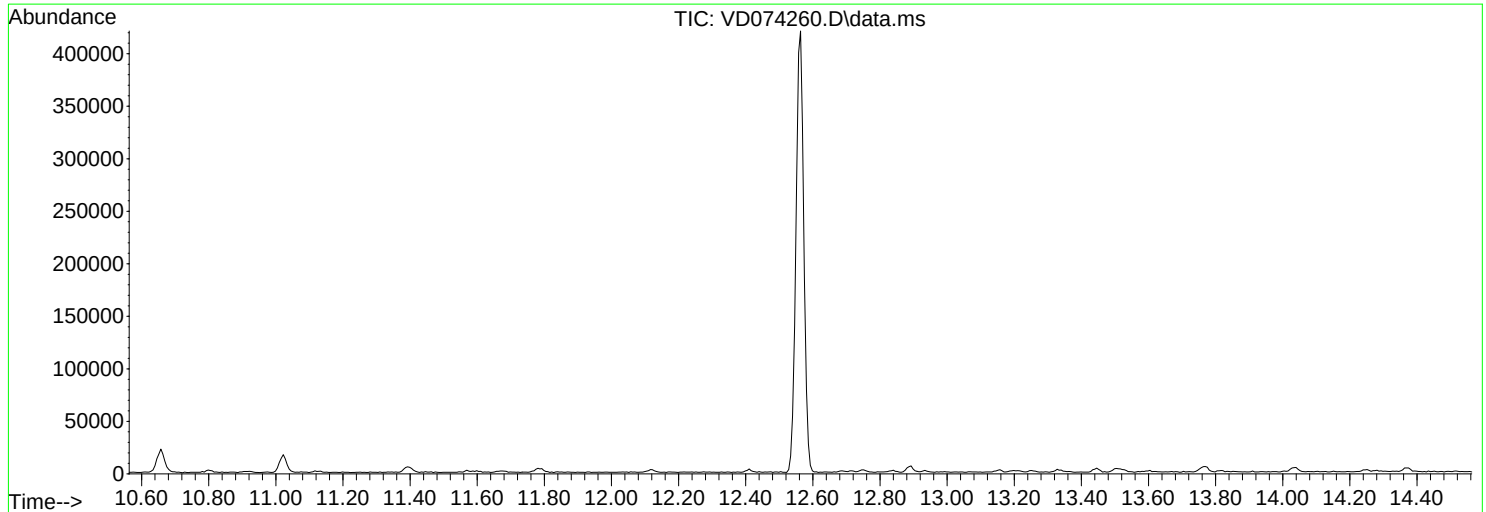

AutoFind: Scans 1865, 1866, 1867; Background Corrected with Scan 1857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	13205	PASS
75	95	30	60	51.7	36947	PASS
95	95	100	100	100.0	71464	PASS
96	95	5	9	6.7	4773	PASS
173	174	0.00	2	1.7	1087	PASS
174	95	50	100	90.0	64320	PASS
175	174	5	9	8.5	5489	PASS
176	174	95	101	95.8	61595	PASS
177	176	5	9	6.6	4051	PASS