

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD091418\
 Data File : VD060009.D
 Acq On : 14 Sep 2018 14:46
 Operator : JC/SY
 Sample : J4873-03RE
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 NF-CON-2RE

Quant Time: Sep 14 15:47:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091318S.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 13 16:17:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.38	168	1448436	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	7.42	114	2027960	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.27	117	1643149	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.36	152	839850	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.76	65	509013	45.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.12%	
35) Dibromofluoromethane	6.31	113	28368	1.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	3.58%	
50) Toluene-d8	9.43	98	1797785	40.94	ug/l	0.00
Spiked Amount	50.000		Recovery	=	81.88%	
62) 4-Bromofluorobenzene	12.42	95	677754	40.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	80.80%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD091418\
Data File : VD060009.D
Acq On : 14 Sep 2018 14:46
Operator : JC/SY
Sample : J4873-03RE
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
NF-CON-2RE

Quant Time: Sep 14 15:47:18 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D091318S.M
Quant Title : SW846 8260
QLast Update : Thu Sep 13 16:17:40 2018
Response via : Initial Calibration

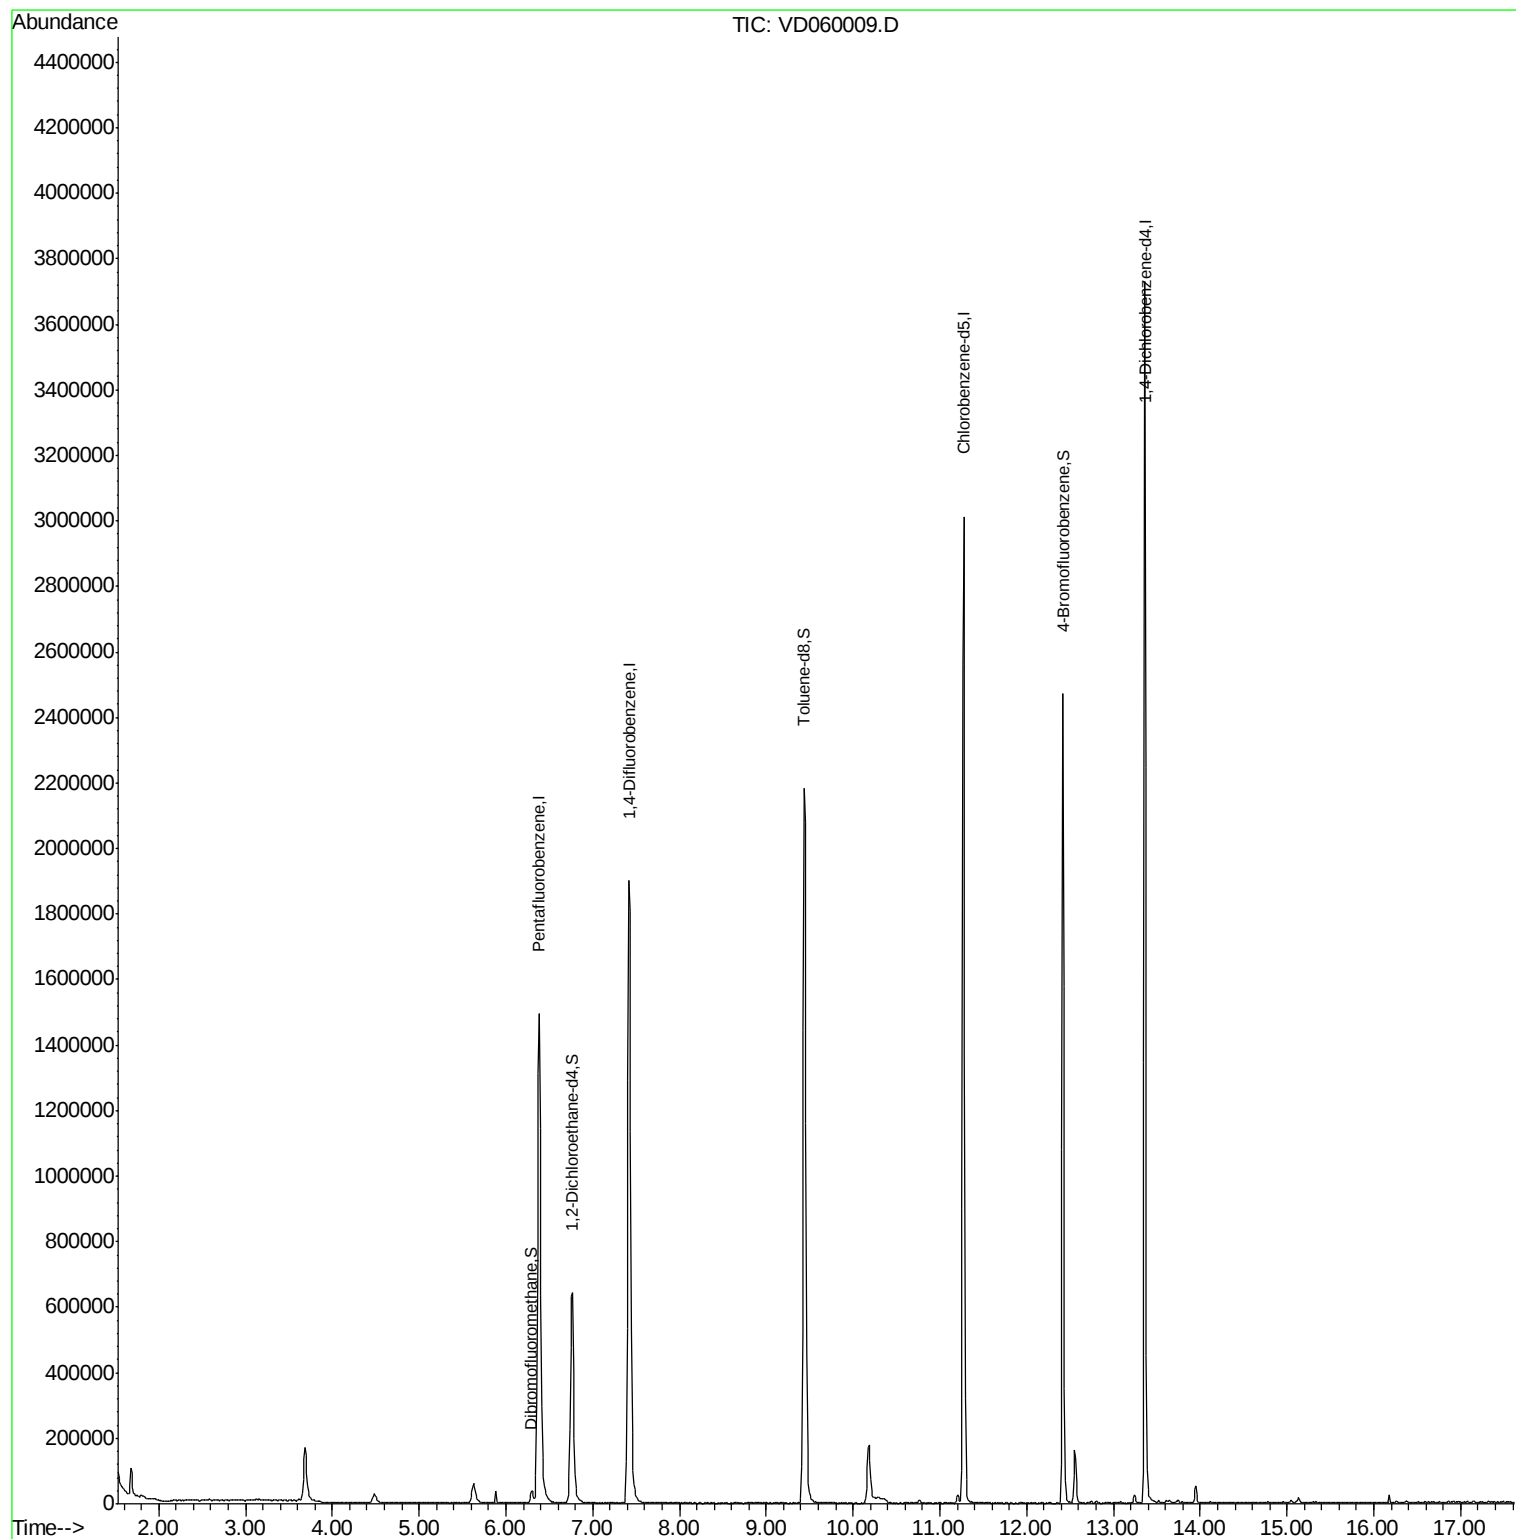

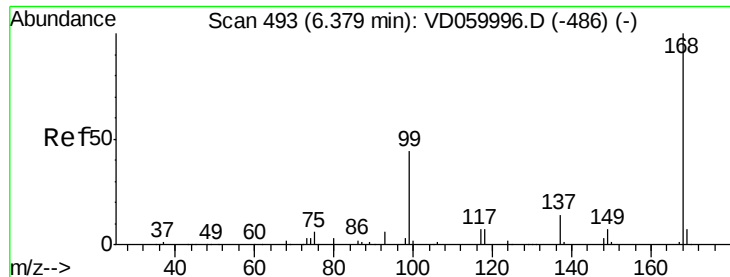

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 6.38 min Scan# 494

Delta R.T. 0.00 min

Lab File: VD060009.D

Acq: 14 Sep 2018 14:46

Instrument :

MSVOA_D

ClientSampleId :


NF-CON-2RE

Tot Ion:168 Resp: 1448436

Ion Ratio Lower Upper




168 100

99 49.1 38.5 57.7

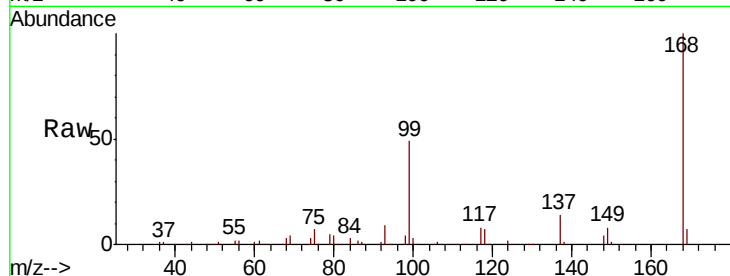

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

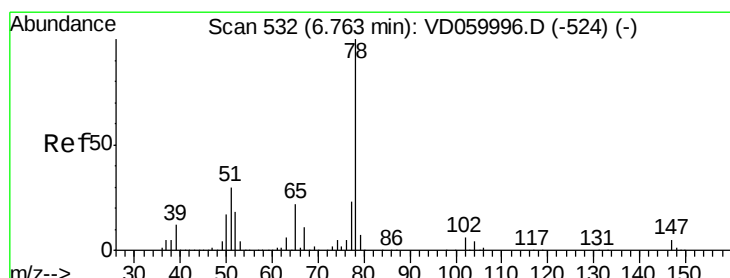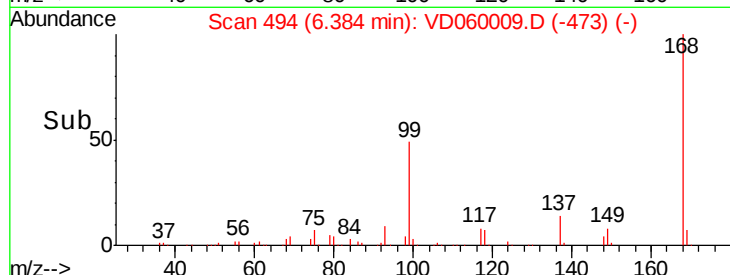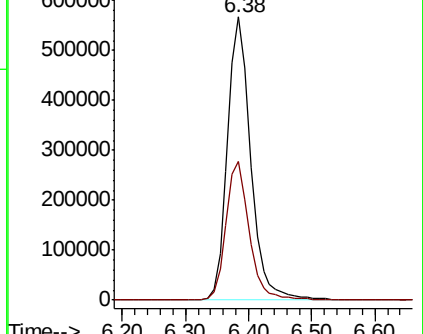

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 6.76 min Scan# 532

Delta R.T. -0.00 min

Lab File: VD060009.D


Acq: 14 Sep 2018 14:46

Tgt Ion: 65 Resp: 509013

Ion Ratio Lower Upper



65 100


67 52.1 0.0 104.8

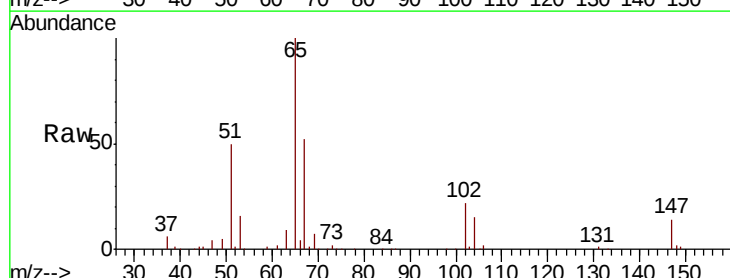

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

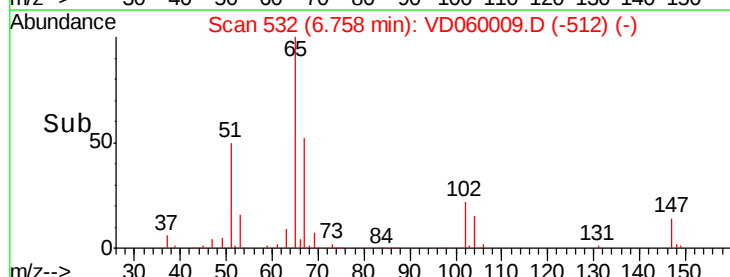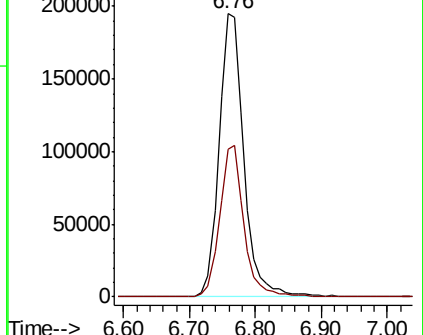


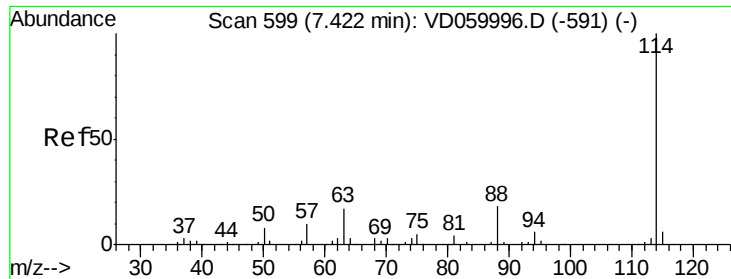




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 7.42 min Scan# 599
 Delta R.T. -0.00 min
 Lab File: VD060009.D
 Acq: 14 Sep 2018 14:46

Instrument :
 MSVOA_D
 ClientSampleId :
 NF-CON-2RE

Tot Ion:114 Resp: 2027960
 Ion Ratio Lower Upper
 114 100
 63 19.1 0.0 34.4
 88 18.4 0.0 35.8

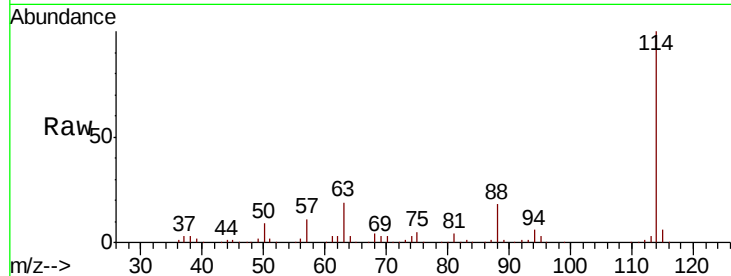


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

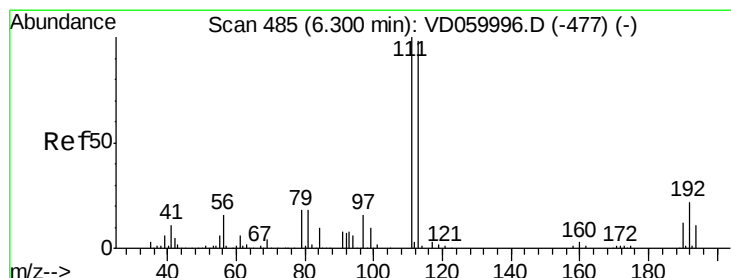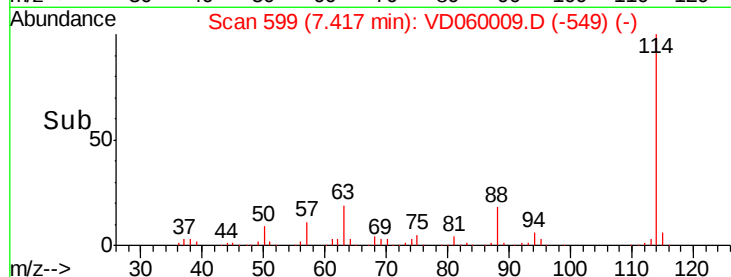
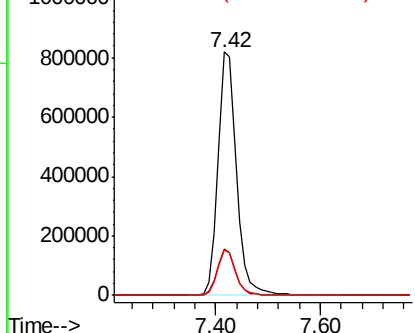



#35
 Dibromofluoromethane
 Concen: 50.00 ug/l
 RT: 6.31 min Scan# 486
 Delta R.T. 0.00 min
 Lab File: VD060009.D
 Acq: 14 Sep 2018 14:46

Tgt Ion:113 Resp: 28368
 Ion Ratio Lower Upper
 113 100
 111 99.0 81.3 121.9
 192 19.8 18.1 27.1

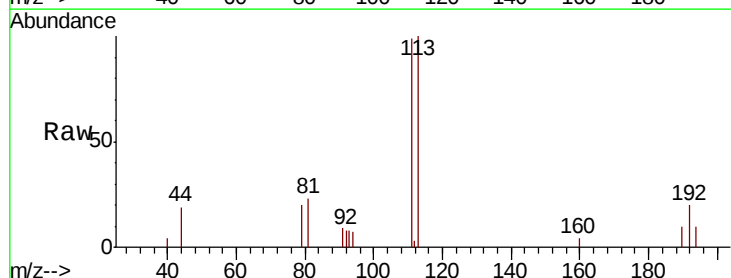

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

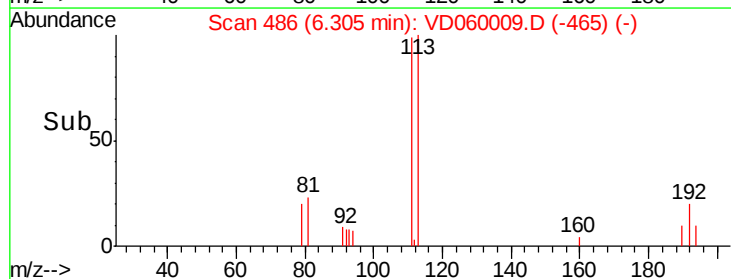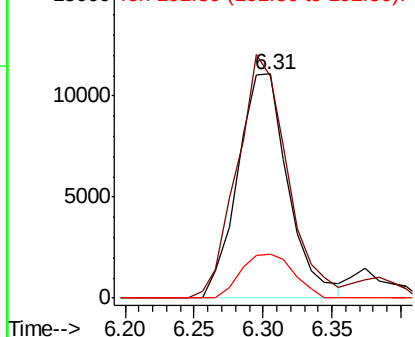


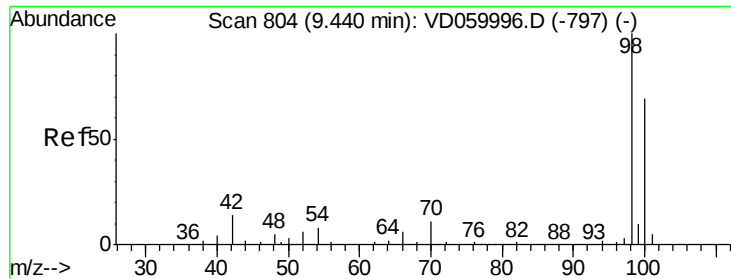




#50
Toluene-d8
Concen: N.D. ug/l
RT: 9.43 min Scan# 804
Delta R.T. -0.01 min
Lab File: VD060009.D
Acq: 14 Sep 2018 14:46

Instrument :
MSVOA_D
ClientSampleId :
NF-CON-2RE

Tot Ion: 98 Resp: 1797785
Ion Ratio Lower Upper
98 100
100 68.7 55.8 83.6

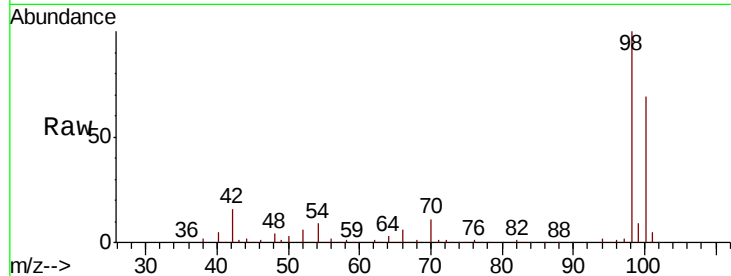


Abundance Ion 98.05 (97.75 to 98.75): VD0
Ion 100.05 (99.75 to 100.75): VD

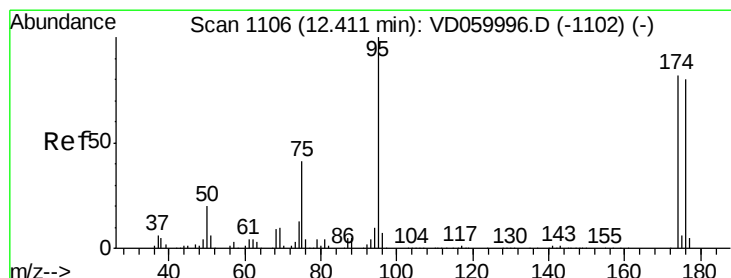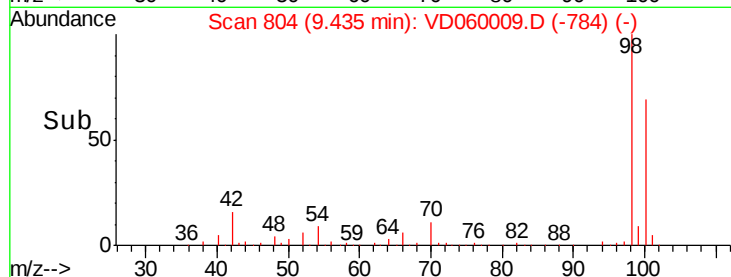
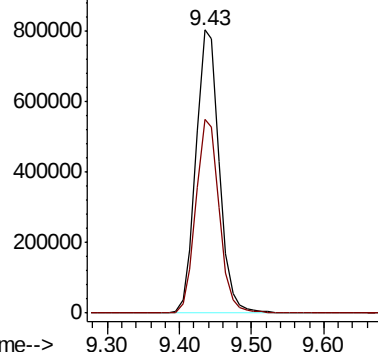



#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.42 min Scan# 1107
Delta R.T. 0.00 min
Lab File: VD060009.D
Acq: 14 Sep 2018 14:46

Tgt Ion: 95 Resp: 677754
Ion Ratio Lower Upper
95 100
174 89.0 0.0 165.0
176 86.5 0.0 160.2

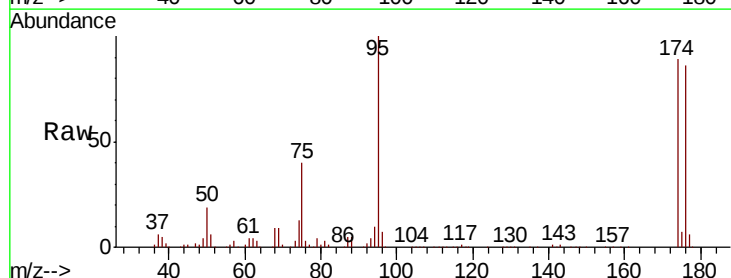

Abundance Ion 95.00 (94.70 to 95.70): VD0
Ion 173.90 (173.60 to 174.60): V
Ion 175.90 (175.60 to 176.60): V

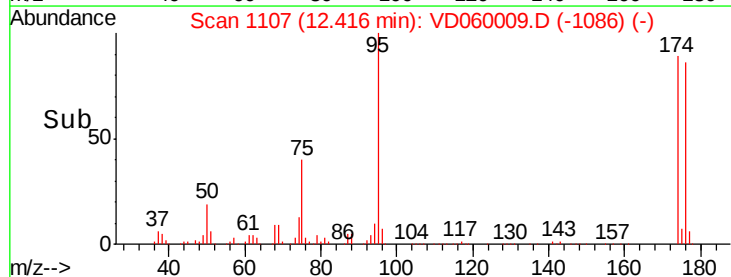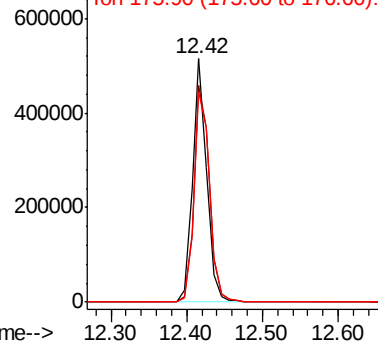


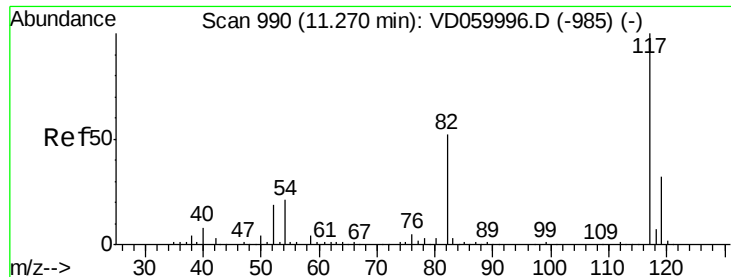




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.27 min Scan# 991
Delta R.T. 0.00 min
Lab File: VD060009.D
Acq: 14 Sep 2018 14:46

Instrument :
MSVOA_D
ClientSampleId :
NF-CON-2RE

Tot Ion:117 Resp: 1643149
Ion Ratio Lower Upper
117 100
82 52.6 41.7 62.5
119 33.0 26.0 39.0

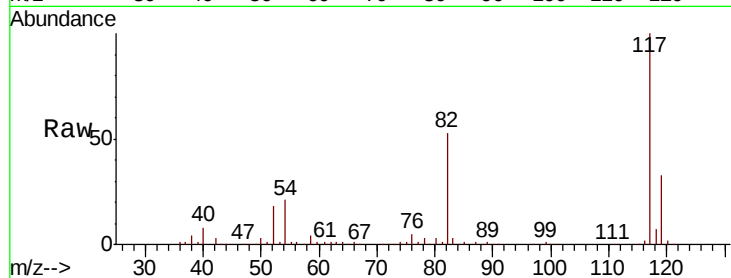


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

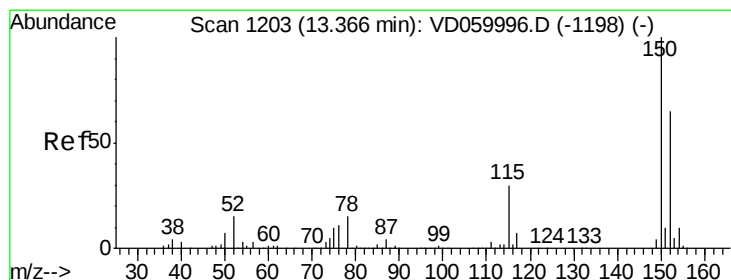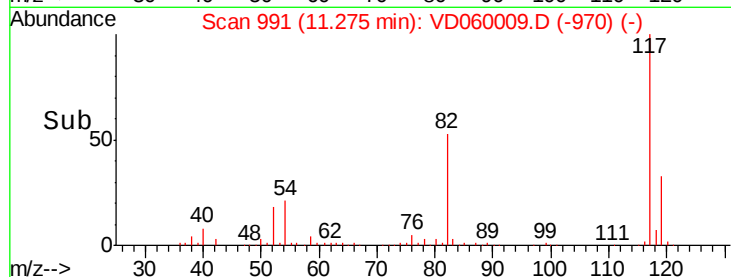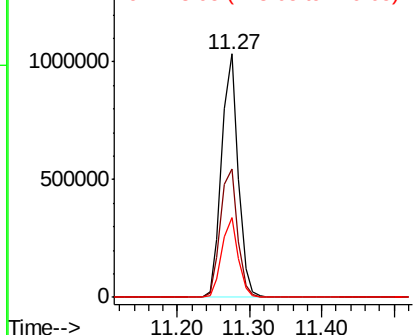

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.36 min Scan# 1203
Delta R.T. -0.00 min
Lab File: VD060009.D
Acq: 14 Sep 2018 14:46

Tgt Ion:152 Resp: 839850
Ion Ratio Lower Upper
152 100
115 54.9 24.6 73.8
150 155.5 0.0 313.4

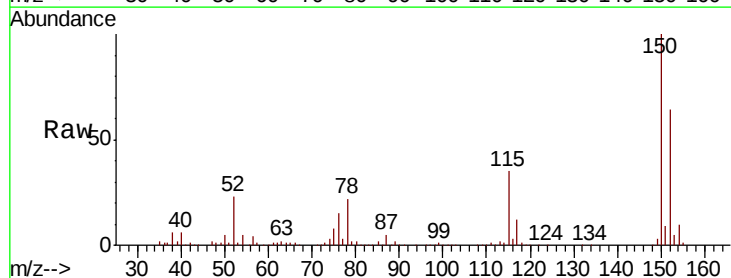

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

