


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD091418\  
Data File : VD060000.D  
Acq On : 14 Sep 2018 9:54  
Operator : JC/SY  
Sample : BFB  
Misc : 5.00µl/5ml/MSVOA D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D091318S.M  
Title : SW846 8260  
Last Update : Thu Sep 13 16:17:40 2018

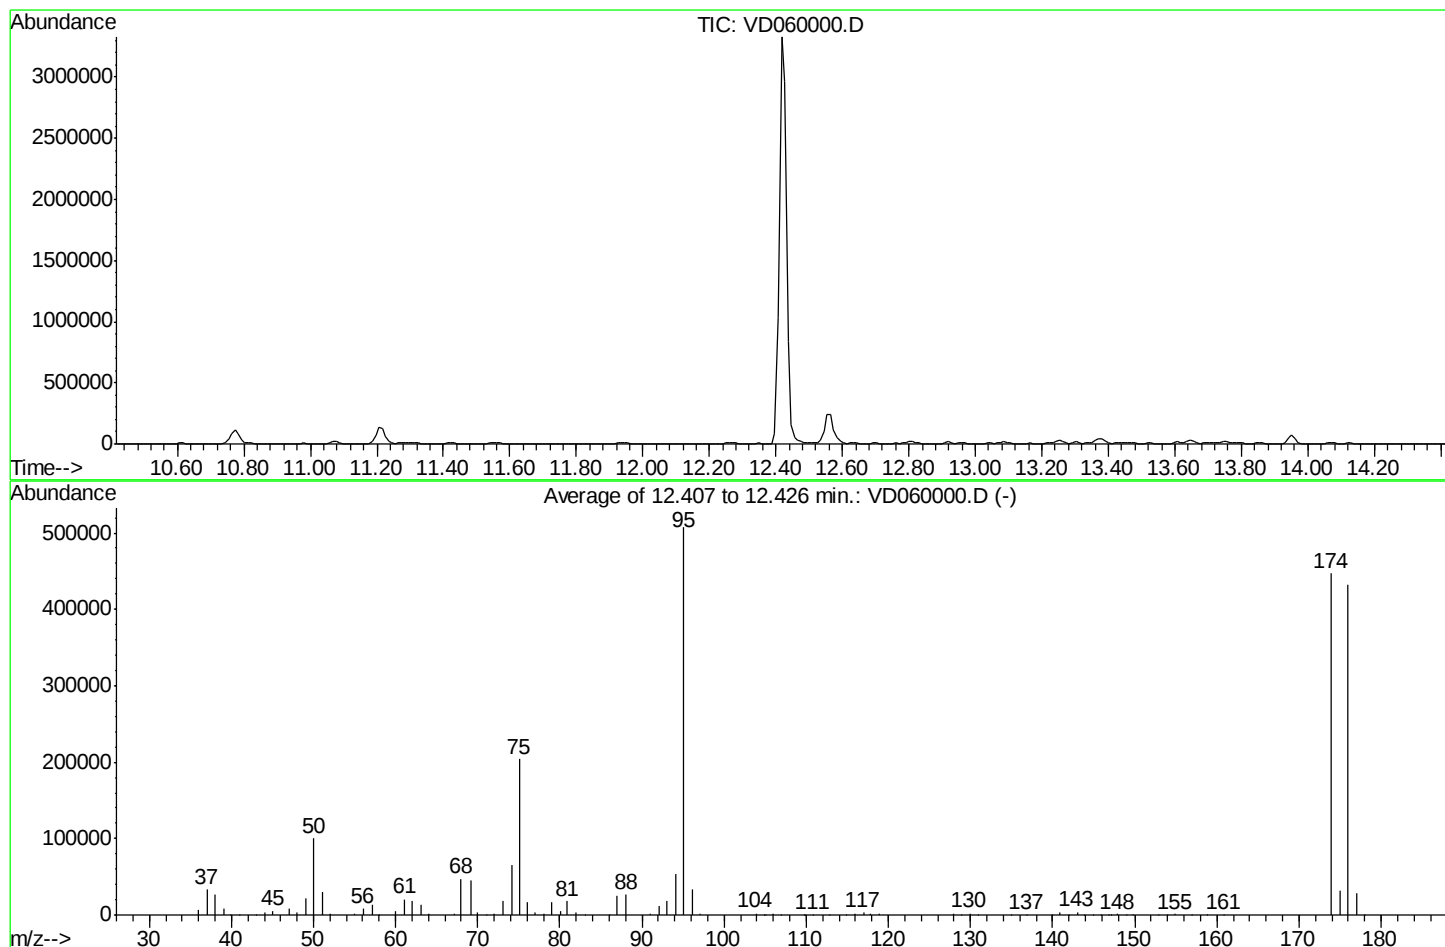

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1101

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.7      | 100197  | PASS             |
| 75          | 95           | 30           | 60           | 40.2      | 203952  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 507349  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 34202   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 88.0      | 446562  | PASS             |
| 175         | 174          | 5            | 9            | 7.3       | 32487   | PASS             |
| 176         | 174          | 95           | 101          | 96.6      | 431552  | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 29039   | PASS             |