
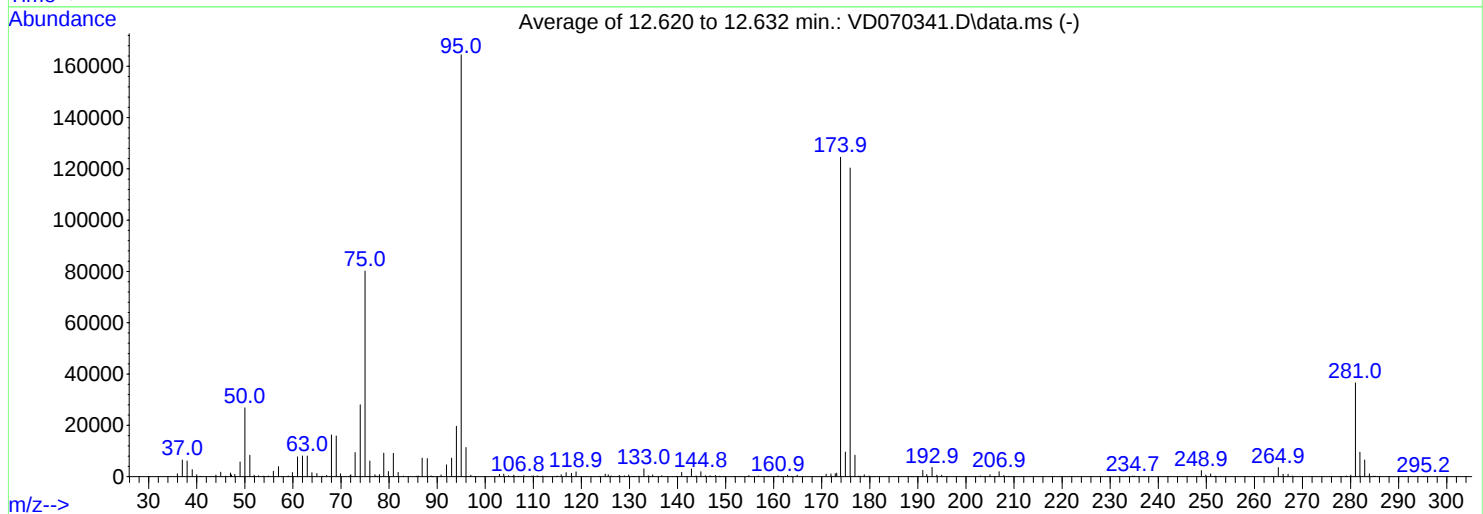


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091421\
 Data File : VD070341.D
 Acq On : 14 Sep 2021 09:14
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
 Title : SW846 8260
 Last Update : Thu Sep 09 03:07:09 2021

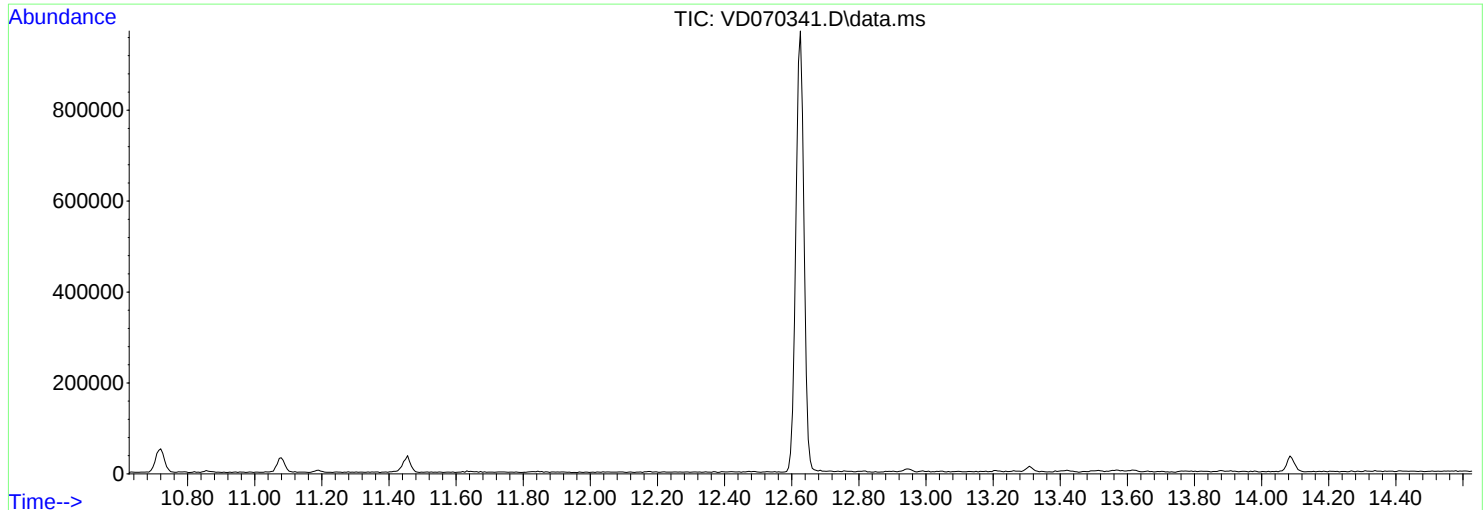

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	26848	PASS
75	95	30	60	48.7	80160	PASS
95	95	100	100	100.0	164459	PASS
96	95	5	9	6.9	11333	PASS
173	174	0.00	2	1.1	1385	PASS
174	95	50	100	75.7	124517	PASS
175	174	5	9	7.7	9602	PASS
176	174	95	101	96.7	120349	PASS
177	176	5	9	6.9	8339	PASS