

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091422\
 Data File : VD074297.D
 Acq On : 14 Sep 2022 21:06
 Operator : VA/SY
 Sample : N4579-07RE
 Misc : 2.04G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CHERRY-HILL-COMP-12RE

Quant Time: Sep 15 04:16:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090922S.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 10 04:45:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	104741	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	192654	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.575	117	173390	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.510	152	78115	50.000	ug/l	0.01

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	40991	38.387	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	76.780%
35) Dibromofluoromethane	7.805	113	43742	32.793	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	65.580%
50) Toluene-d8	10.269	98	157315	33.312	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	66.620%
62) 4-Bromofluorobenzene	12.569	95	49489	26.793	ug/l	0.01
Spiked Amount	50.000	Range	25 - 144	Recovery	=	53.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091422\
Data File : VD074297.D
Acq On : 14 Sep 2022 21:06
Operator : VA/SY
Sample : N4579-07RE
Misc : 2.04G/5.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CHERRY-HILL-COMP-12RE

Quant Time: Sep 15 04:16:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090922S.M
Quant Title : SW846 8260
QLast Update : Sat Sep 10 04:45:19 2022
Response via : Initial Calibration




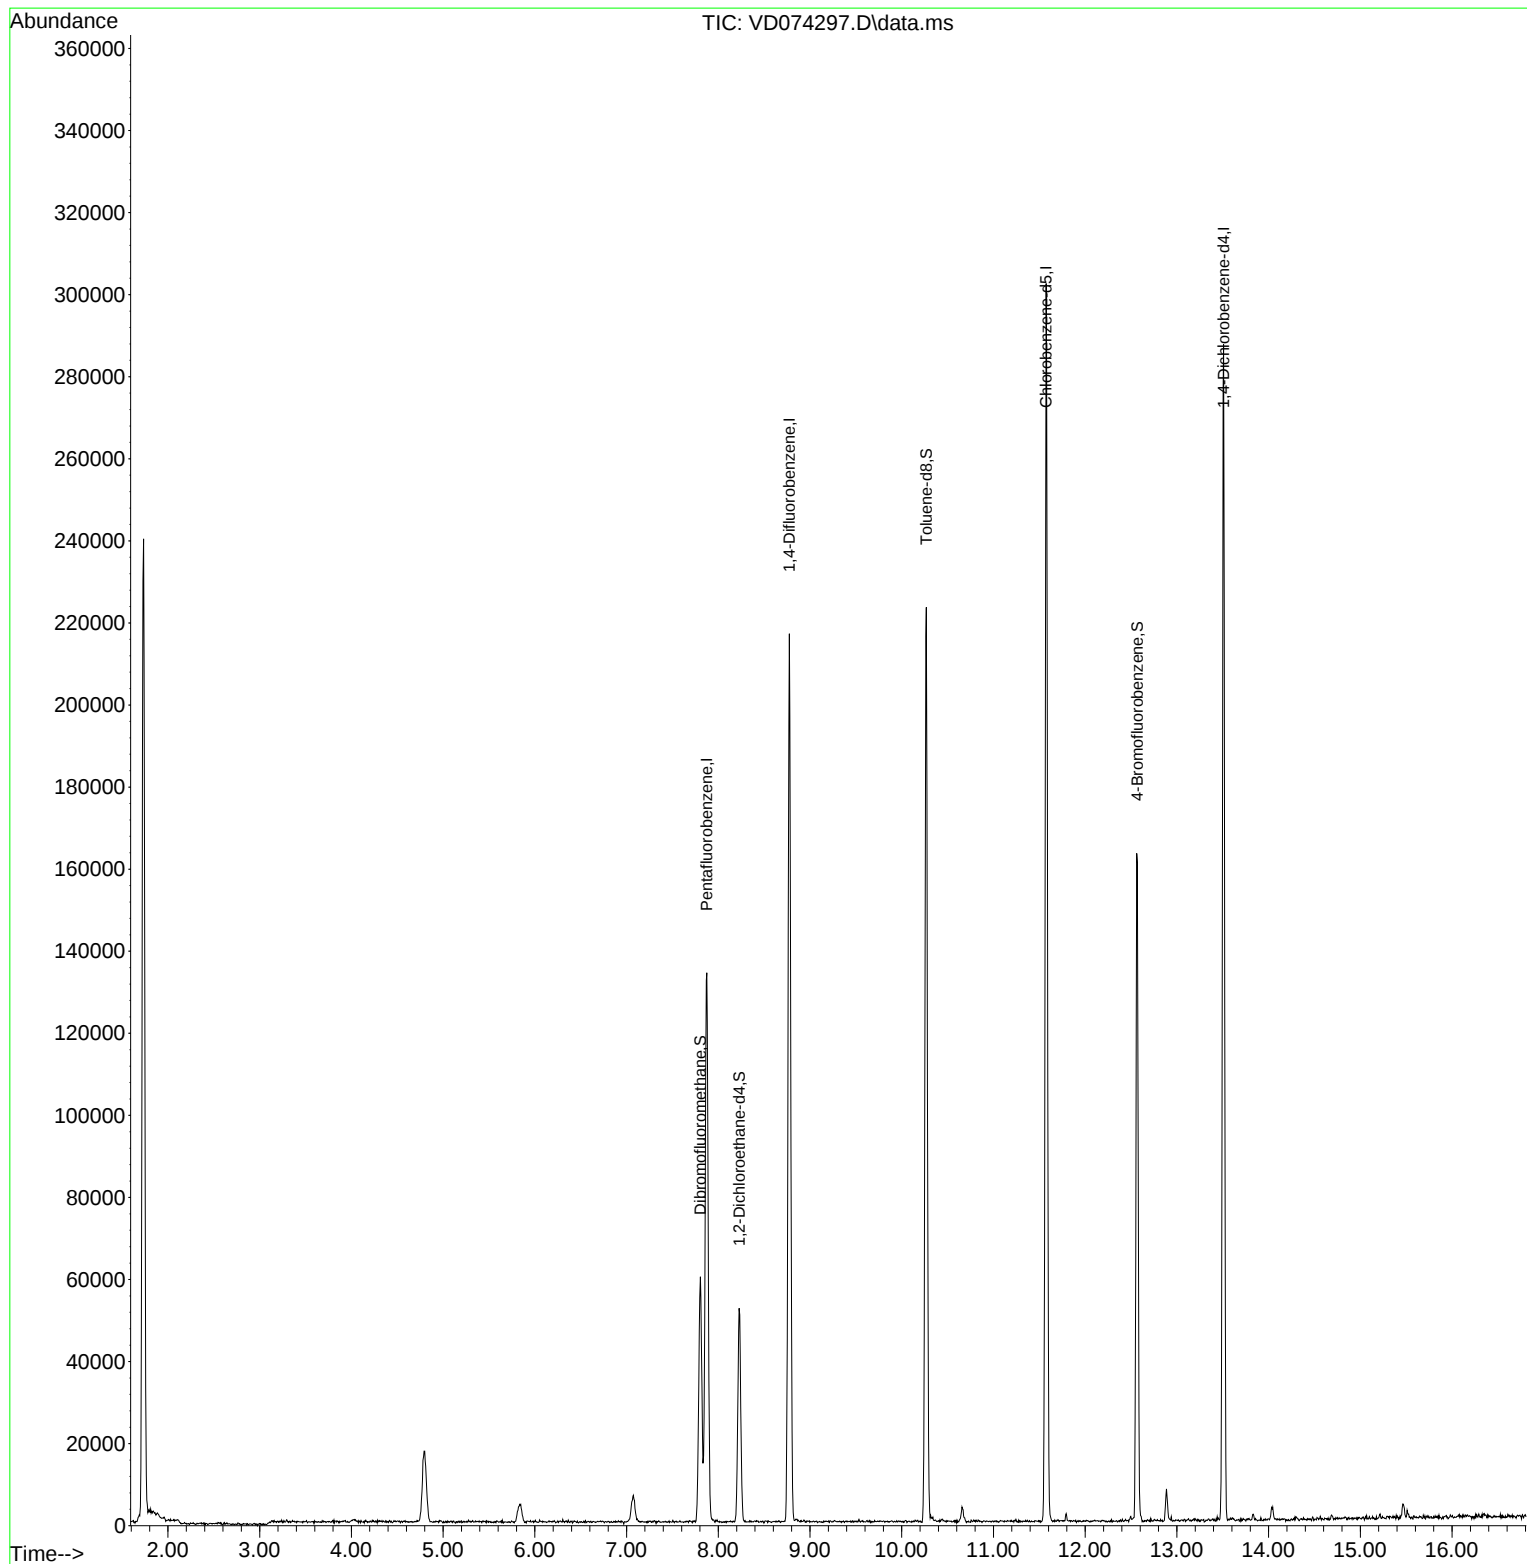


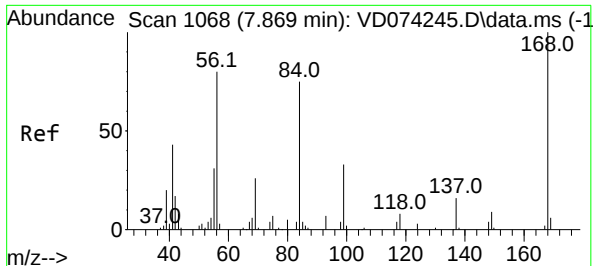

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1109
Delta R.T. 0.006 min
Lab File: VD074297.D
Acq: 14 Sep 2022 21:06




Instrument :
MSVOA_D
ClientSampleId :
CHERRY-HILL-COMP-12RE


Tgt Ion:168 Resp: 104741
Ion Ratio Lower Upper
168 100
99 56.5 43.0 64.6

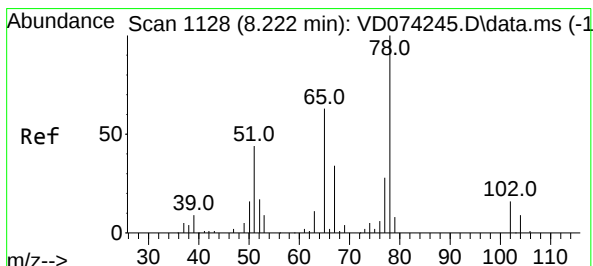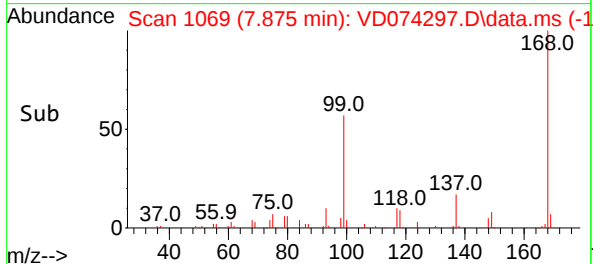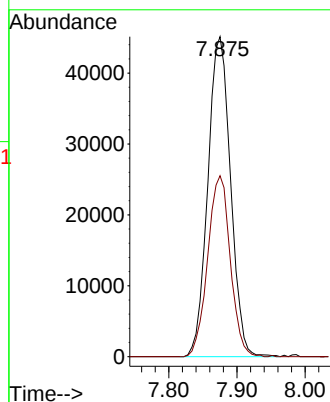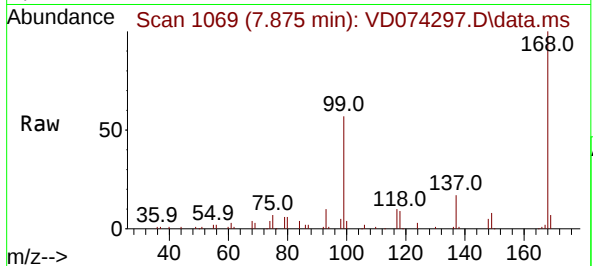

#33
1,2-Dichloroethane-d4
Concen: 38.387 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. 0.006 min
Lab File: VD074297.D
Acq: 14 Sep 2022 21:06

Tgt Ion: 65 Resp: 40991
Ion Ratio Lower Upper
65 100
67 53.7 0.0 110.6

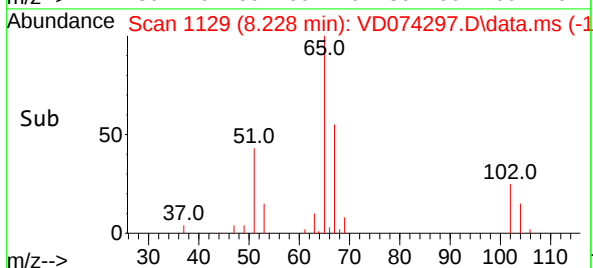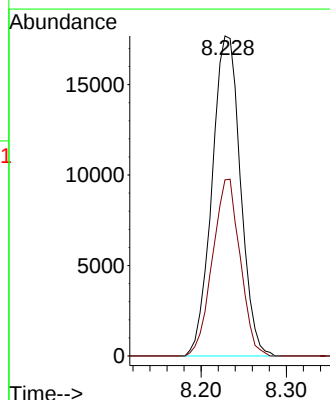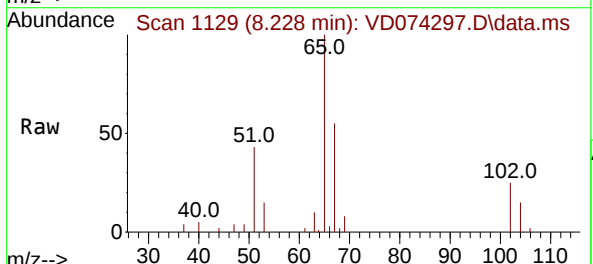

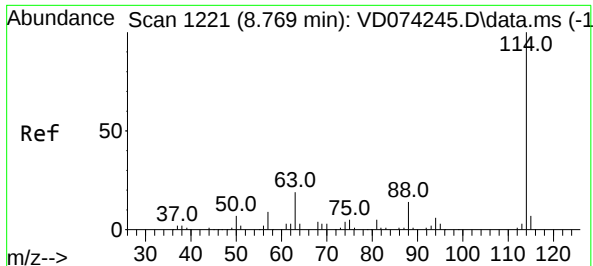

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD074297.D

Acq: 14 Sep 2022 21:06

Instrument :

MSVOA_D

ClientSampleId :

CHERRY-HILL-COMP-12RE





Tgt Ion:114 Resp: 192654

Ion Ratio Lower Upper

114 100

63 20.1 0.0 37.6

88 13.8 0.0 28.4

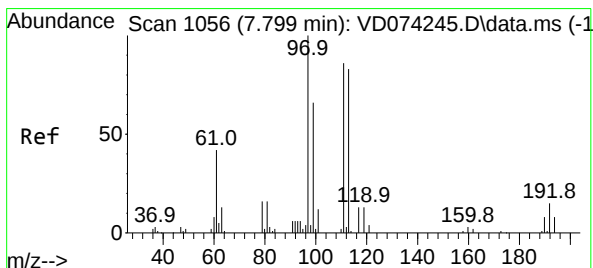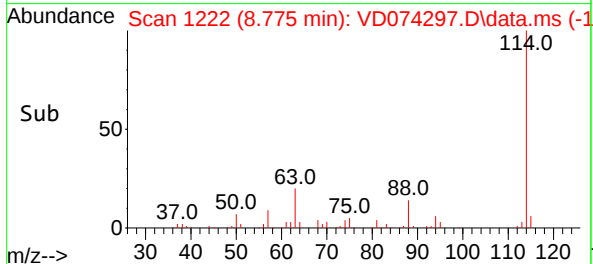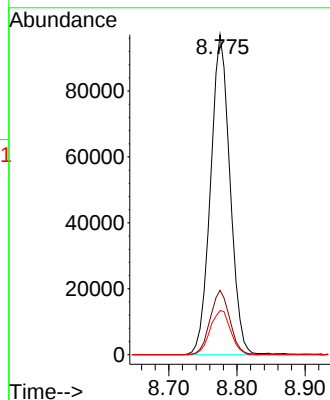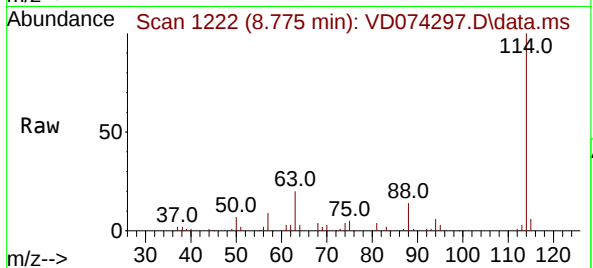

#35

Dibromofluoromethane

Concen: 32.793 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VD074297.D

Acq: 14 Sep 2022 21:06




Tgt Ion:113 Resp: 43742


Ion Ratio Lower Upper

113 100

111 103.3 83.0 124.6

192 17.8 16.2 24.2


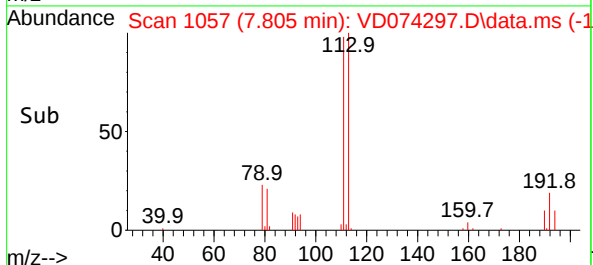
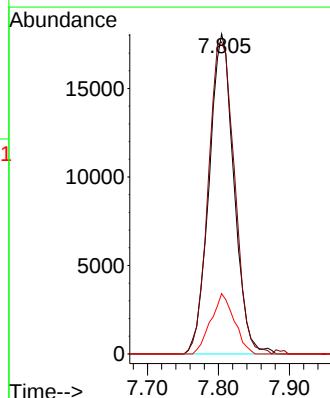
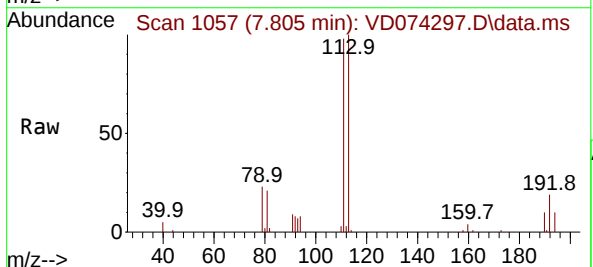


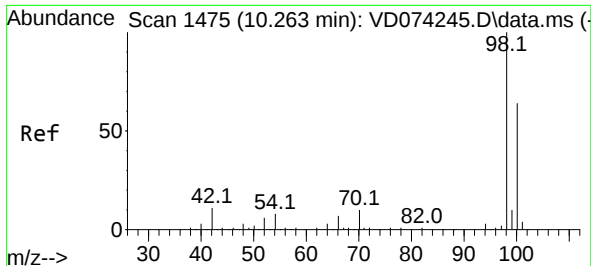

#50
Toluene-d8
Concen: 33.312 ug/l
RT: 10.269 min Scan# 1475
Delta R.T. 0.006 min
Lab File: VD074297.D
Acq: 14 Sep 2022 21:06




Instrument :
MSVOA_D
ClientSampleId :
CHERRY-HILL-COMP-12RE


Tgt Ion: 98 Resp: 157315
Ion Ratio Lower Upper
98 100
100 63.1 51.8 77.8

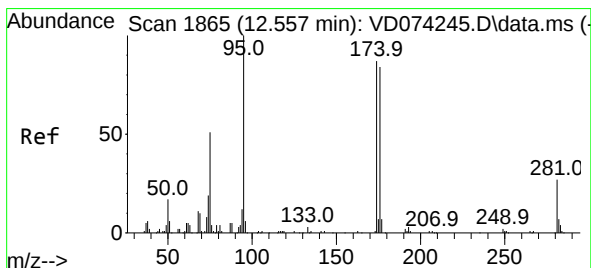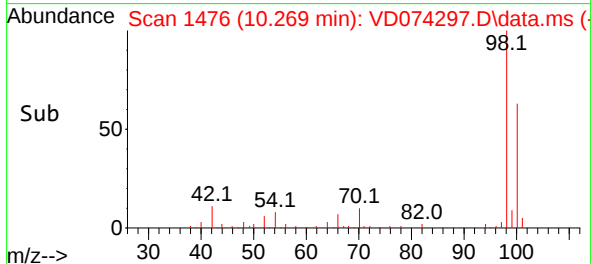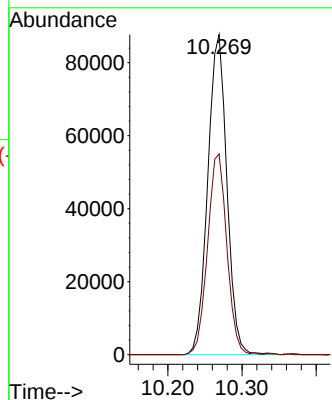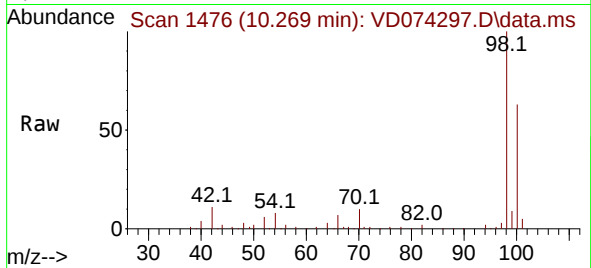

#62
4-Bromofluorobenzene
Concen: 26.793 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. 0.012 min
Lab File: VD074297.D
Acq: 14 Sep 2022 21:06

Tgt Ion: 95 Resp: 49489
Ion Ratio Lower Upper
95 100
174 86.9 0.0 179.2
176 85.2 0.0 171.4


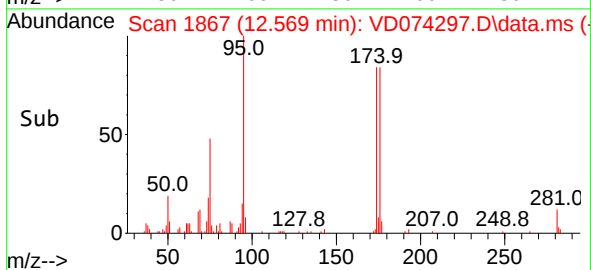
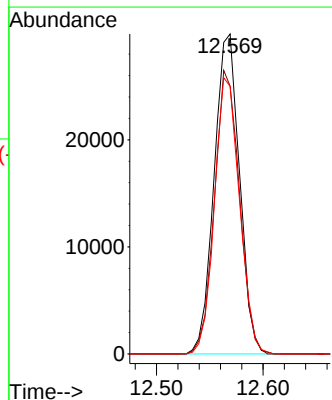
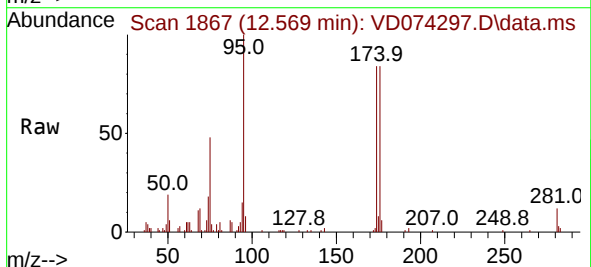


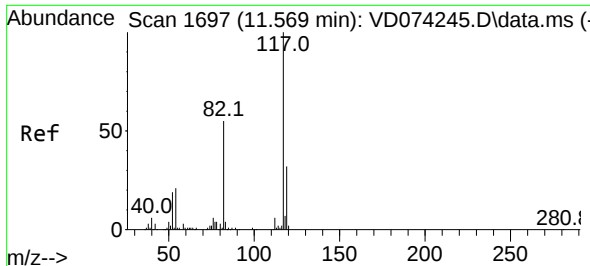

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.575 min Scan# 11
Delta R.T. 0.006 min
Lab File: VD074297.D
Acq: 14 Sep 2022 21:06

Instrument :
MSVOA_D
ClientSampleId :
CHERRY-HILL-COMP-12RE

Tgt Ion:117 Resp: 173390
Ion Ratio Lower Upper
117 100
82 53.3 44.2 66.2
119 33.3 25.4 38.0

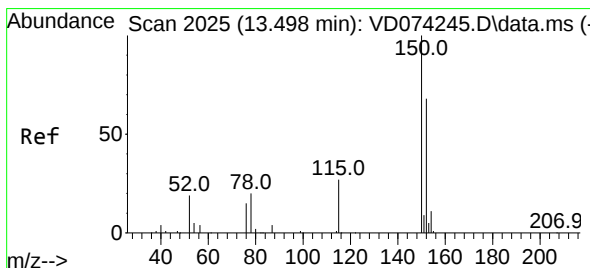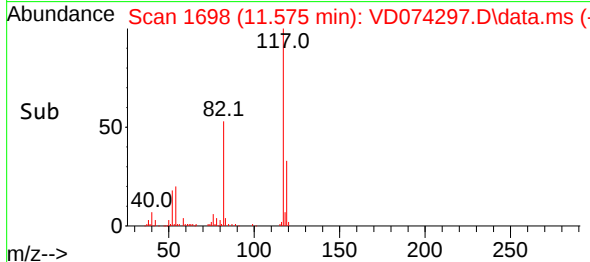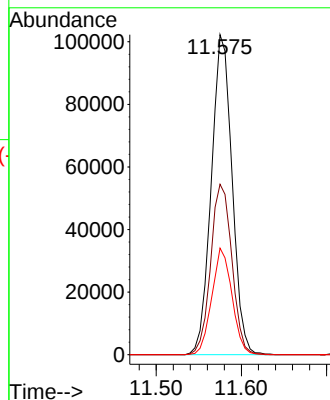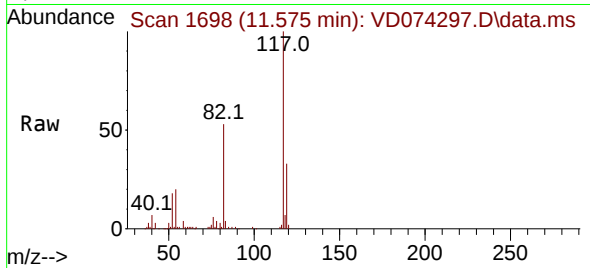

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.510 min Scan# 2027
Delta R.T. 0.012 min
Lab File: VD074297.D
Acq: 14 Sep 2022 21:06

Tgt Ion:152 Resp: 78115
Ion Ratio Lower Upper
152 100
115 55.8 28.4 85.2
150 157.4 0.0 351.0

