



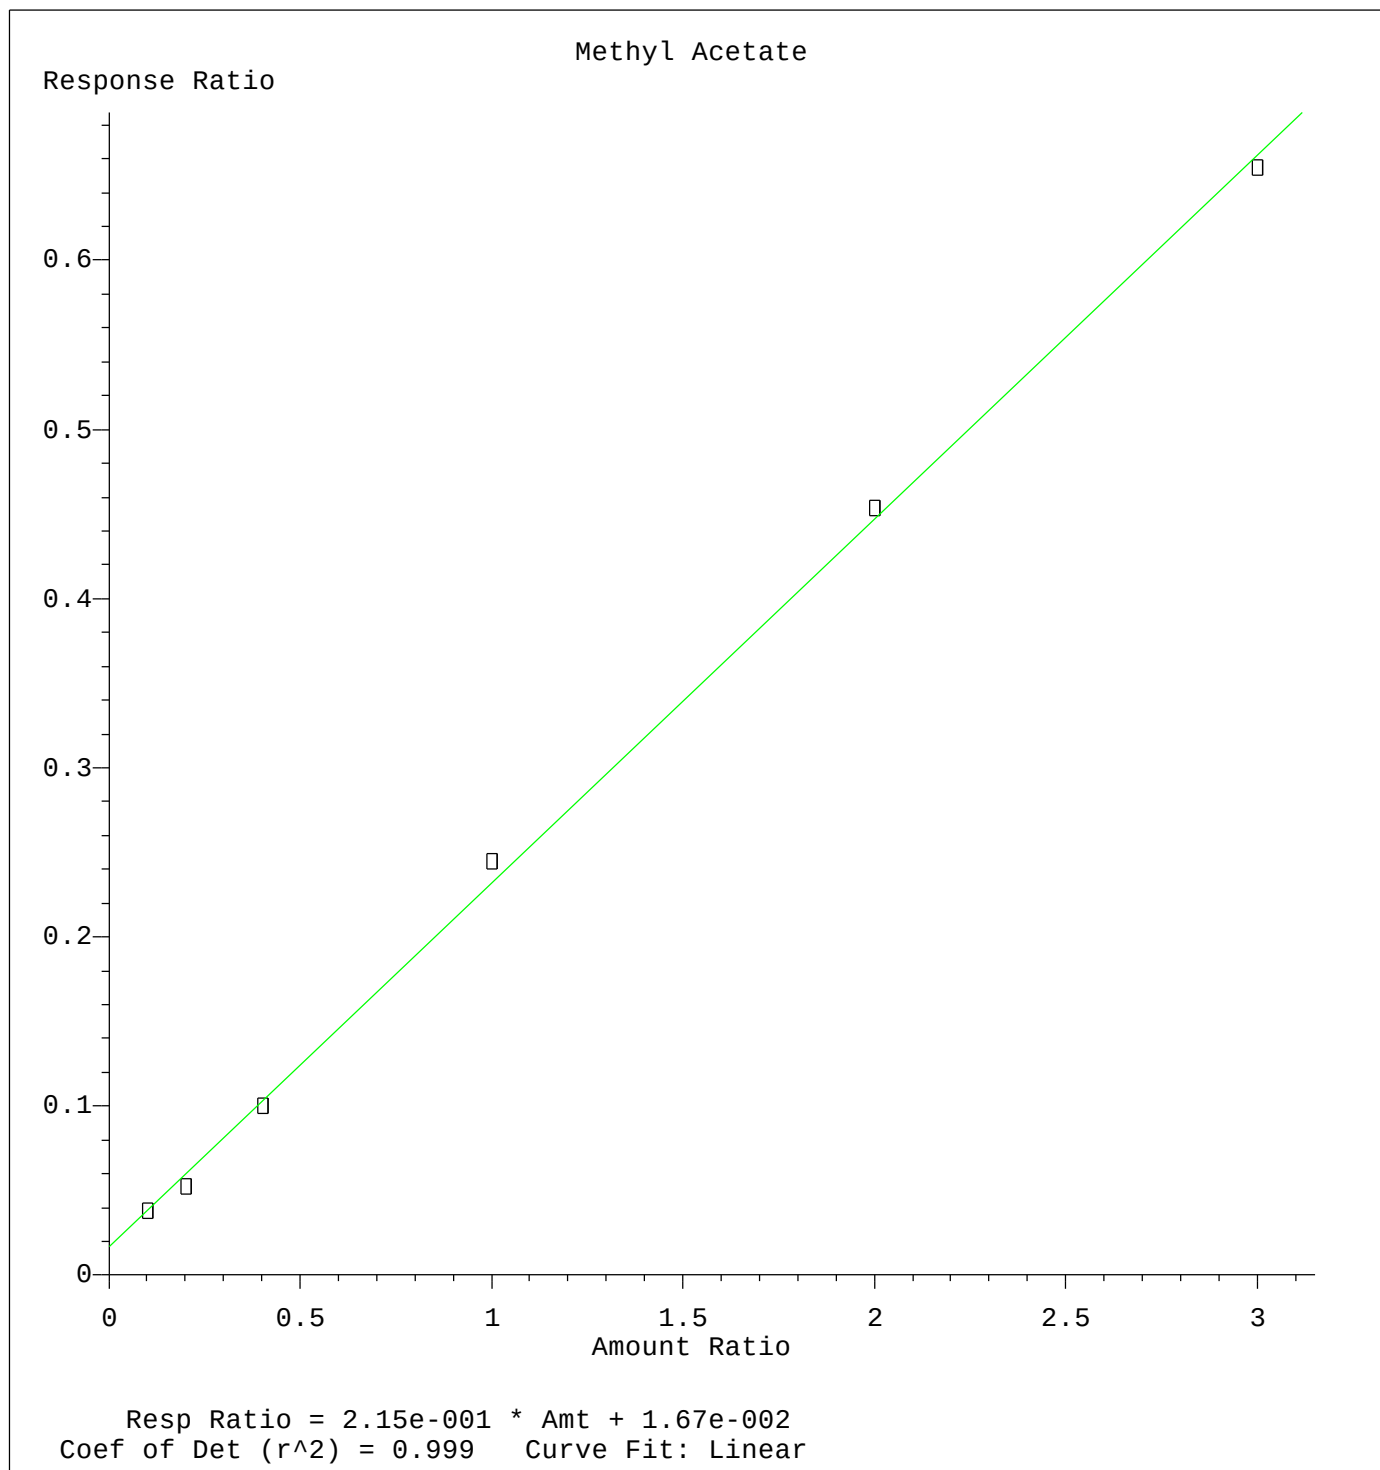


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091520S.M
Calibration Table Last Updated: Tue Sep 15 16:35:37 2020

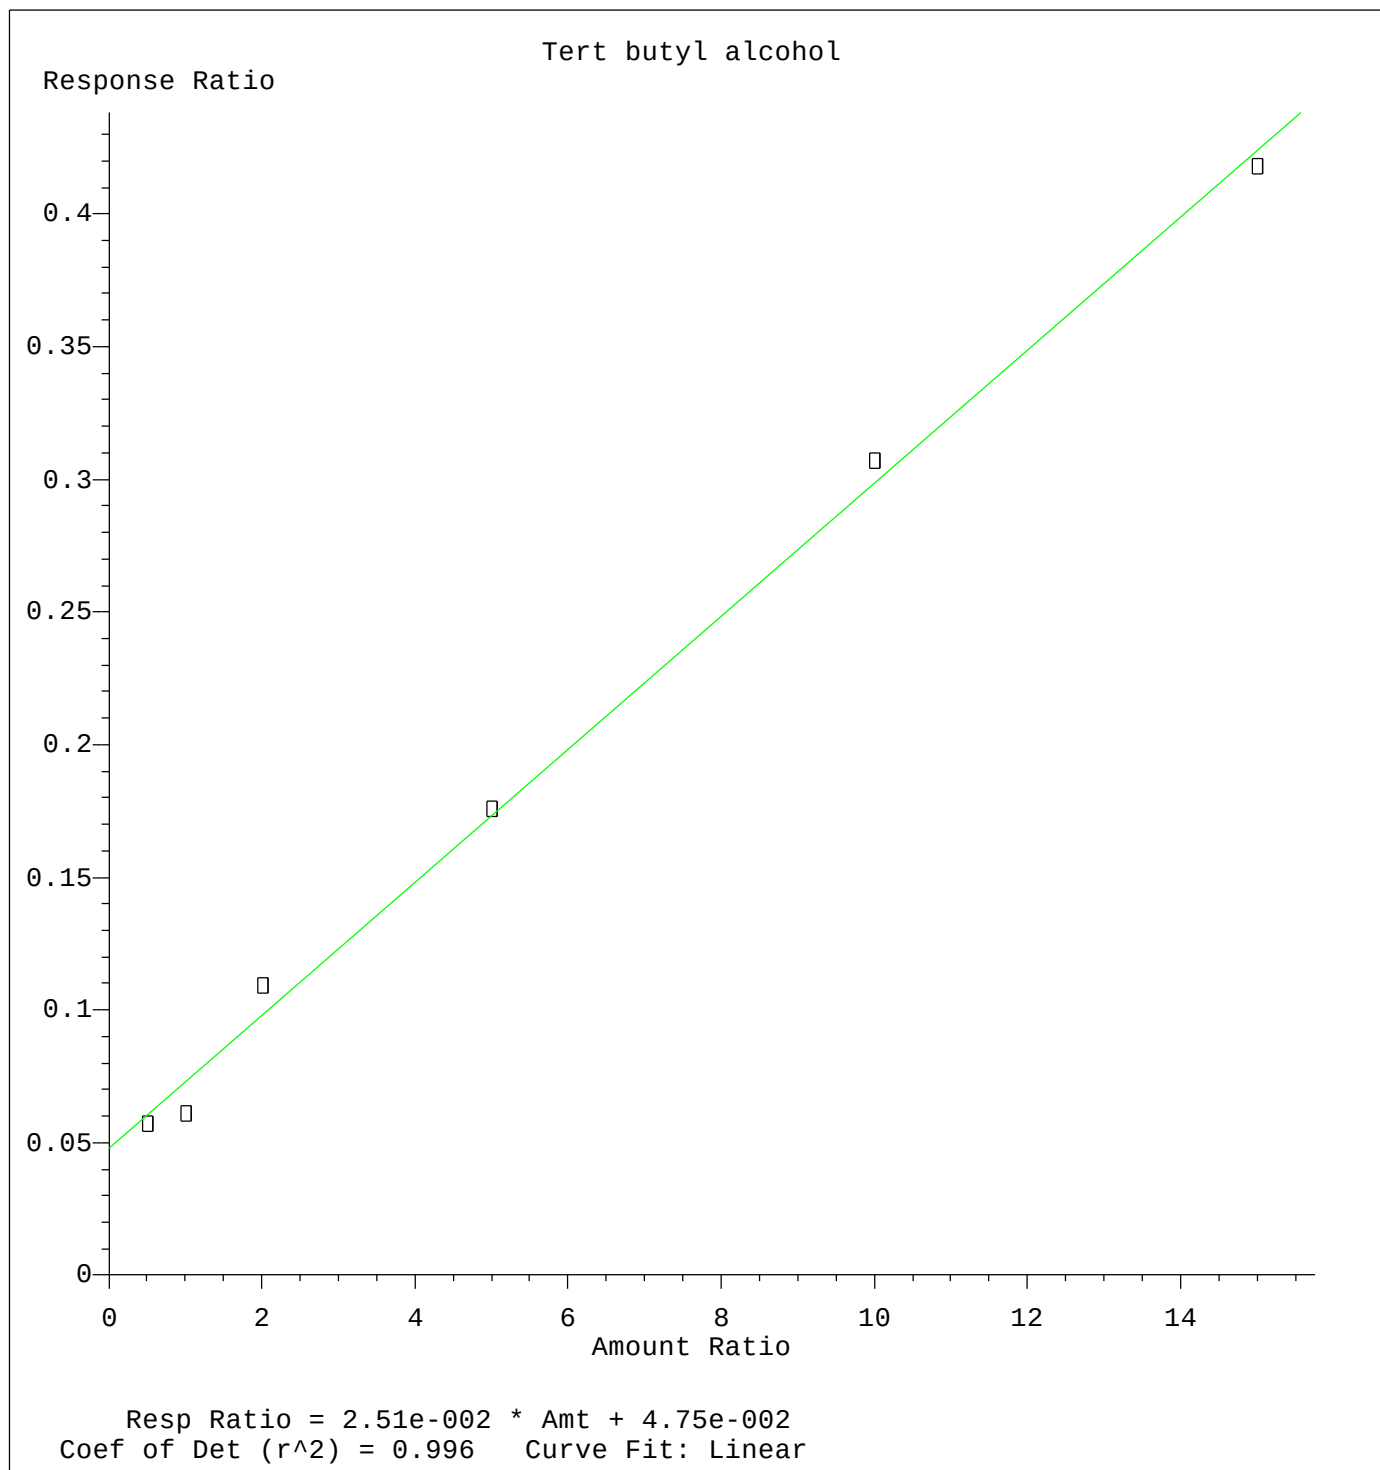

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091520S.M
Calibration Table Last Updated: Tue Sep 15 16:35:37 2020

Dichlorodifluoromethane

Response Ratio

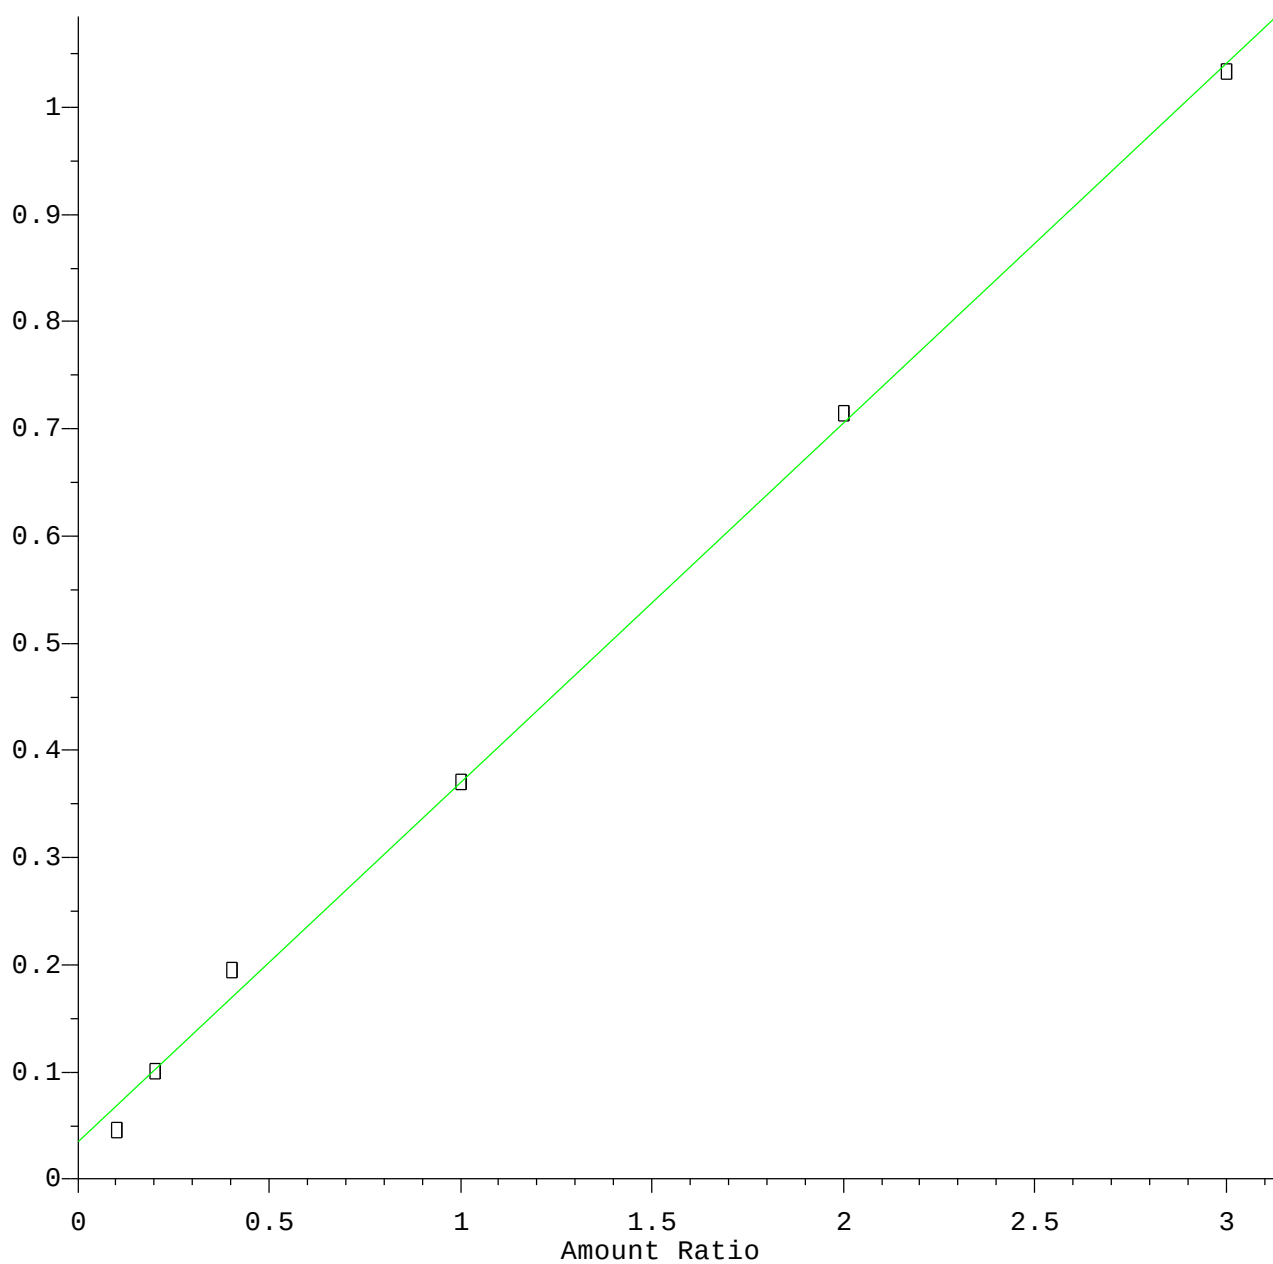


Resp Ratio = $3.35 \times 10^{-1} \times \text{Amt} + 3.49 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091520S.M
Calibration Table Last Updated: Tue Sep 15 16:35:37 2020

Methylene Chloride

Response Ratio

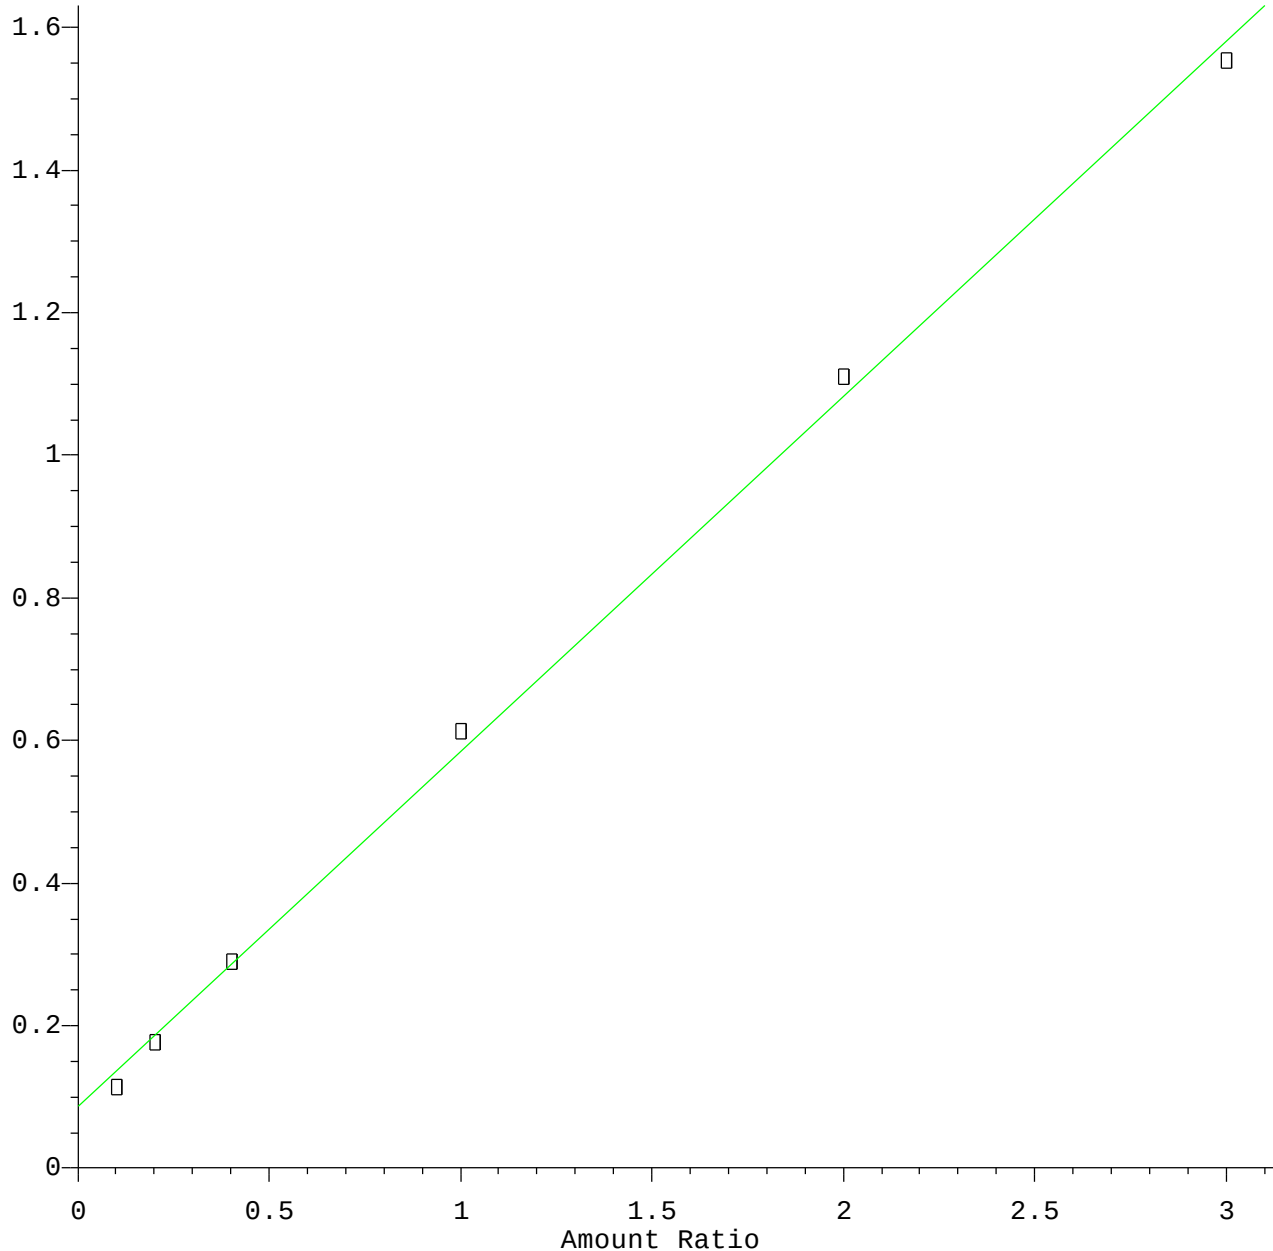

Resp Ratio = $4.98 \times 10^{-1} \times \text{Amt} + 8.60 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091520S.M
Calibration Table Last Updated: Tue Sep 15 16:35:37 2020