


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD091520\
 Data File : VD066694.D
 Acq On : 15 Sep 2020 12:30
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091520S.M
 Title : SW846 8260
 Last Update : Tue Sep 15 16:35:37 2020

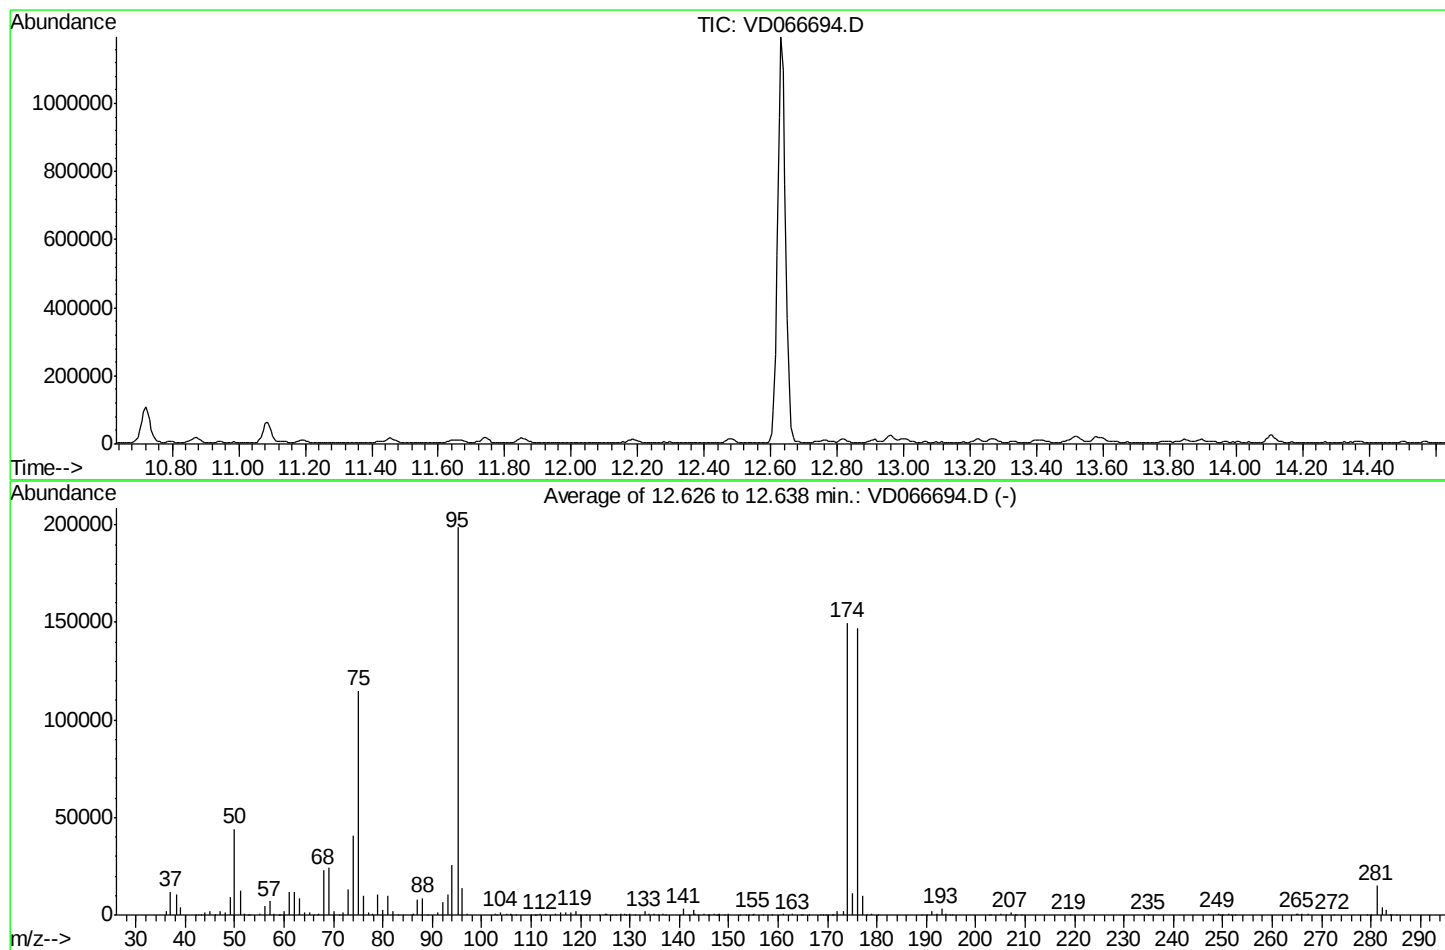

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	44197	PASS
75	95	30	60	57.8	114896	PASS
95	95	100	100	100.0	198762	PASS
96	95	5	9	6.9	13706	PASS
173	174	0.00	2	1.5	2215	PASS
174	95	50	100	75.4	149914	PASS
175	174	5	9	7.4	11100	PASS
176	174	95	101	98.2	147197	PASS
177	176	5	9	6.9	10189	PASS