
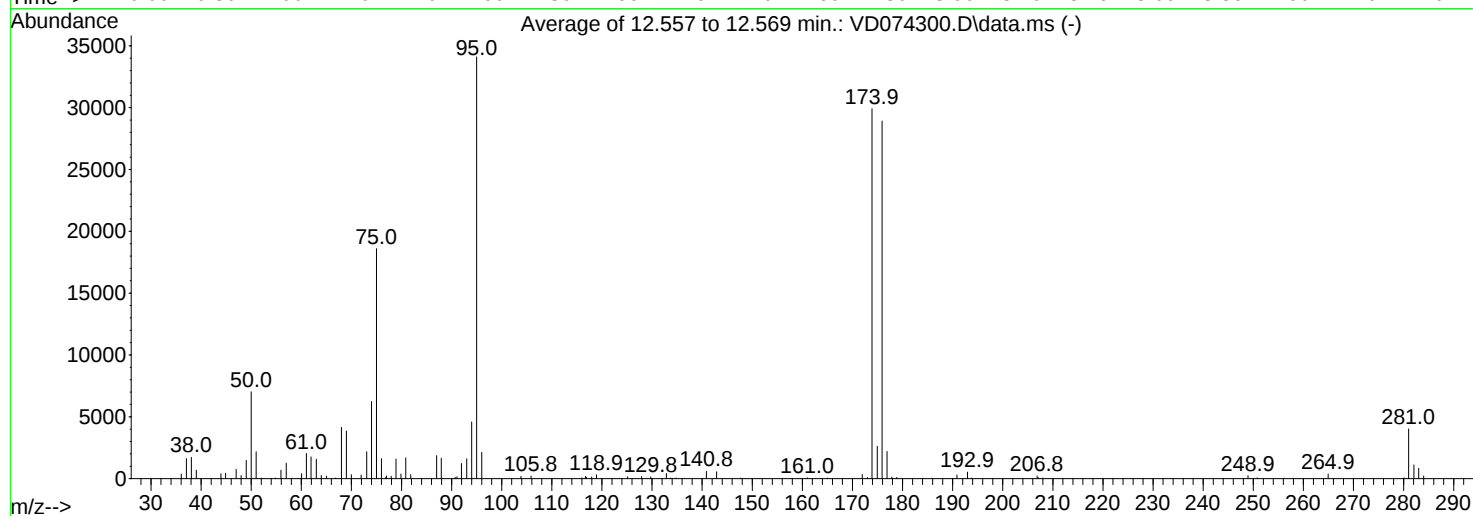


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091522\
 Data File : VD074300.D
 Acq On : 15 Sep 2022 10:02
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090922S.M
 Title : SW846 8260
 Last Update : Sat Sep 10 04:45:19 2022

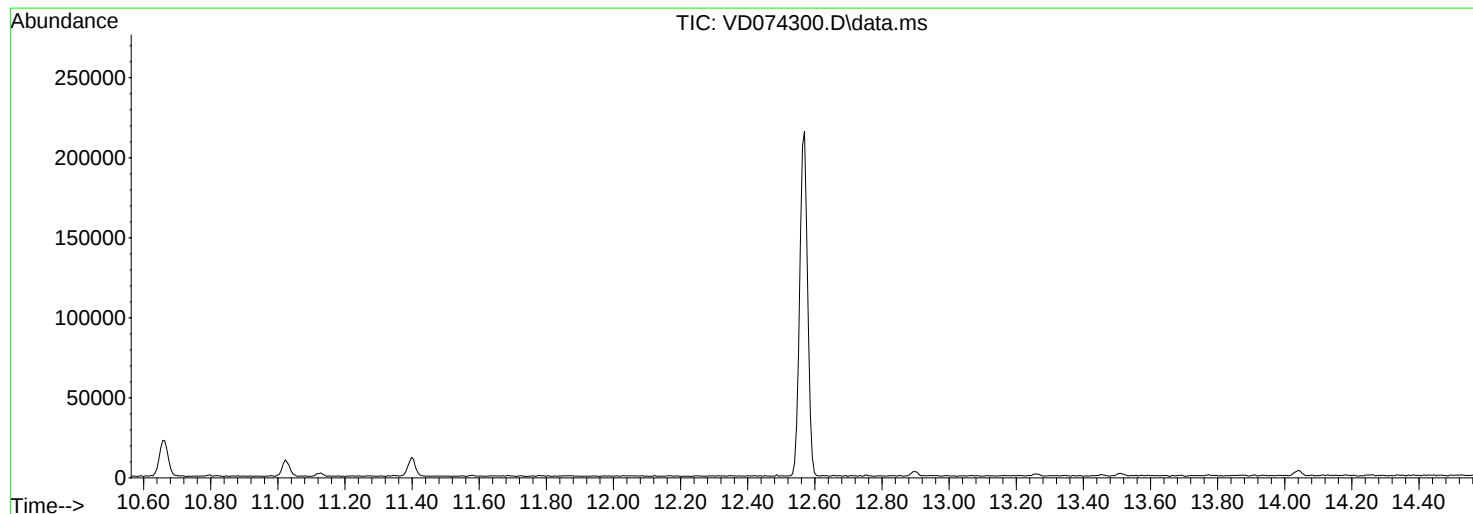

AutoFind: Scans 1865, 1866, 1867; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	7028	PASS
75	95	30	60	54.5	18591	PASS
95	95	100	100	100.0	34109	PASS
96	95	5	9	6.2	2126	PASS
173	174	0.00	2	0.3	93	PASS
174	95	50	100	87.7	29915	PASS
175	174	5	9	8.8	2621	PASS
176	174	95	101	96.7	28920	PASS
177	176	5	9	7.6	2202	PASS