
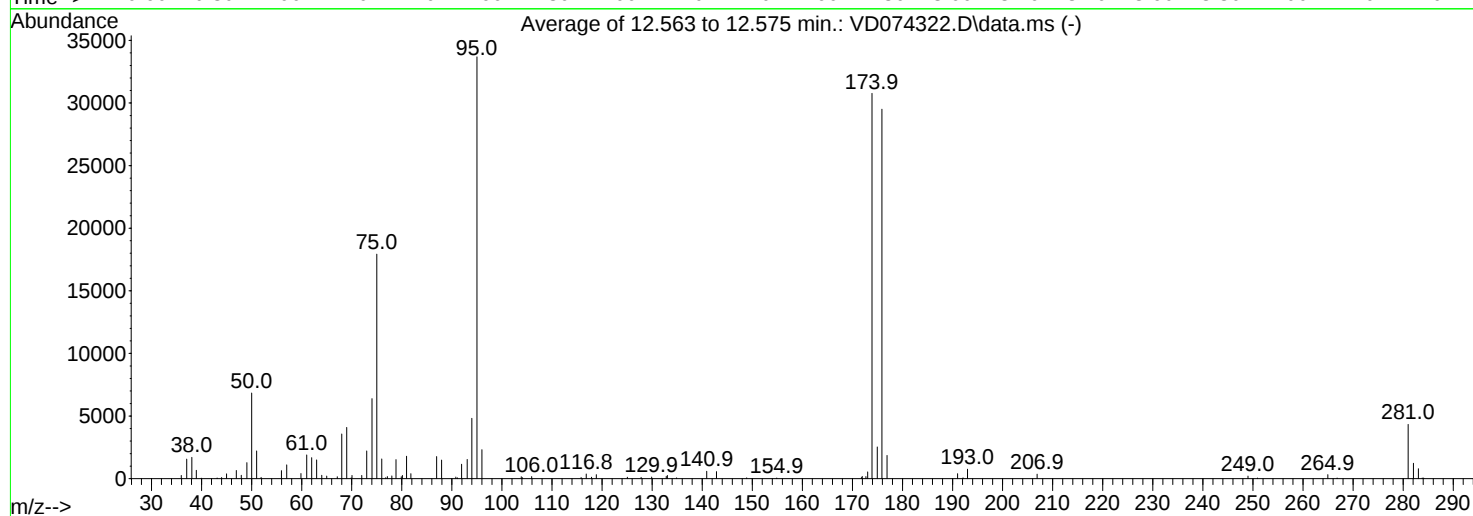


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091622\
Data File : VD074322.D
Acq On : 16 Sep 2022 09:39
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D091622S.M
Title : SW846 8260
Last Update : Sat Sep 17 04:16:54 2022

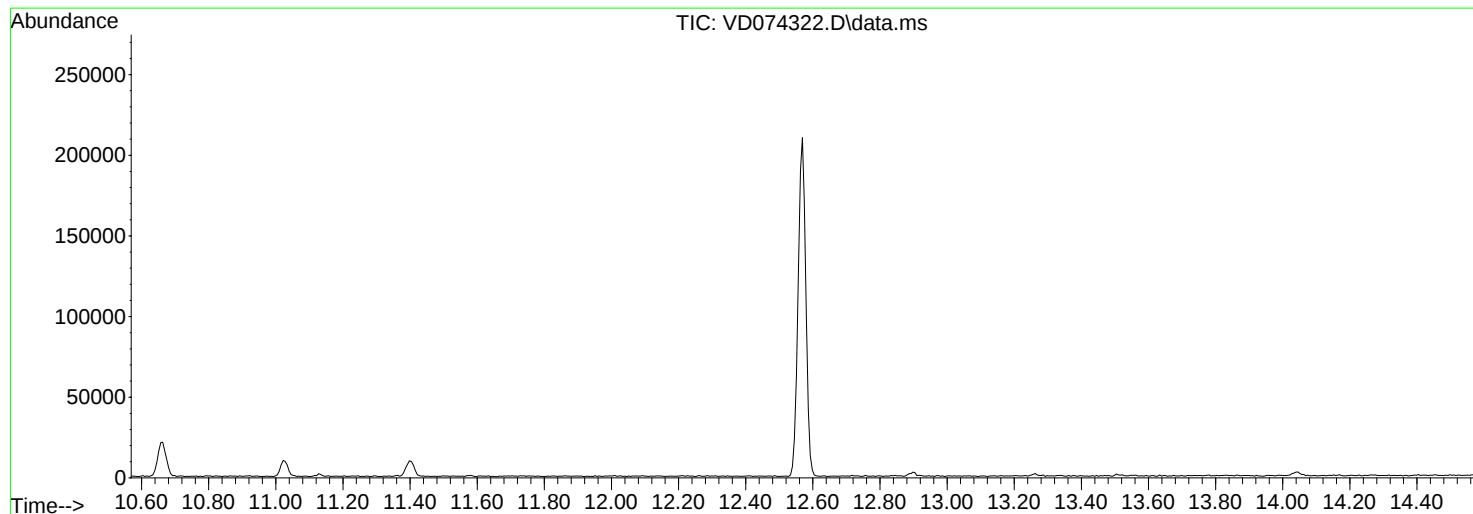

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	6838	PASS
75	95	30	60	53.2	17924	PASS
95	95	100	100	100.0	33688	PASS
96	95	5	9	6.9	2318	PASS
173	174	0.00	2	1.8	540	PASS
174	95	50	100	91.3	30768	PASS
175	174	5	9	8.2	2535	PASS
176	174	95	101	95.9	29504	PASS
177	176	5	9	6.3	1854	PASS