
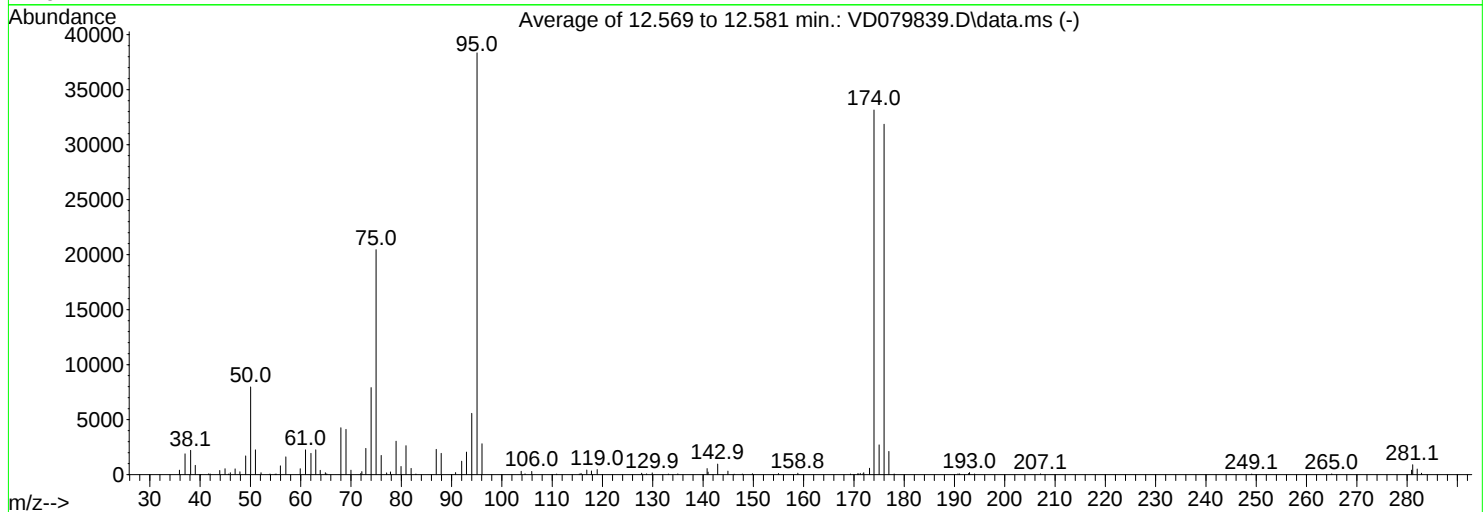


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091624\
Data File : VD079839.D
Acq On : 16 Sep 2024 10:44
Operator : RP/MD
Sample : BFB829
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB829

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Tue Sep 17 04:25:03 2024

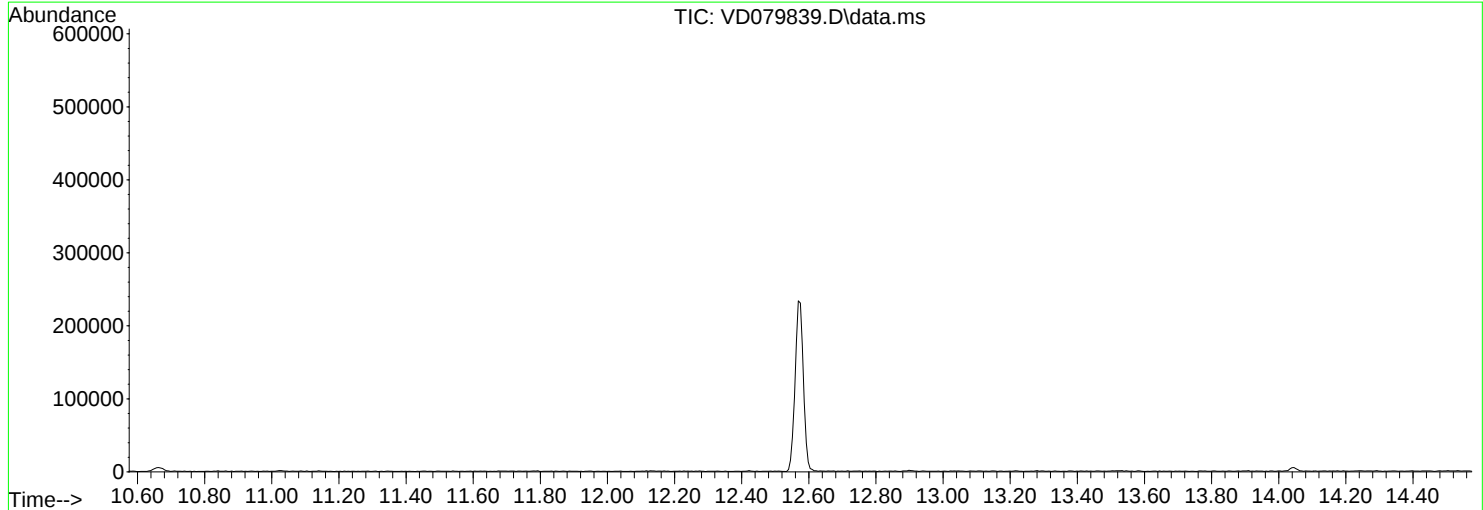

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	7970	PASS
75	95	30	80	53.3	20452	PASS
95	95	100	100	100.0	38347	PASS
96	95	5	9	7.3	2805	PASS
173	174	0.00	2	1.8	583	PASS
174	95	50	120	86.5	33155	PASS
175	174	5	9	8.2	2710	PASS
176	174	95	105	96.1	31859	PASS
177	176	5	10	6.6	2117	PASS

m/z	Abundance
40.10	516.0
43.90	260.0

Instrument :
MSVOA_D
ClientSampleId :
BFB829

m/z	Abundance
35.90	448.0
37.00	2387.0
38.10	2481.0
39.10	1025.0
39.90	573.0
44.00	578.0
45.00	646.0
46.00	187.0
47.00	503.0
47.80	281.0
49.10	1833.0
50.00	8484.0
51.00	2621.0
52.10	181.0
56.00	1062.0
57.10	1880.0
60.00	518.0
61.00	2617.0
62.00	2413.0
63.00	2830.0
63.90	421.0
64.90	229.0
68.00	4977.0
69.00	4043.0
70.00	235.0
72.20	448.0
73.00	3099.0
74.00	8589.0
75.00	22992.0
76.00	1937.0
77.10	298.0
77.90	275.0
78.90	3108.0
79.90	937.0
81.00	2862.0
82.10	553.0
87.00	2080.0
87.90	1730.0
90.80	265.0
92.00	1419.0
93.00	2387.0
94.00	6734.0
95.10	40800.0
96.00	3433.0
103.90	336.0
105.90	356.0
110.90	165.0
115.40	179.0
115.80	171.0
116.90	505.0
117.80	268.0
118.90	559.0
129.90	258.0
140.80	1185.0
142.90	820.0
144.90	258.0
149.80	249.0
155.00	294.0
169.30	157.0
170.70	199.0
171.80	235.0
173.10	949.0
174.00	36256.0
175.00	3039.0
176.00	34784.0
176.90	2360.0
178.00	164.0
190.70	220.0
192.80	300.0
194.00	171.0
249.10	157.0
265.00	238.0
280.90	1217.0
282.10	553.0
282.90	171.0

Instrument :
MSVOA_D
ClientSampleId :
BFB829

m/z	Abundance
35.90	508.0
37.00	1837.0
38.10	2555.0
39.10	795.0
39.80	416.0
42.00	162.0
44.00	708.0
44.90	689.0
45.90	188.0
46.90	790.0
47.90	333.0
49.00	2050.0
50.10	8893.0
51.00	1910.0
52.10	331.0
54.90	154.0
55.90	936.0
57.00	1616.0
59.80	664.0
61.00	2295.0
62.10	1684.0
63.00	2259.0
63.90	379.0
65.20	223.0
68.00	4149.0
69.00	4444.0
70.00	667.0
72.10	367.0
72.90	2291.0
74.00	8778.0
75.00	22992.0
76.00	1767.0
77.10	196.0
77.80	209.0
79.00	3310.0
80.00	652.0
80.90	3024.0
81.90	482.0
86.90	2604.0
88.00	2278.0
90.80	306.0
92.00	1336.0
92.90	2255.0
94.00	5813.0
95.00	43416.0
96.10	2784.0
103.90	283.0
105.90	275.0
117.00	304.0
117.80	491.0
119.00	584.0
127.80	414.0
128.80	204.0
129.90	216.0
141.00	716.0
143.00	1352.0
145.00	431.0
146.20	151.0
158.90	223.0
170.90	217.0
171.20	201.0
172.00	335.0
174.00	36768.0
175.00	2869.0
176.00	34200.0
177.00	2284.0
193.00	321.0
281.10	1074.0
281.90	616.0
282.80	206.0

Instrument :
MSVOA_D
ClientSampleId :
BFB829

m/z	Abundance
35.80	250.0
37.00	1435.0
38.10	1597.0
39.00	714.0
40.00	576.0
41.70	201.0
43.80	631.0
45.00	300.0
45.70	183.0
46.10	157.0
46.90	271.0
48.00	178.0
49.00	1244.0
50.10	6533.0
51.00	2259.0
53.90	174.0
55.10	172.0
55.90	417.0
57.00	1335.0
59.90	419.0
60.90	1856.0
62.00	1702.0
63.10	1670.0
63.90	401.0
64.90	304.0
68.00	3653.0
69.00	3880.0
70.00	308.0
71.90	258.0
73.00	1750.0
74.00	6379.0
75.00	15372.0
76.00	1518.0
77.90	277.0
78.90	2717.0
79.90	649.0
80.90	2038.0
81.90	664.0
82.90	196.0
87.00	2232.0
87.90	1809.0
92.00	897.0
93.00	1502.0
94.10	4154.0
95.00	30824.0
96.10	2197.0
103.80	280.0
104.60	198.0
106.00	251.0
115.70	185.0
116.80	458.0
117.90	250.0
118.90	271.0
133.10	169.0
135.00	214.0
140.80	469.0
142.80	702.0
144.90	272.0
147.80	175.0
158.80	154.0
171.30	172.0
171.90	192.0
173.10	800.0
174.00	26440.0
175.00	2223.0
176.00	26592.0
176.90	1708.0
191.00	230.0
193.00	260.0
207.10	222.0
281.10	1652.0
281.90	368.0

Instrument :
MSVOA_D
ClientSampleId :
BFB829