

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD091720\
 Data File : VD066739.D
 Acq On : 17 Sep 2020 12:47
 Operator : VA/SY
 Sample : L3868-01
 Misc : 7.28G/5.00ml/MSVOA D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 PL-02-091520

Quant Time: Sep 18 01:32:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091520S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 15 16:35:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.98
34) 1,4-Difluorobenzene	0.00	114	0m	50.00	ug/l	-8.86
63) Chlorobenzene-d5	0.00	117	0m	50.00	ug/l	-11.64
72) 1,4-Dichlorobenzene-d4	0.00	152	0m	50.00	ug/l	-13.58

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0d	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0d	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD091720\
Data File : VD066739.D
Acq On : 17 Sep 2020 12:47
Operator : VA/SY
Sample : L3868-01
Misc : 7.28G/5.00ml/MSVOA D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PL-02-091520

Quant Time: Sep 18 01:32:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D091520S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 15 16:35:37 2020
Response via : Initial Calibration

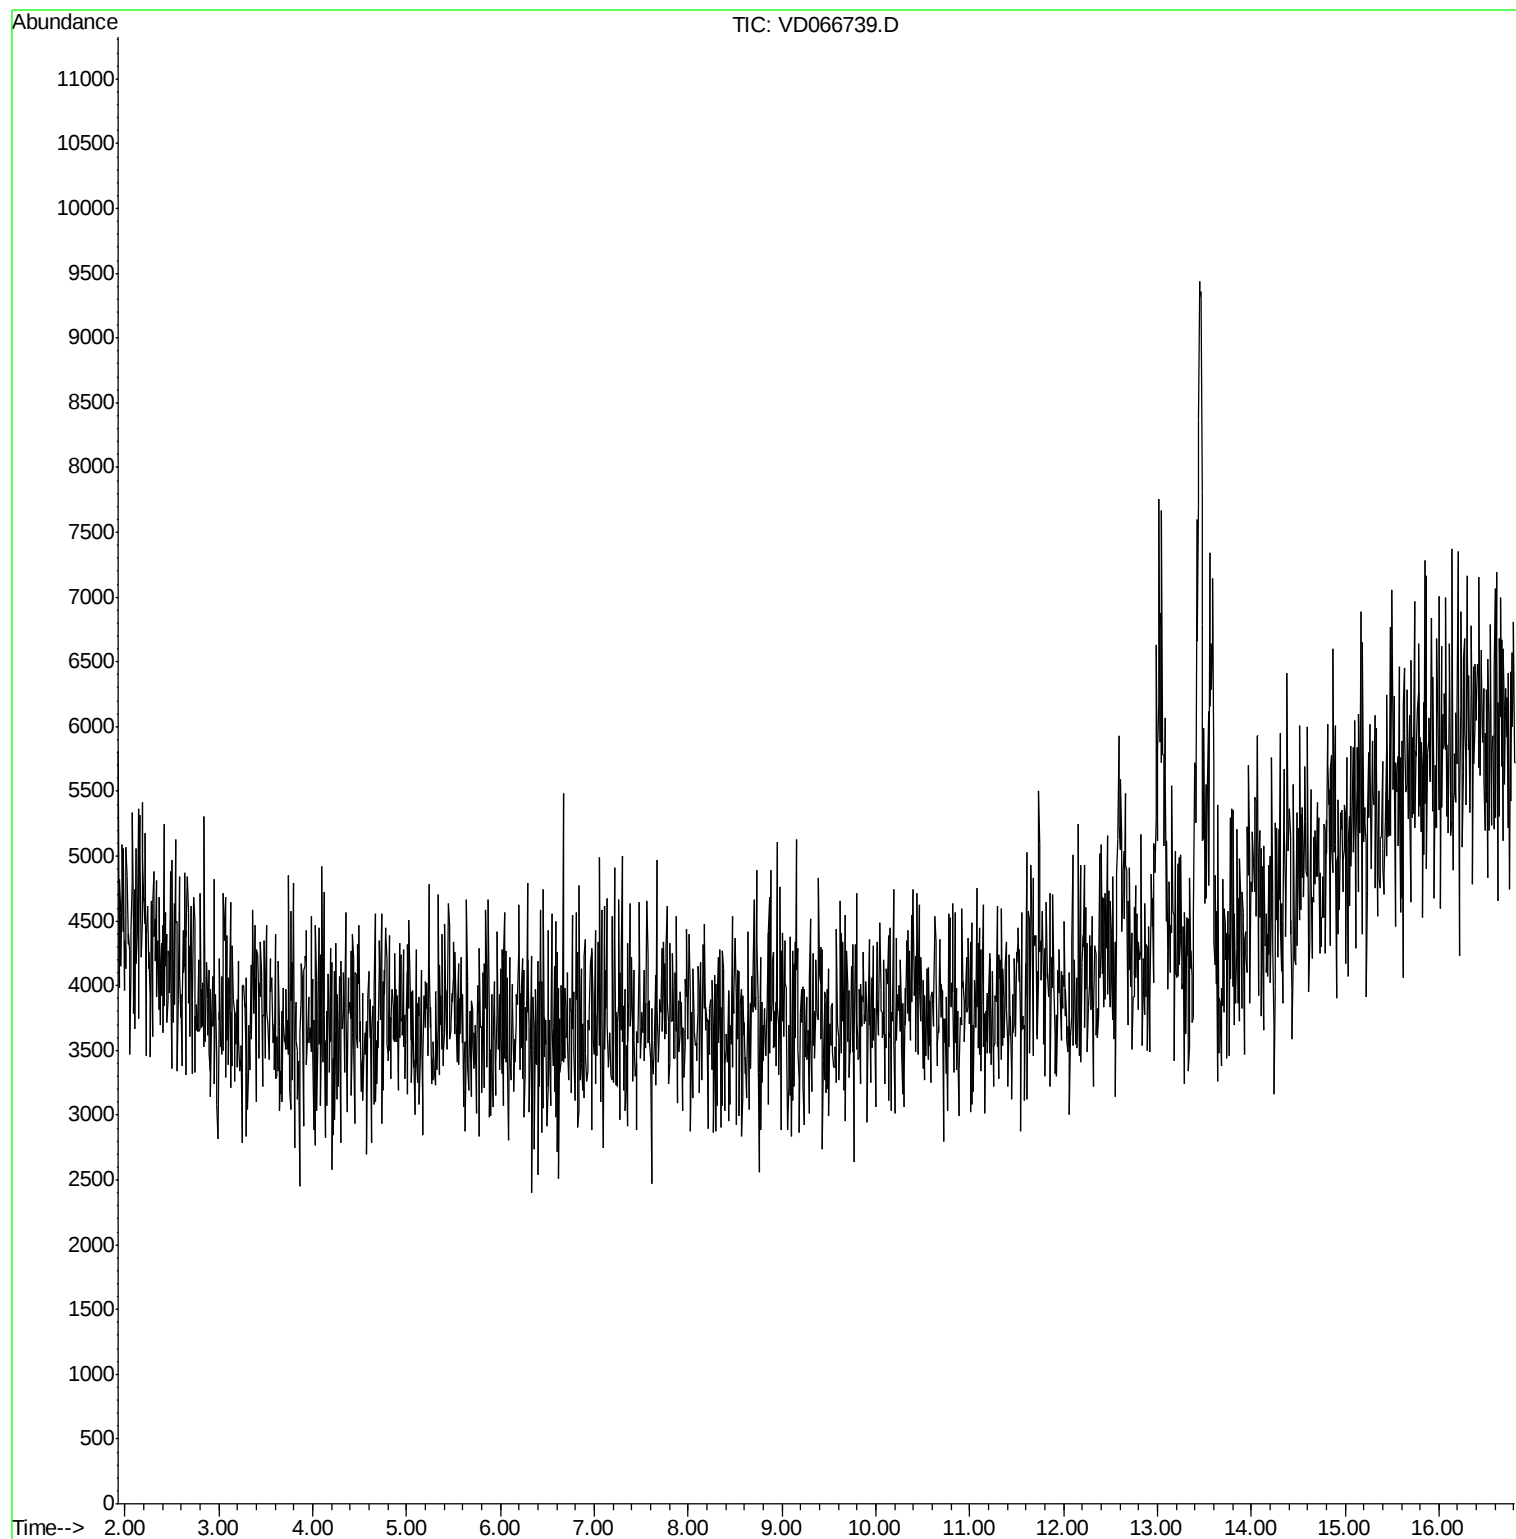


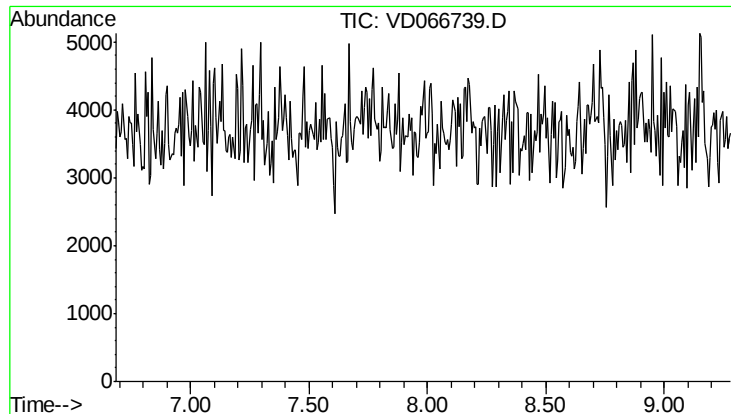


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.98 min

Lab File: VD066739.D
Acq: 17 Sep 2020 12:47

Instrument :
MSVOA_D
ClientSampleId :
PL-02-091520


Tot Ion: 168
Sig Exp Ratio
168 100
99 68.0

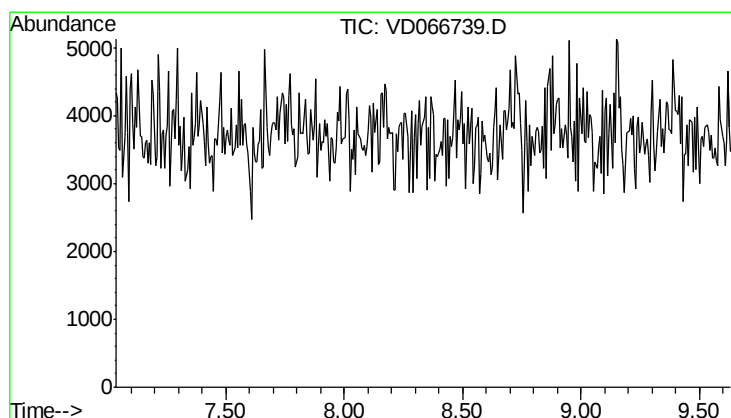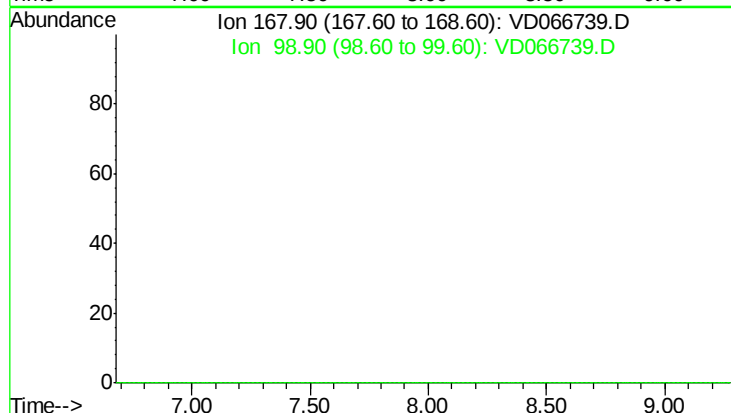


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.33 min

Lab File: VD066739.D
Acq: 17 Sep 2020 12:47

Tgt Ion: 65
Sig Exp Ratio
65 100
67 51.1


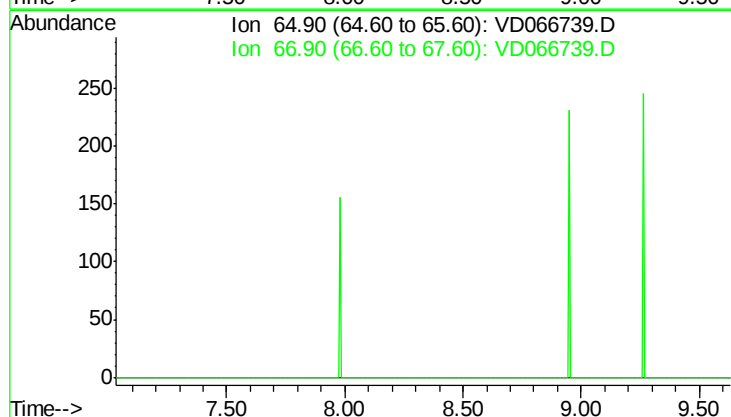


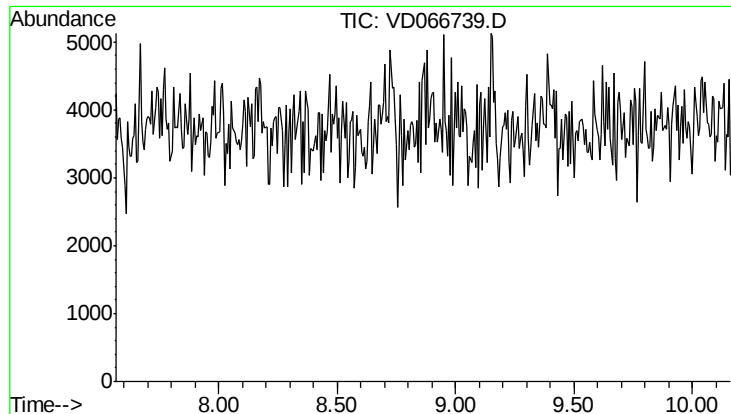

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.86 min
 Lab File: VD066739.D
 Acq: 17 Sep 2020 12:47


Instrument :
 MSVOA_D
 ClientSampleId :
 PL-02-091520


Tot Ion	114
Sig	Exp Ratio
114	100
63	18.8
88	16.1

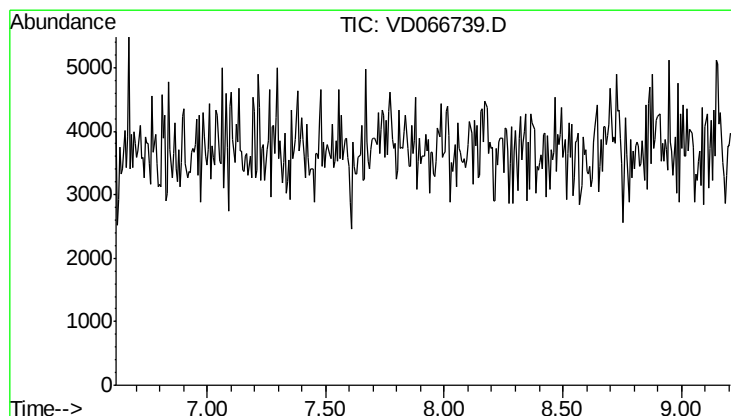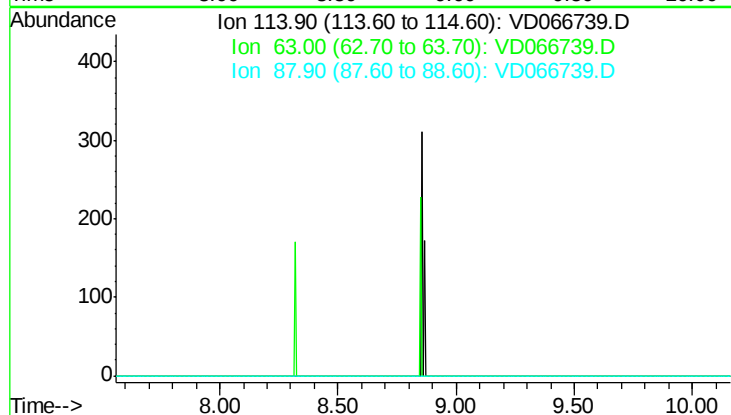

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.91 min
 Lab File: VD066739.D
 Acq: 17 Sep 2020 12:47

Tgt Ion	113
Sig	Exp Ratio
113	100
111	104.0
192	18.5

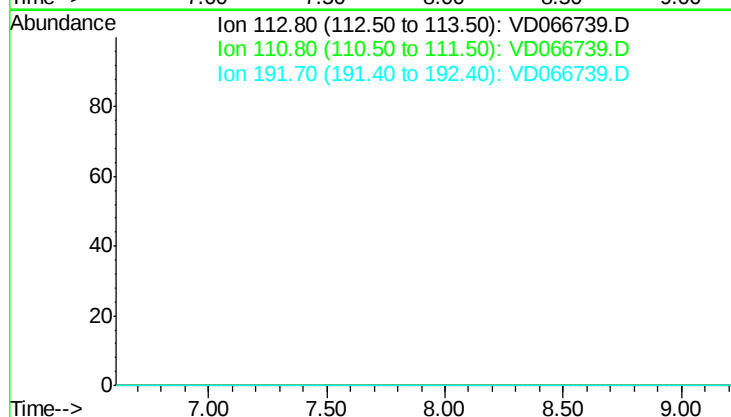


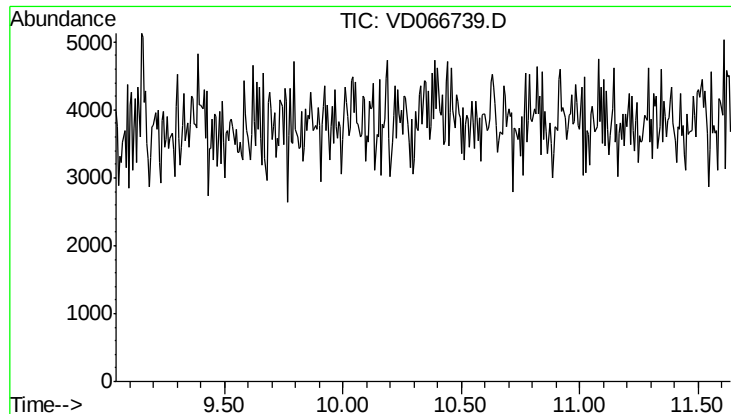


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.34 min

Lab File: VD066739.D
Acq: 17 Sep 2020 12:47

Instrument :
MSVOA_D
ClientSampleId :
PL-02-091520


Tot Ion	98
Sig	Exp Ratio
98	100
100	65.9

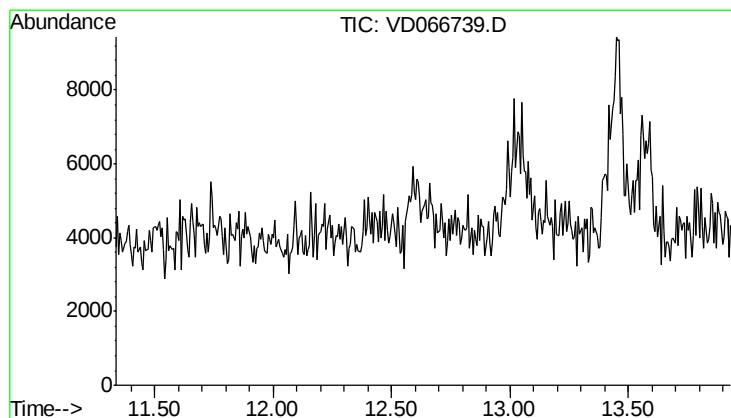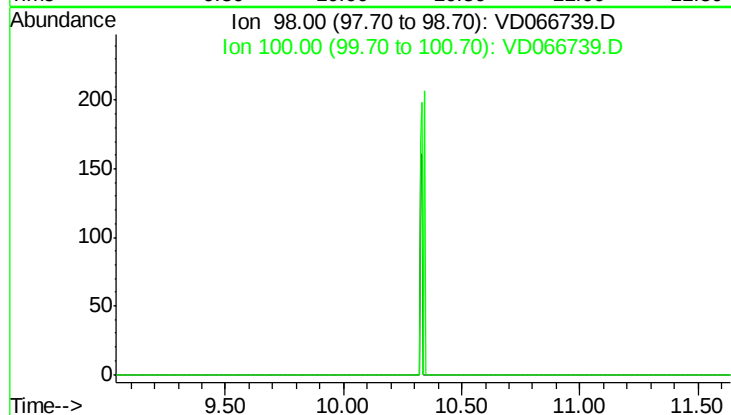


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.63 min

Lab File: VD066739.D
Acq: 17 Sep 2020 12:47

Tgt Ion	95
Sig	Exp Ratio
95	100
174	78.3
176	75.1

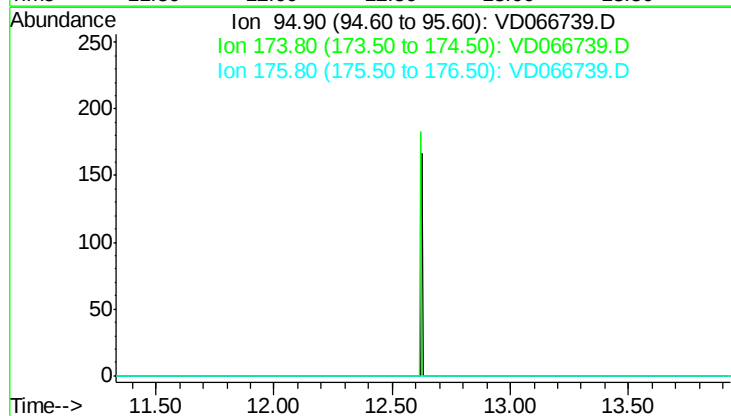


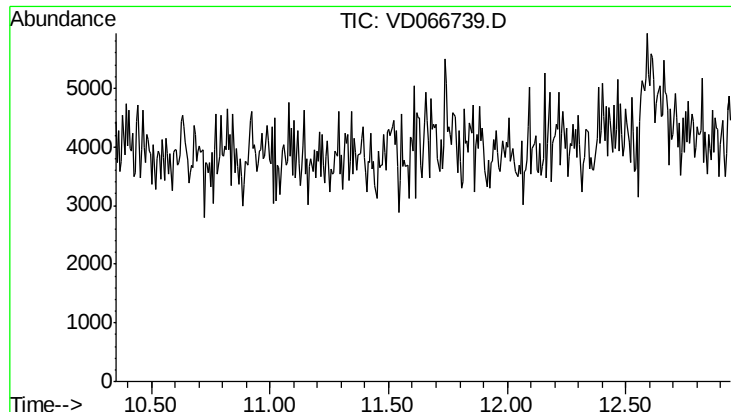


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.64 min

Lab File: VD066739.D
 Acq: 17 Sep 2020 12:47

Instrument :
 MSVOA_D
 ClientSampleId :
 PL-02-091520

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 56.7
 119 32.2

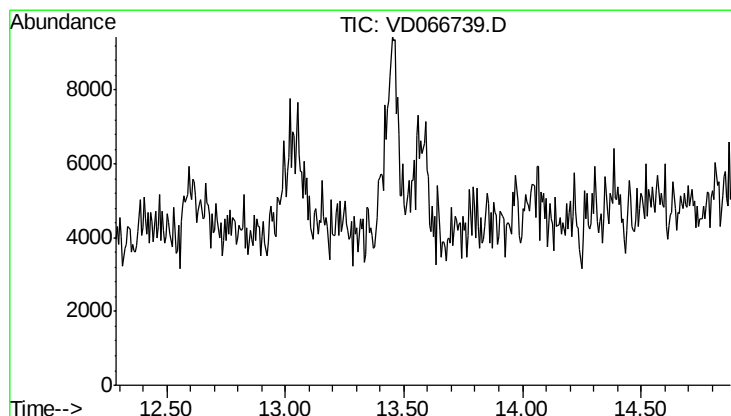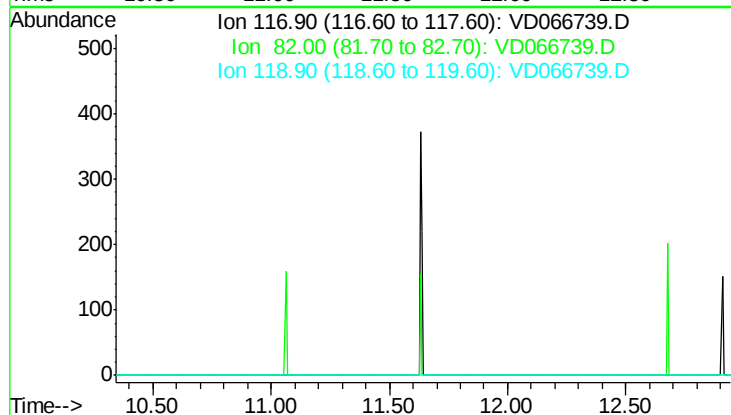

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.58 min

Lab File: VD066739.D
 Acq: 17 Sep 2020 12:47

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 61.0
 150 172.3

