
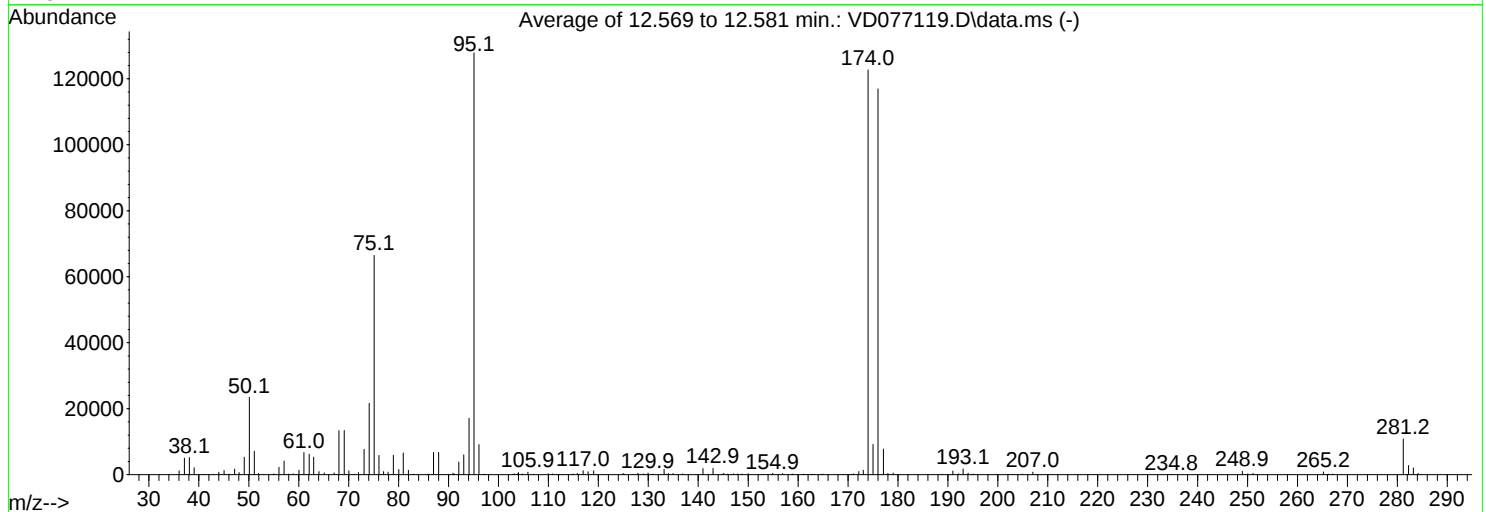


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091823\
Data File : VD077119.D
Acq On : 18 Sep 2023 09:11
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D091823S.M
Title : SW846 8260
Last Update : Tue Sep 19 04:46:37 2023

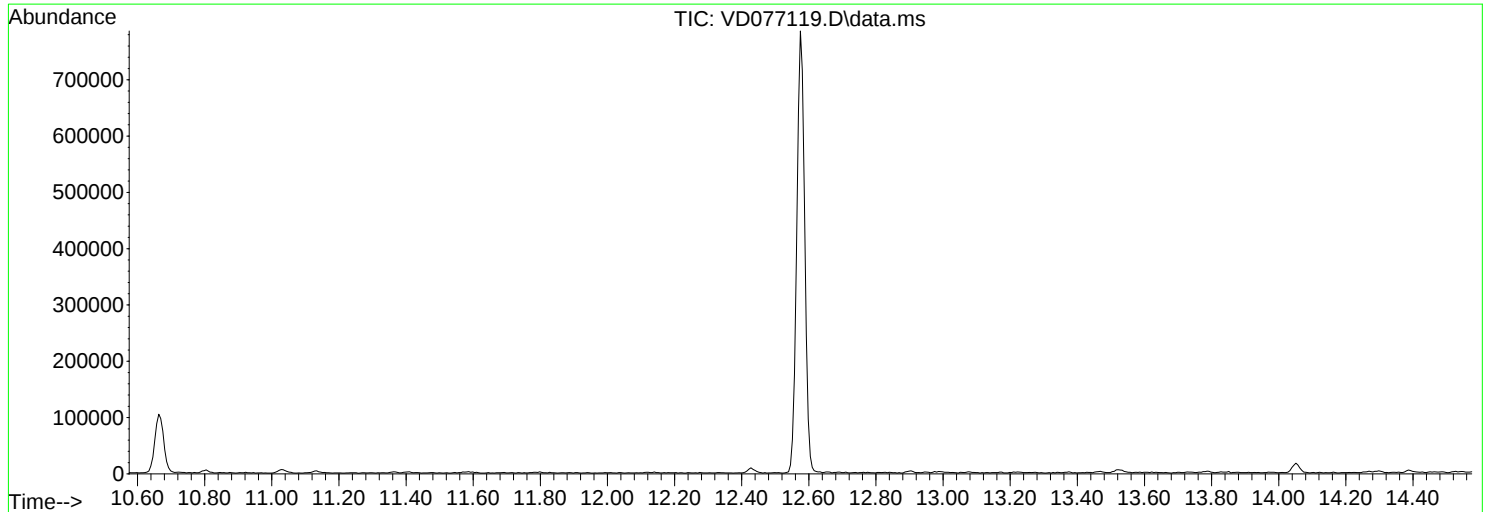

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	23413	PASS
75	95	30	60	52.0	66459	PASS
95	95	100	100	100.0	127864	PASS
96	95	5	9	7.1	9139	PASS
173	174	0.00	2	1.1	1356	PASS
174	95	50	100	96.0	122739	PASS
175	174	5	9	7.5	9185	PASS
176	174	95	101	95.3	116933	PASS
177	176	5	9	6.6	7758	PASS