




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091824\
Data File : VD079859.D
Acq On : 18 Sep 2024 12:43
Operator : RP/MD
Sample : P4083-01RE
Misc : 5.66G/10ml/MSVOA_D/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4ES1RE

Manual IntegrationsAPPROVED

Quant Time: Sep 19 01:53:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 19 01:50:07 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/24/2024
Supervised By :Semsettin Yesilyurt 09/24/2024

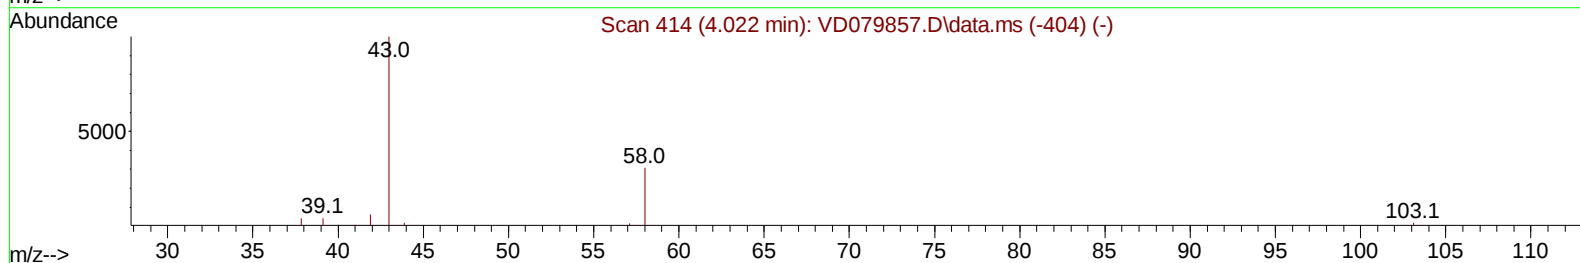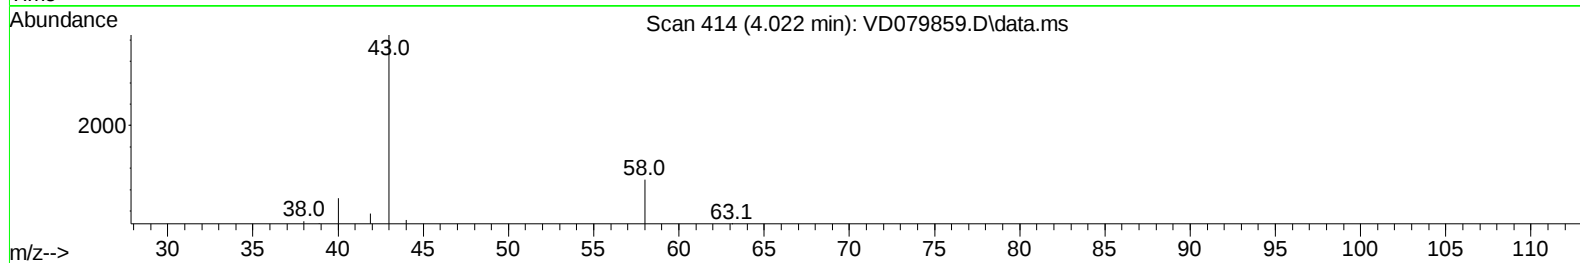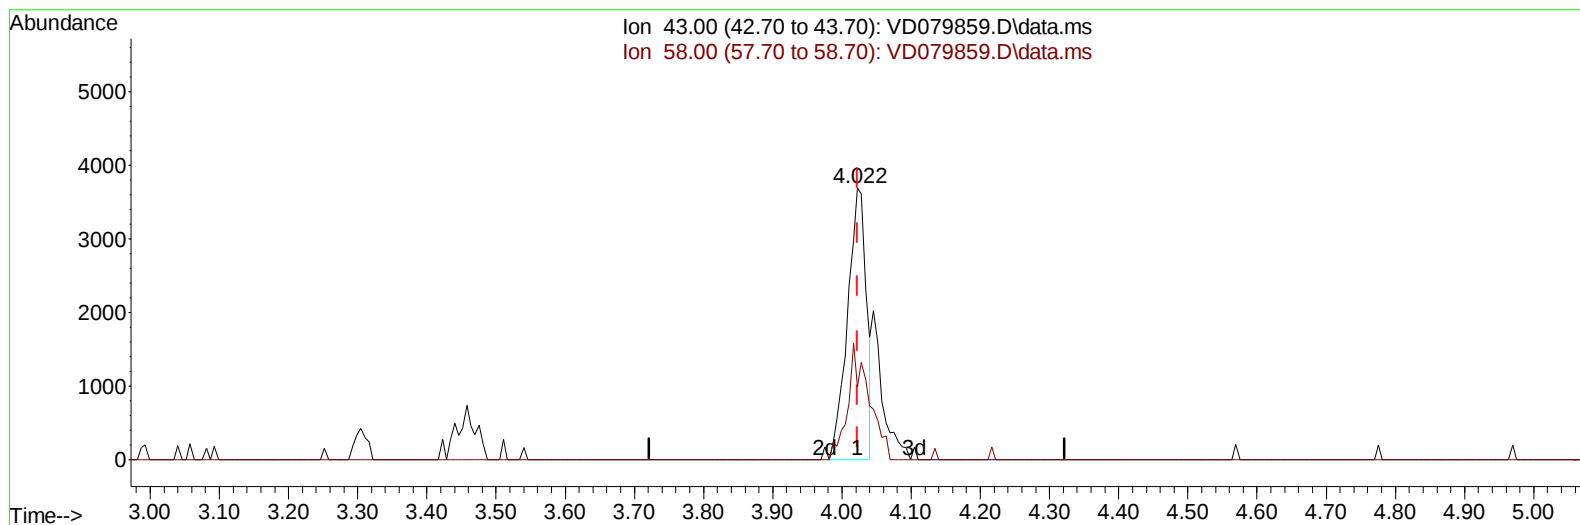

TIC: VD079859.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 12.76 ug/L

response 6996

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	37.90	25.06
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091824\
Data File : VD079859.D
Acq On : 18 Sep 2024 12:43
Operator : RP/MD
Sample : P4083-01RE
Misc : 5.66G/10ml/MSVOA_D/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4ES1RE

Manual IntegrationsAPPROVED

Quant Time: Sep 19 01:53:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 19 01:50:07 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/24/2024
Supervised By :Semsettin Yesilyurt 09/24/2024

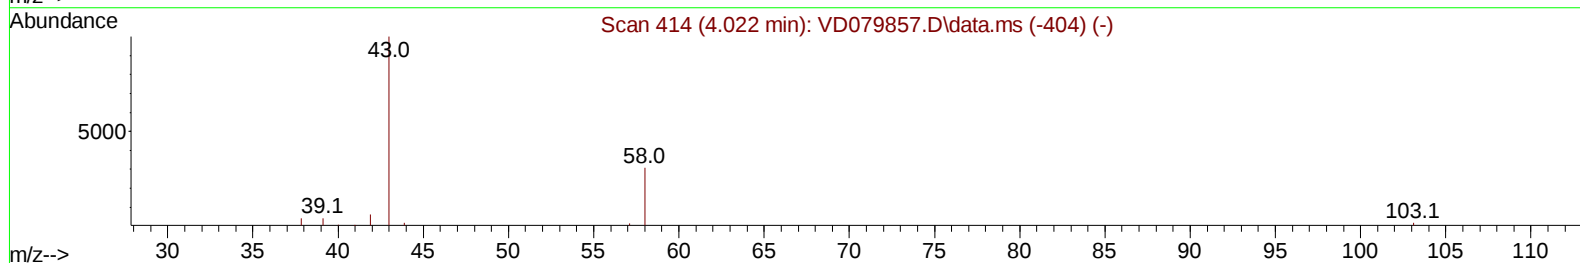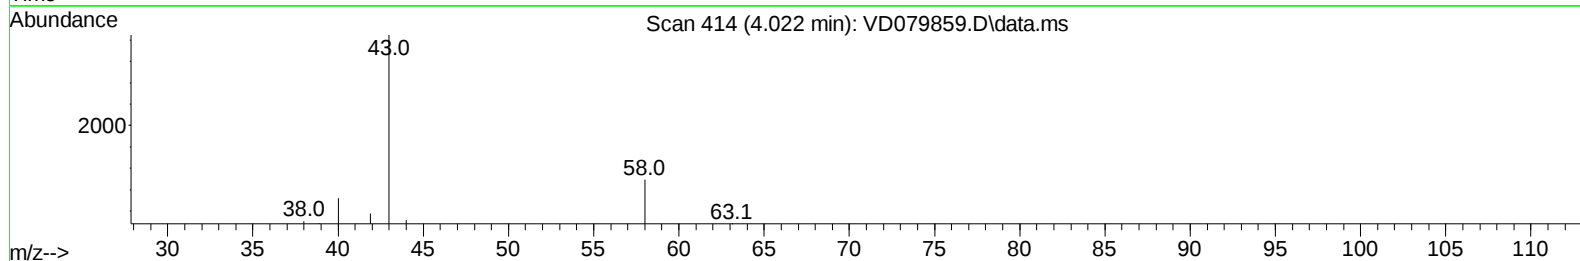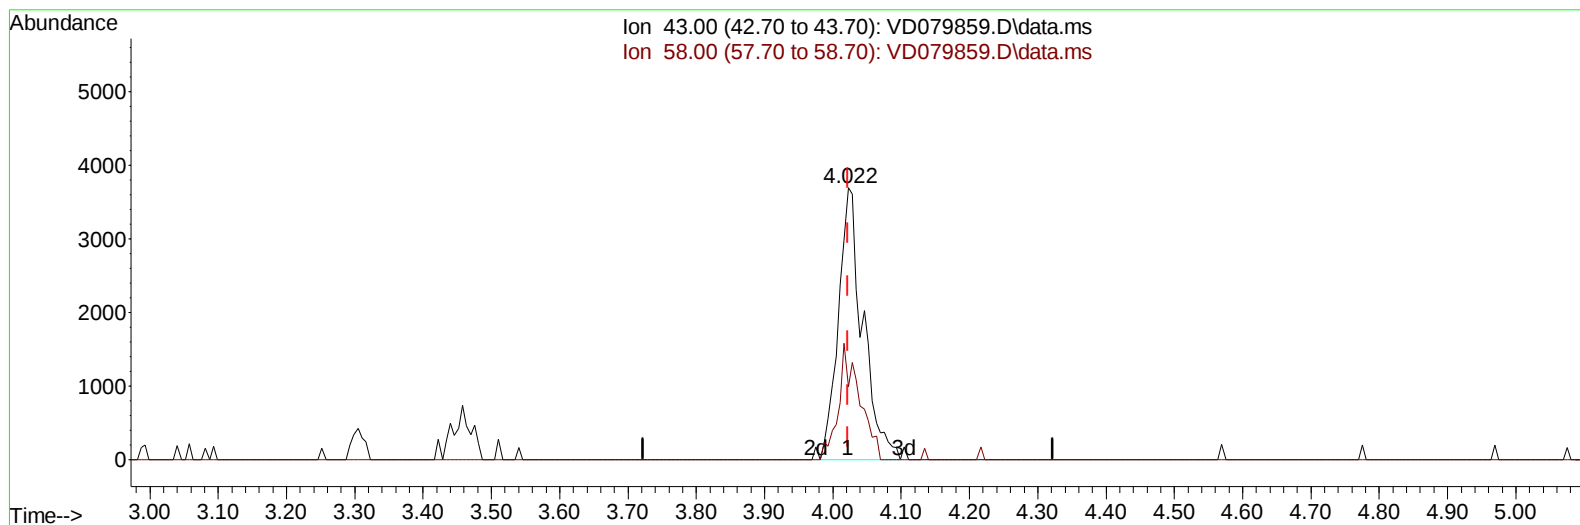

TIC: VD079859.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 16.75 ug/L m

response 9182

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	37.90	19.09
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091824\
 Data File : VD079859.D
 Acq On : 18 Sep 2024 12:43
 Operator : RP/MD
 Sample : P4083-01RE
 Misc : 5.66G/10mL/MSVOA_D/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A4ES1RE

Manual IntegrationsAPPROVED

Quant Time: Sep 19 01:53:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 19 01:50:07 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/24/2024
 Supervised By :Semsettin Yesilyurt 09/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		111282	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		70698	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		13874	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		72258	14.933	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	59.720%		
7) Chloroethane-d5	2.805	69		71455	18.651	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	74.600%		
11) 1,1-Dichloroethene-d2	3.917	65		12568	14.305	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.240%		
21) 2-Butanone-d5	6.981	46		16809	37.387	ug/L	-0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	74.780%		
24) Chloroform-d	7.569	84		70704	19.328	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	77.320%		
26) 1,2-Dichloroethane-d4	8.228	65		40843	21.352	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	85.400%		
32) Benzene-d6	8.199	84		128330	25.711	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	102.840%		
36) 1,2-Dichloropropane-d6	9.210	67		46611	30.491	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	121.960%#		
41) Toluene-d8	10.269	98		86730	19.747	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	79.000%		
43) trans-1,3-Dichloroprop...	10.522	79		14559	22.152	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	88.600%		
47) 2-Hexanone-d5	10.875	63		11657	46.779	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	93.560%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84		22189	19.753	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	79.000%		
66) 1,2-Dichlorobenzene-d4	13.816	152		9632	18.409	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	73.640%#		
Target Compounds							
13) Acetone	4.022	43		9182m	16.752	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091824\
Data File : VD079859.D
Acq On : 18 Sep 2024 12:43
Operator : RP/MD
Sample : P4083-01RE
Misc : 5.66G/10ml/MSVOA_D/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4ES1RE

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/24/2024
Supervised By :Semsettin Yesilyurt 09/24/2024

Quant Time: Sep 19 01:53:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 19 01:50:07 2024
Response via : Initial Calibration

