
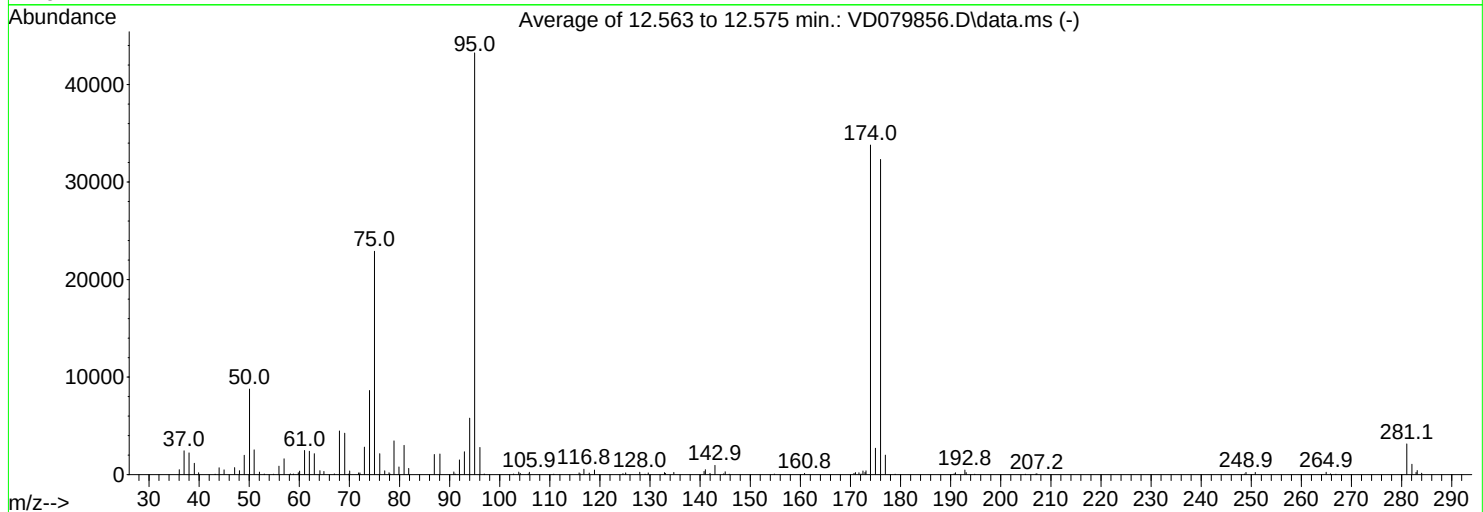


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091824\
Data File : VD079856.D
Acq On : 18 Sep 2024 09:04
Operator : RP/MD
Sample : BFB831
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB831

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Thu Sep 19 01:50:07 2024

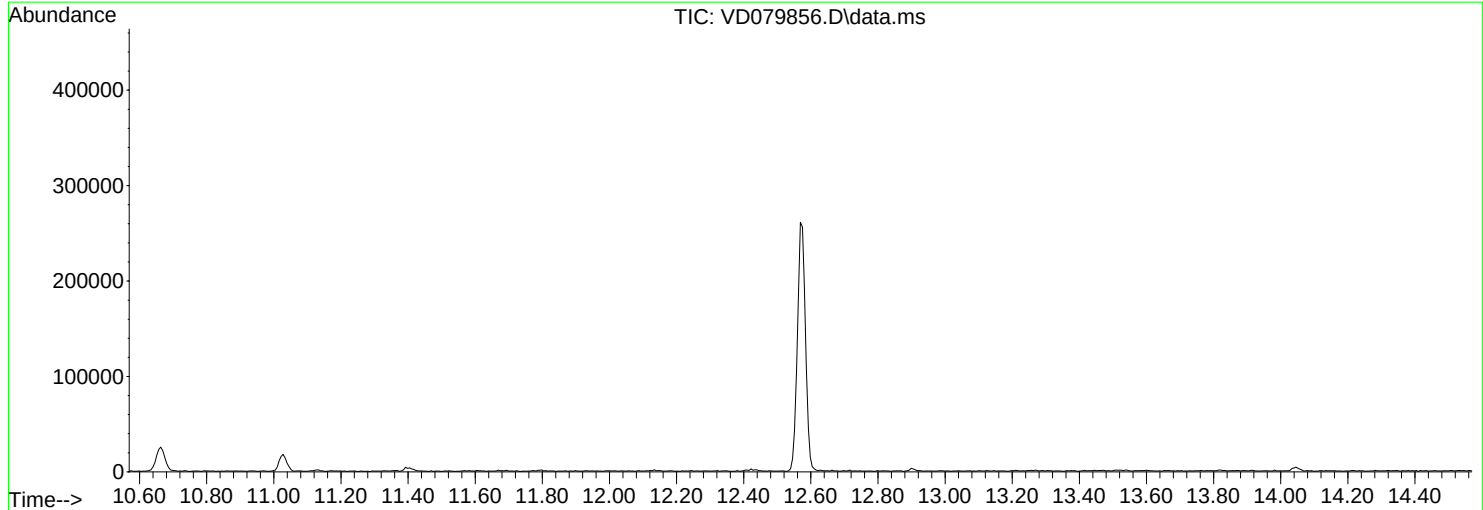

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	8782	PASS
75	95	30	80	53.0	22904	PASS
95	95	100	100	100.0	43248	PASS
96	95	5	9	6.4	2786	PASS
173	174	0.00	2	1.2	403	PASS
174	95	50	120	78.2	33800	PASS
175	174	5	9	8.0	2702	PASS
176	174	95	105	95.6	32312	PASS
177	176	5	10	6.2	2002	PASS

m/z	Abundance
39.90	483.0

Instrument :
MSVOA_D
ClientSampleId :
BFB831

m/z	Abundance
36.00	415.0
37.00	1989.0
38.00	1674.0
39.10	939.0
39.90	757.0
44.10	641.0
45.00	336.0
47.00	558.0
48.00	410.0
49.00	1341.0
50.00	7362.0
51.00	1982.0
52.10	210.0
55.90	858.0
57.00	1441.0
58.80	193.0
59.80	583.0
61.10	1869.0
62.00	1621.0
63.10	1828.0
64.10	280.0
64.90	224.0
68.00	3724.0
69.10	3625.0
69.90	219.0
70.10	215.0
71.80	229.0
72.10	205.0
73.00	2407.0
74.00	7097.0
75.00	20056.0
76.10	2011.0
77.00	519.0
77.90	232.0
78.90	2713.0
80.00	521.0
80.90	2887.0
81.80	491.0
87.00	1658.0
88.00	1605.0
90.80	193.0
91.10	220.0
91.90	997.0
93.00	1832.0
94.00	4919.0
95.00	33664.0
96.00	2129.0
103.80	290.0
105.70	223.0
115.80	286.0
116.90	382.0
118.90	535.0
128.10	202.0
134.80	181.0
140.90	408.0
142.00	161.0
142.90	675.0
144.70	266.0
145.10	239.0
171.10	245.0
172.10	222.0
172.90	707.0
174.00	25448.0
175.00	1941.0
176.00	25976.0
177.00	1436.0
178.90	158.0
191.10	204.0
192.90	414.0
248.70	200.0
265.00	179.0
281.00	2218.0
282.10	737.0
282.90	690.0

Instrument :
MSVOA_D
ClientSampleId :
BFB831

m/z	Abundance
36.10	519.0
37.00	2354.0
38.00	2614.0
39.10	1287.0
40.00	505.0
43.20	162.0
44.00	746.0
45.00	513.0
47.10	703.0
48.10	403.0
49.00	2344.0
50.00	9837.0
51.00	2954.0
52.00	247.0
53.00	218.0
56.00	921.0
56.90	1308.0
60.00	636.0
61.00	3059.0
62.00	2518.0
63.00	2089.0
64.10	503.0
64.90	271.0
68.00	4831.0
69.00	4354.0
70.00	436.0
72.10	353.0
73.00	3216.0
74.00	9401.0
75.00	24352.0
76.10	2459.0
77.10	317.0
78.10	193.0
78.90	3898.0
79.90	1201.0
80.90	3291.0
81.90	784.0
86.90	2520.0
88.10	2572.0
90.90	347.0
91.90	1690.0
92.90	2535.0
94.00	6402.0
95.00	50120.0
96.10	3266.0
96.90	183.0
104.10	391.0
105.90	338.0
110.80	164.0
116.10	211.0
116.80	689.0
118.00	191.0
118.90	418.0
124.60	164.0
125.20	298.0
127.90	230.0
129.00	158.0
129.60	266.0
132.90	639.0
134.70	202.0
140.70	604.0
141.10	559.0
142.90	1337.0
145.00	363.0
145.80	153.0
154.80	198.0
160.90	209.0
170.90	406.0
171.70	223.0
172.50	495.0
173.10	1208.0
174.00	38368.0
174.90	2811.0
176.00	35544.0
176.90	2116.0
190.90	372.0
193.10	664.0
207.00	194.0
249.00	349.0
250.80	270.0
264.90	268.0
281.10	2930.0
282.10	1015.0
283.10	683.0
284.00	423.0

Instrument :
MSVOA_D
ClientSampleId :
BFB831

m/z	Abundance
36.10	584.0
37.00	3003.0
38.00	2392.0
39.00	1248.0
40.00	770.0
43.90	713.0
45.00	614.0
47.20	891.0
48.00	406.0
49.00	2285.0
50.10	9148.0
51.00	2692.0
52.00	353.0
54.90	152.0
56.00	812.0
57.00	2119.0
58.20	259.0
60.10	458.0
61.00	2512.0
62.00	3036.0
62.90	2529.0
64.10	459.0
64.90	488.0
67.00	227.0
68.00	4878.0
69.00	4792.0
70.00	489.0
71.90	312.0
73.00	2831.0
74.00	9380.0
75.00	24304.0
76.00	1977.0
77.00	361.0
77.90	363.0
78.90	3752.0
79.80	649.0
80.90	2839.0
81.90	644.0
87.00	2007.0
88.00	2169.0
90.80	302.0
92.00	1829.0
93.00	2676.0
94.00	6051.0
95.00	45960.0
96.00	2962.0
102.80	213.0
103.80	511.0
105.90	428.0
115.90	253.0
116.70	609.0
117.80	319.0
118.90	488.0
124.60	151.0
125.10	262.0
127.90	311.0
129.70	289.0
133.10	339.0
134.70	285.0
141.00	971.0
141.90	218.0
143.00	865.0
144.90	310.0
160.80	190.0
170.70	383.0
171.70	369.0
172.50	624.0
174.00	37584.0
175.10	3355.0
176.00	35416.0
177.00	2454.0
190.70	236.0
192.80	1012.0
194.80	150.0
204.90	161.0
207.20	300.0
248.90	354.0
250.80	405.0
264.90	277.0
265.80	236.0
266.90	166.0
281.10	4316.0
282.00	1447.0
283.10	599.0

Instrument :
MSVOA_D
ClientSampleId :
BFB831