


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD092018\
Data File : VD060048.D
Acq On : 20 Sep 2018 10:31
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091318S.M
Title : SW846 8260
Last Update : Thu Sep 13 16:17:40 2018

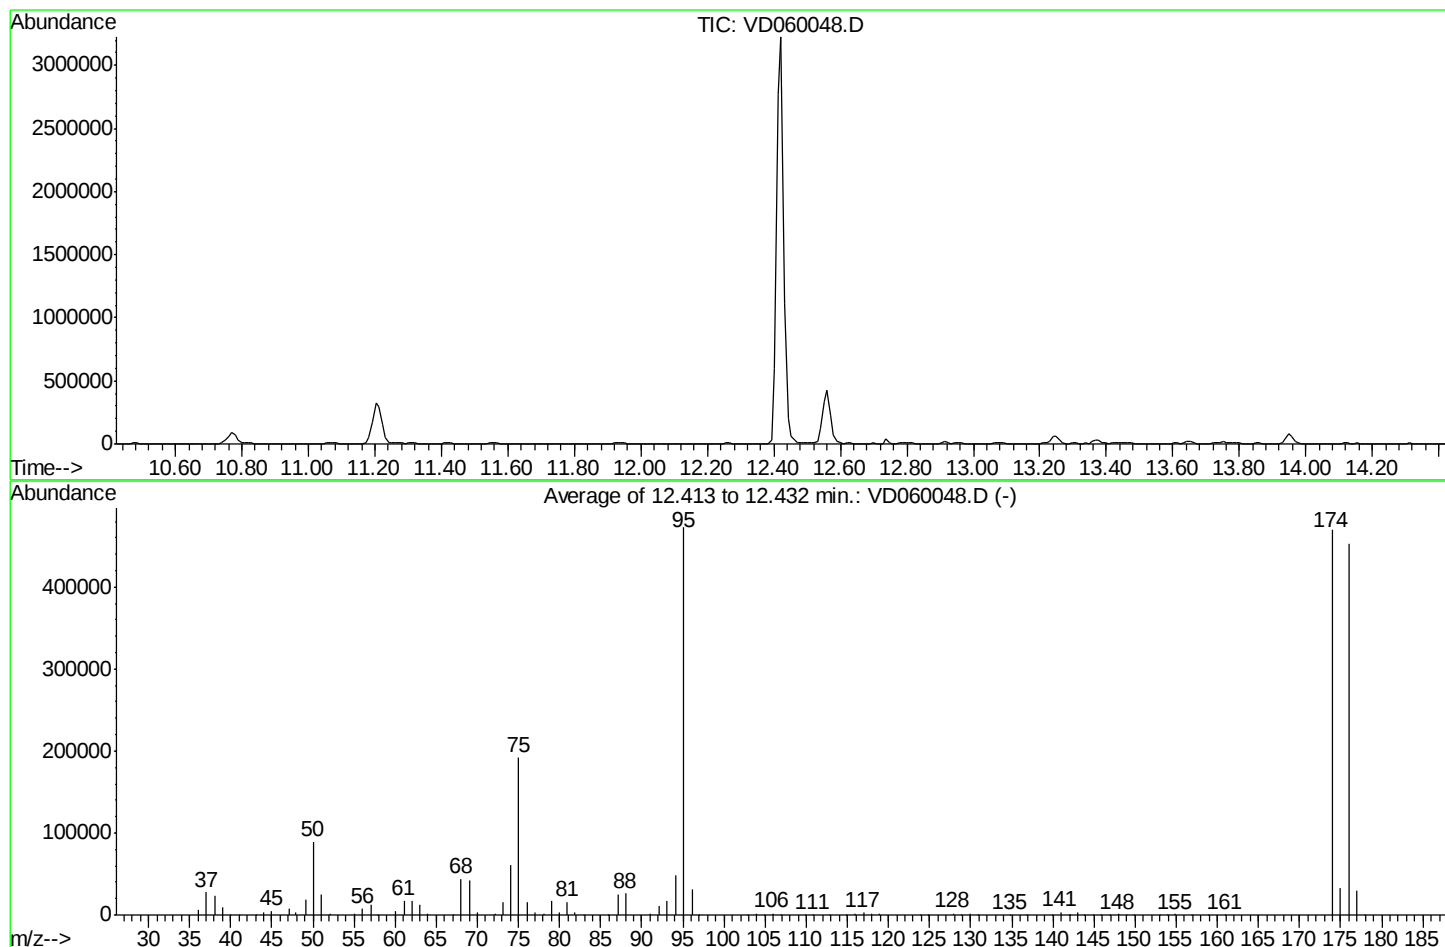

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1101

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	89213	PASS
75	95	30	60	40.5	191290	PASS
95	95	100	100	100.0	472789	PASS
96	95	5	9	6.7	31802	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	99.3	469397	PASS
175	174	5	9	7.0	32976	PASS
176	174	95	101	96.6	453376	PASS
177	176	5	9	6.6	29746	PASS