


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092118\
Data File : VD060063.D
Acq On : 21 Sep 2018 9:59
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D091318S.M
Title : SW846 8260
Last Update : Thu Sep 13 16:17:40 2018

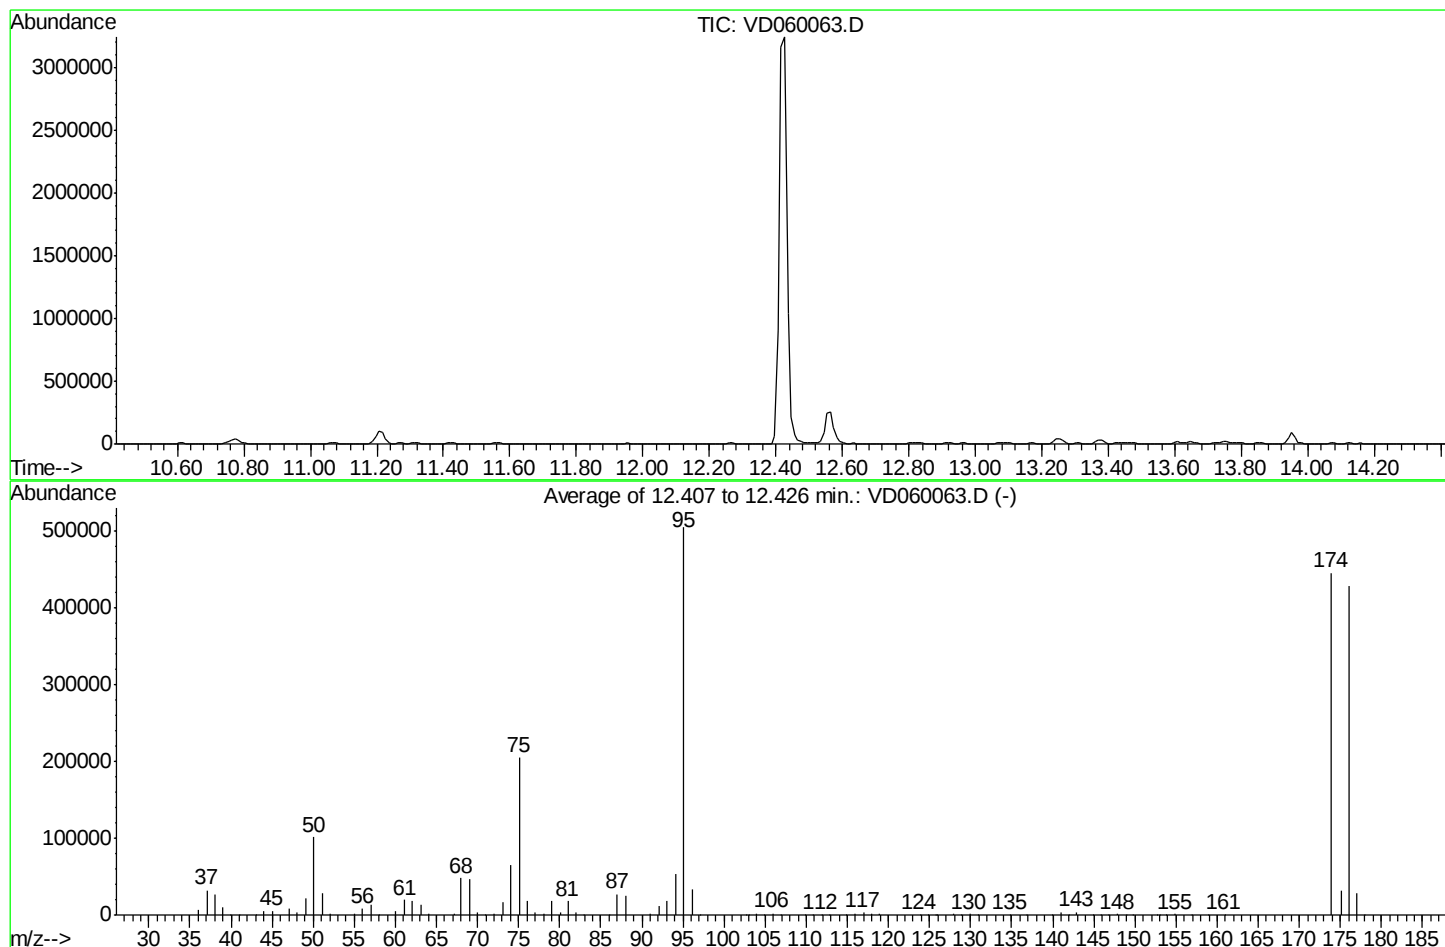

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	100968	PASS
75	95	30	60	40.6	204957	PASS
95	95	100	100	100.0	504768	PASS
96	95	5	9	6.7	34067	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.2	445293	PASS
175	174	5	9	7.2	31880	PASS
176	174	95	101	96.3	428906	PASS
177	176	5	9	6.7	28830	PASS