

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092123\
 Data File : VD077179.D
 Acq On : 21 Sep 2023 14:31
 Operator : JC/SY
 Sample : 04469-02
 Misc : 4.54G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EZYL8

Quant Time: Sep 22 01:31:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM090123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 22 01:29:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	286179	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	277134	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	118579	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.270	65	143207	20.308	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.240%
7) Chloroethane-d5	2.805	69	129842	22.391	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.560%
11) 1,1-Dichloroethene-d2	3.911	65	35088	21.905	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.600%
21) 2-Butanone-d5	6.981	46	46378	52.207	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.420%
24) Chloroform-d	7.563	84	178088	22.742	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.960%
26) 1,2-Dichloroethane-d4	8.228	65	92678	24.971	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.880%
32) Benzene-d6	8.199	84	356964	23.321	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.280%
36) 1,2-Dichloropropane-d6	9.210	67	113017	25.747	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.000%
41) Toluene-d8	10.269	98	309607	22.097	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.400%
43) trans-1,3-Dichloroprop...	10.522	79	41762	20.881	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.520%
47) 2-Hexanone-d5	10.875	63	32780	46.756	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.520%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	91880	23.479	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.920%
66) 1,2-Dichlorobenzene-d4	13.816	152	98031	25.757	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.040%
Target Compounds						Qvalue
14) Carbon disulfide	4.269	76	6717	0.540	ug/L	# 85
16) Methylene chloride	4.799	84	17461	2.998	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092123\
Data File : VD077179.D
Acq On : 21 Sep 2023 14:31
Operator : JC/SY
Sample : 04469-02
Misc : 4.54G/10.0ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EZYL8

Quant Time: Sep 22 01:31:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM090123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 22 01:29:35 2023
Response via : Initial Calibration




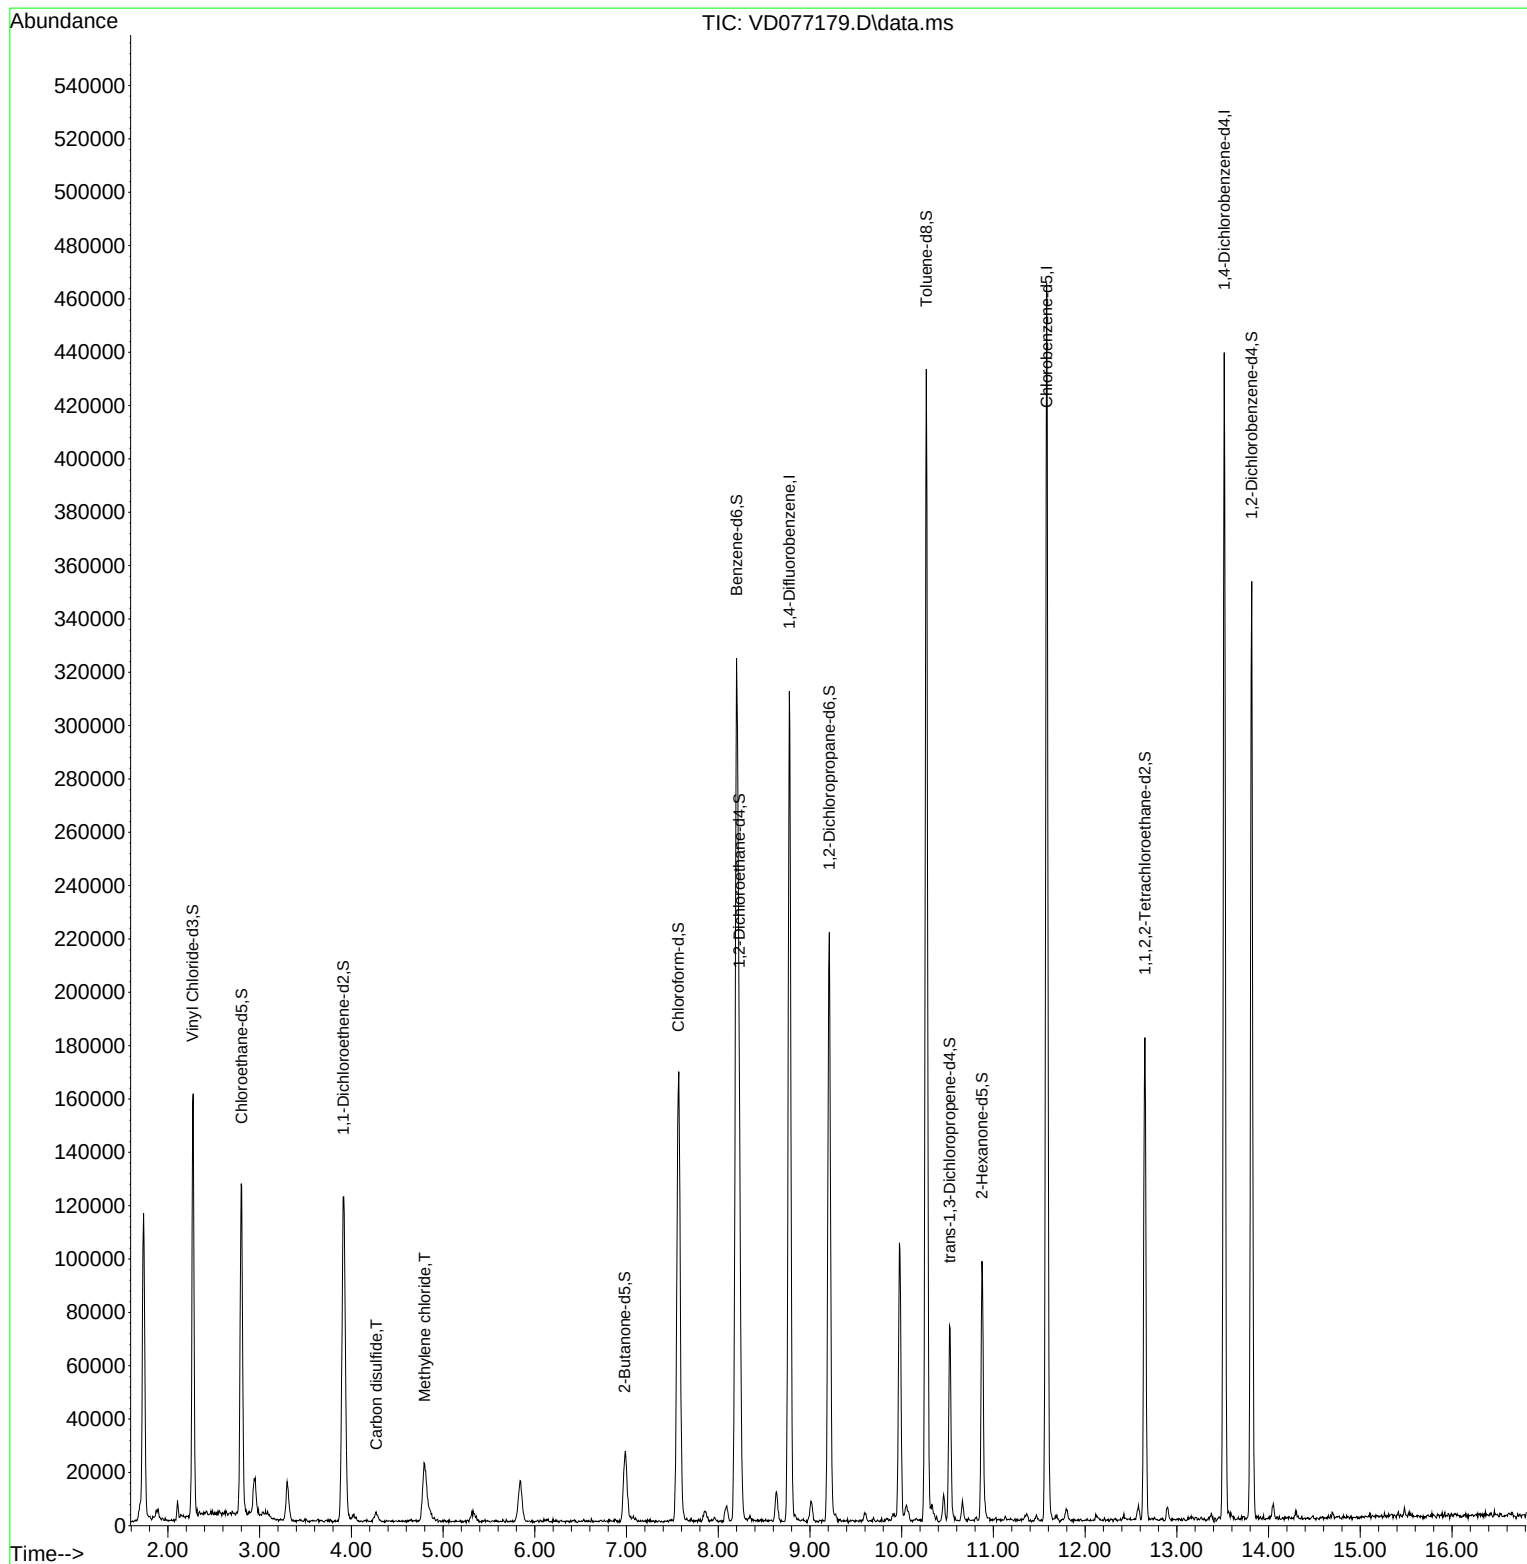


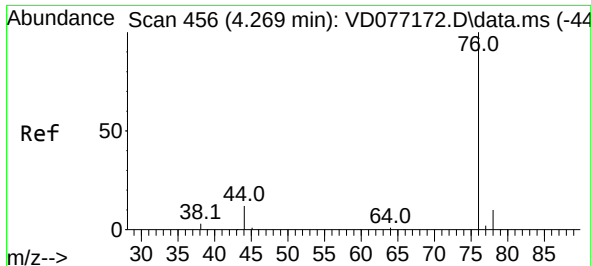

#14
Carbon disulfide
Concen: 0.540 ug/L
RT: 4.269 min Scan# 41
Delta R.T. 0.000 min
Lab File: VD077179.D
Acq: 21 Sep 2023 14:31

Instrument :
MSVOA_D
ClientSampleId :
EZY8

Tgt Ion: 76 Resp: 6717
Ion Ratio Lower Upper
76 100
78 14.9 7.5 11.3#

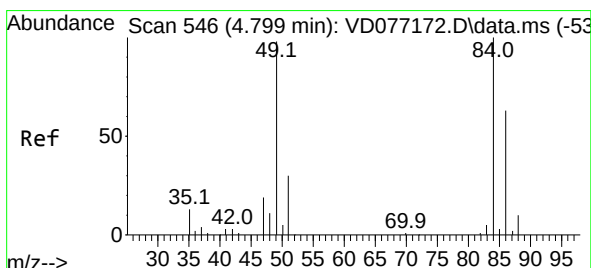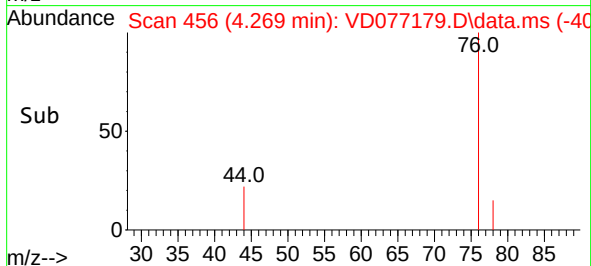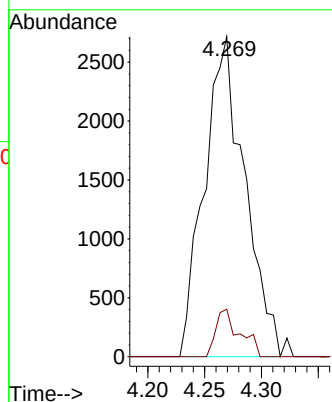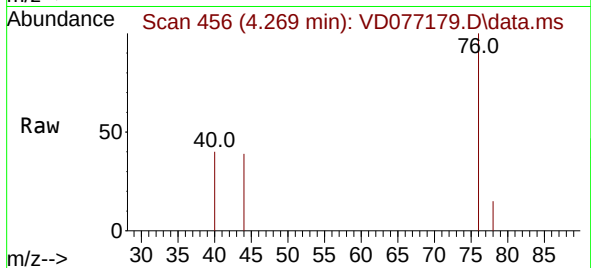

#16
Methylene chloride
Concen: 2.998 ug/L
RT: 4.799 min Scan# 546
Delta R.T. 0.000 min
Lab File: VD077179.D
Acq: 21 Sep 2023 14:31

Tgt Ion: 84 Resp: 17461
Ion Ratio Lower Upper
84 100
86 64.5 45.3 84.1
49 104.7 69.2 128.6

