
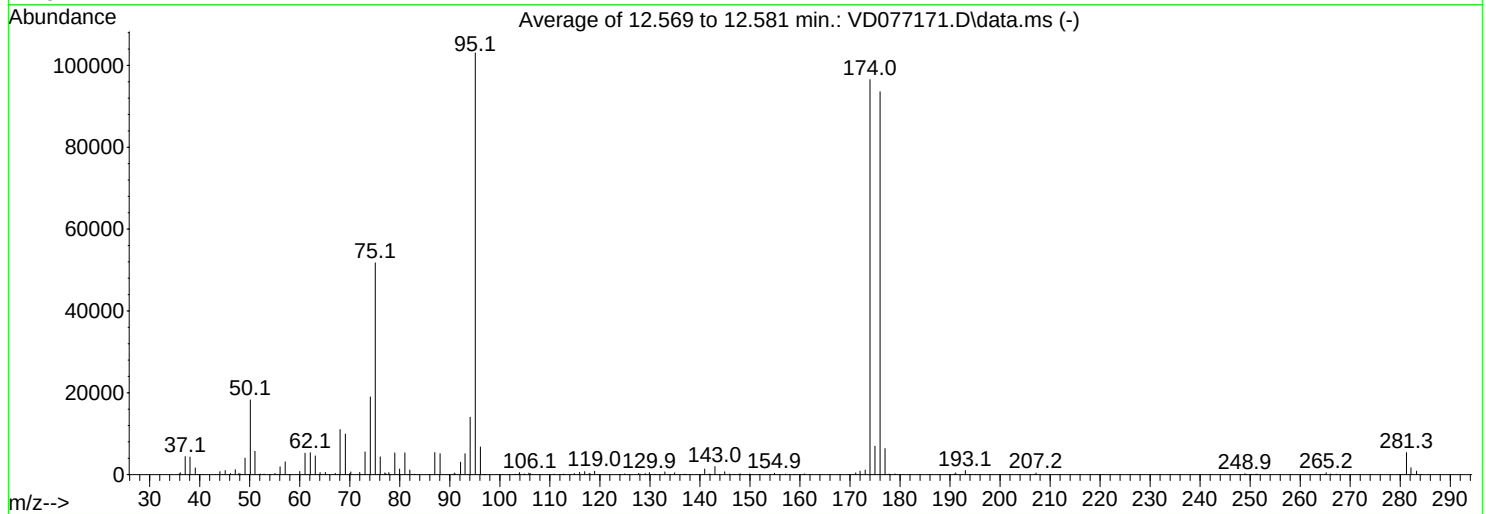


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092123\
 Data File : VD077171.D
 Acq On : 21 Sep 2023 08:52
 Operator : JC/SY
 Sample : BFB163
 Misc : 5.00G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB163

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM090123SMA.M
 Title : SFAM01.0
 Last Update : Fri Sep 22 23:41:10 2023

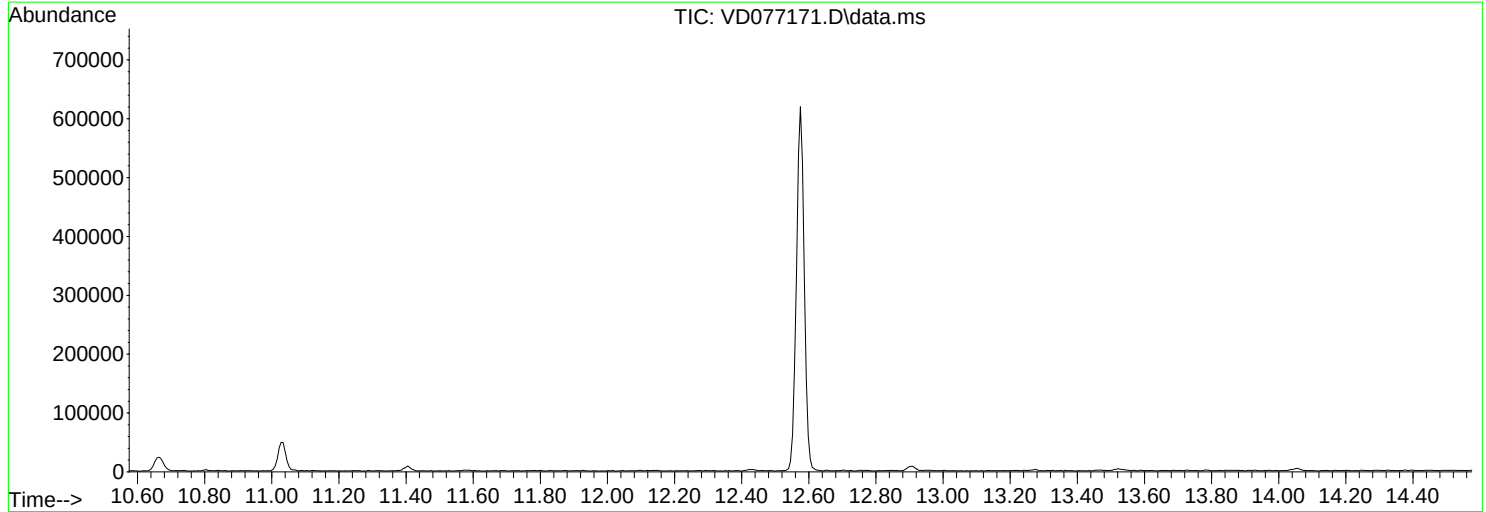

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	18280	PASS
75	95	30	80	50.2	51755	PASS
95	95	100	100	100.0	103077	PASS
96	95	5	9	6.6	6752	PASS
173	174	0.00	2	1.2	1128	PASS
174	95	50	120	93.6	96528	PASS
175	174	5	9	7.2	6951	PASS
176	174	95	105	96.9	93552	PASS
177	176	5	10	6.8	6379	PASS

Scan 1859 (12.522 min): VD077171.D\data.ms
BFB163

m/z	Abundance
40.00	1468.0
44.10	509.0
96.80	172.0

Instrument :
MSVOA_D
ClientSampleId :
BFB163

m/z	Abundance
35.90	623.0
37.10	4753.0
38.00	4671.0
39.10	1846.0
40.00	1164.0
44.10	1192.0
45.10	1042.0
46.20	427.0
47.10	1412.0
48.20	536.0
49.10	4191.0
50.10	17648.0
51.10	5644.0
52.00	191.0
52.20	194.0
52.90	248.0
55.10	220.0
56.10	1964.0
57.10	3436.0
57.90	176.0
60.10	822.0
61.10	5487.0
62.10	5108.0
63.10	4914.0
64.10	560.0
65.10	450.0
67.10	313.0
68.10	10525.0
69.10	9721.0
70.00	798.0
71.90	594.0
73.00	6183.0
74.10	18568.0
75.10	49440.0
76.10	4340.0
77.10	538.0
77.90	387.0
79.00	5901.0
80.00	1105.0
81.00	4975.0
81.90	1186.0
87.00	5687.0
88.00	4780.0
90.90	504.0
92.10	3723.0
93.10	5249.0
94.10	14161.0
95.10	98056.0
96.10	6612.0
96.90	185.0
103.00	182.0
103.80	502.0
104.80	191.0
105.80	719.0
112.80	240.0
114.80	166.0
116.00	467.0
117.00	704.0
117.80	534.0
119.00	529.0
124.90	264.0
128.00	464.0
129.00	383.0
129.90	518.0
133.00	604.0
135.00	550.0
137.20	214.0
141.00	1320.0
141.80	209.0
143.10	1829.0
145.00	773.0
145.90	175.0
146.80	188.0
148.00	299.0
150.00	213.0
154.80	322.0
171.30	364.0
172.00	602.0
173.00	1410.0
174.00	92392.0
175.00	6758.0
176.00	86416.0
177.00	5950.0
177.80	191.0
179.00	212.0
190.90	519.0
193.10	716.0
207.10	498.0
248.90	291.0
251.30	206.0
264.90	291.0
265.30	186.0

Instrument :
MSVOA_D
ClientSampleId :
BFB163

266.10	165.0
281.20	4420.0
282.30	768.0
283.30	644.0

Instrument :
MSVOA_D
ClientSampleId :
BFB163

m/z	Abundance
36.10	788.0
37.10	4658.0
38.10	4839.0
39.10	1634.0
40.00	1036.0
44.00	1211.0
45.10	1335.0
47.00	1300.0
47.90	644.0
49.00	4182.0
50.10	19832.0
51.10	6425.0
52.10	332.0
54.20	152.0
54.90	230.0
56.00	1977.0
57.10	3496.0
58.20	167.0
60.00	702.0
61.00	5835.0
62.10	6306.0
63.10	4816.0
64.00	647.0
65.10	748.0
67.20	311.0
68.00	13039.0
69.10	11145.0
70.20	1066.0
72.00	601.0
73.00	5307.0
74.10	20656.0
75.10	56816.0
76.10	4478.0
76.90	791.0
77.80	845.0
79.00	5608.0
79.90	1661.0
81.00	6448.0
82.00	1121.0
83.00	183.0
85.90	289.0
87.00	5112.0
88.10	5407.0
90.90	672.0
92.20	2874.0
93.00	5469.0
94.10	15674.0
95.10	116576.0
96.10	7674.0
97.00	231.0
103.20	188.0
104.00	891.0
105.00	258.0
105.80	448.0
106.10	423.0
110.80	224.0
112.70	150.0
114.90	336.0
116.00	740.0
117.00	884.0
118.00	589.0
118.90	1190.0
124.00	189.0
125.00	290.0
127.70	519.0
129.10	176.0
130.00	618.0
131.00	395.0
133.10	617.0
134.90	324.0
136.80	180.0
140.90	1529.0
142.10	236.0
143.00	2398.0
144.90	612.0
146.00	244.0
148.10	293.0
149.90	262.0
154.90	504.0
160.90	334.0
171.10	315.0
172.00	912.0
173.00	969.0
174.00	107392.0
175.00	7849.0
176.00	102312.0
177.00	6832.0
178.10	155.0
179.00	413.0
191.10	671.0
193.10	1277.0
195.10	166.0

Instrument :
MSVOA_D
ClientSampleId :
BFB163

207.20	446.0
249.00	466.0
251.00	187.0
265.20	526.0
266.30	151.0
267.20	162.0
281.20	6250.0
282.20	2322.0
283.30	1177.0
284.30	158.0

Instrument :
MSVOA_D
ClientSampleId :
BFB163

m/z	Abundance
36.10	685.0
37.10	3841.0
38.00	3375.0
39.10	1491.0
39.90	1312.0
40.80	153.0
43.10	157.0
44.10	1309.0
45.10	724.0
46.10	351.0
47.20	894.0
47.80	436.0
49.10	3680.0
50.10	17360.0
51.00	5024.0
52.80	199.0
55.10	527.0
56.10	1784.0
57.10	2427.0
59.90	775.0
61.00	4462.0
62.10	4692.0
63.10	4028.0
64.00	343.0
65.10	427.0
67.00	334.0
68.00	9460.0
69.10	8961.0
70.20	925.0
72.10	473.0
73.10	5234.0
74.10	17752.0
75.10	49008.0
76.10	4177.0
77.20	662.0
77.70	329.0
78.10	288.0
79.00	4437.0
79.90	1393.0
81.00	4550.0
82.10	1153.0
82.90	179.0
87.00	5348.0
88.00	5194.0
91.10	463.0
92.10	2583.0
93.10	4693.0
94.00	12336.0
95.10	94600.0
96.10	5971.0
97.10	160.0
103.20	151.0
103.90	606.0
104.90	162.0
106.00	564.0
110.90	153.0
113.00	202.0
115.00	357.0
115.90	487.0
116.90	599.0
118.00	464.0
118.90	701.0
125.60	155.0
127.80	295.0
129.00	298.0
129.80	425.0
132.90	722.0
133.80	219.0
135.00	390.0
136.90	226.0
141.00	1300.0
141.90	248.0
142.90	1710.0
143.90	208.0
145.00	736.0
147.80	338.0
155.00	218.0
157.10	446.0
159.00	240.0
160.80	284.0
171.10	568.0
172.00	1039.0
173.10	1006.0
174.00	89800.0
175.00	6245.0
176.00	91928.0
177.00	6356.0
177.90	248.0
191.20	606.0
192.90	1027.0
194.00	178.0
206.90	234.0

Instrument :
MSVOA_D
ClientSampleId :
BFB163

207.30	250.0
249.20	408.0
250.30	181.0
251.40	248.0
265.10	661.0
266.00	308.0
267.20	226.0
281.30	5559.0
282.10	2013.0
283.20	809.0

Instrument :
MSVOA_D
ClientSampleId :
BFB163