

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092223\
 Data File : VD077201.D
 Acq On : 22 Sep 2023 16:04
 Operator : JC/SY
 Sample : 04527-10
 Misc : 5.03G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EZYY7

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 09/25/2023
 Supervised By :Semsettin Yesilyurt 09/25/2023

Quant Time: Sep 22 23:43:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM090123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 22 23:41:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	262503	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	291944	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	136905	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	115656	17.881	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.520%		
7) Chloroethane-d5	2.799	69	105714	19.874	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.480%		
11) 1,1-Dichloroethene-d2	3.911	65	19142	13.028	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.120%		
21) 2-Butanone-d5	6.981	46	35127	43.108	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.220%		
24) Chloroform-d	7.563	84	144144	20.068	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.280%		
26) 1,2-Dichloroethane-d4	8.234	65	77954	22.898	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.600%		
32) Benzene-d6	8.199	84	295363	18.318	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	73.280%		
36) 1,2-Dichloropropane-d6	9.210	67	97119	21.003	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.000%		
41) Toluene-d8	10.269	98	271865	18.419	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	73.680%		
43) trans-1,3-Dichloroprop...	10.528	79	37699	17.893	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.560%		
47) 2-Hexanone-d5	10.881	63	26415	35.766	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	71.540%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	72210	17.517	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	70.080%		
66) 1,2-Dichlorobenzene-d4	13.816	152	84982	19.339	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	77.360%		
Target Compounds					Qvalue	
13) Acetone	4.022	43	2695m	2.306	ug/L	
16) Methylene chloride	4.805	84	10357m	1.939	ug/L	
25) Chloroform	7.599	83	11948	1.654	ug/L	93
35) Methylcyclohexane	9.269	83	4796	0.669	ug/L #	78
42) Toluene	10.340	91	7767	0.409	ug/L	97
52) Ethylbenzene	11.681	91	1297080	63.096	ug/L	100
53) m,p-Xylene	11.787	106	2892049	364.335	ug/L	96
54) o-Xylene	12.122	106	1034139	134.966	ug/L	99
60) Isopropylbenzene	12.422	105	20087	1.138	ug/L	98
62) 1,3,5-Trimethylbenzene	12.904	105	15105	1.107	ug/L	98
63) 1,2,4-Trimethylbenzene	13.210	105	44748	3.347	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092223\
Data File : VD077201.D
Acq On : 22 Sep 2023 16:04
Operator : JC/SY
Sample : 04527-10
Misc : 5.03G/10.0ml/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_D
ClientSampleId :
EZY7

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 09/25/2023
Supervised By :Semsettin Yesilyurt 09/25/2023

Quant Time: Sep 22 23:43:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM090123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 22 23:41:10 2023
Response via : Initial Calibration

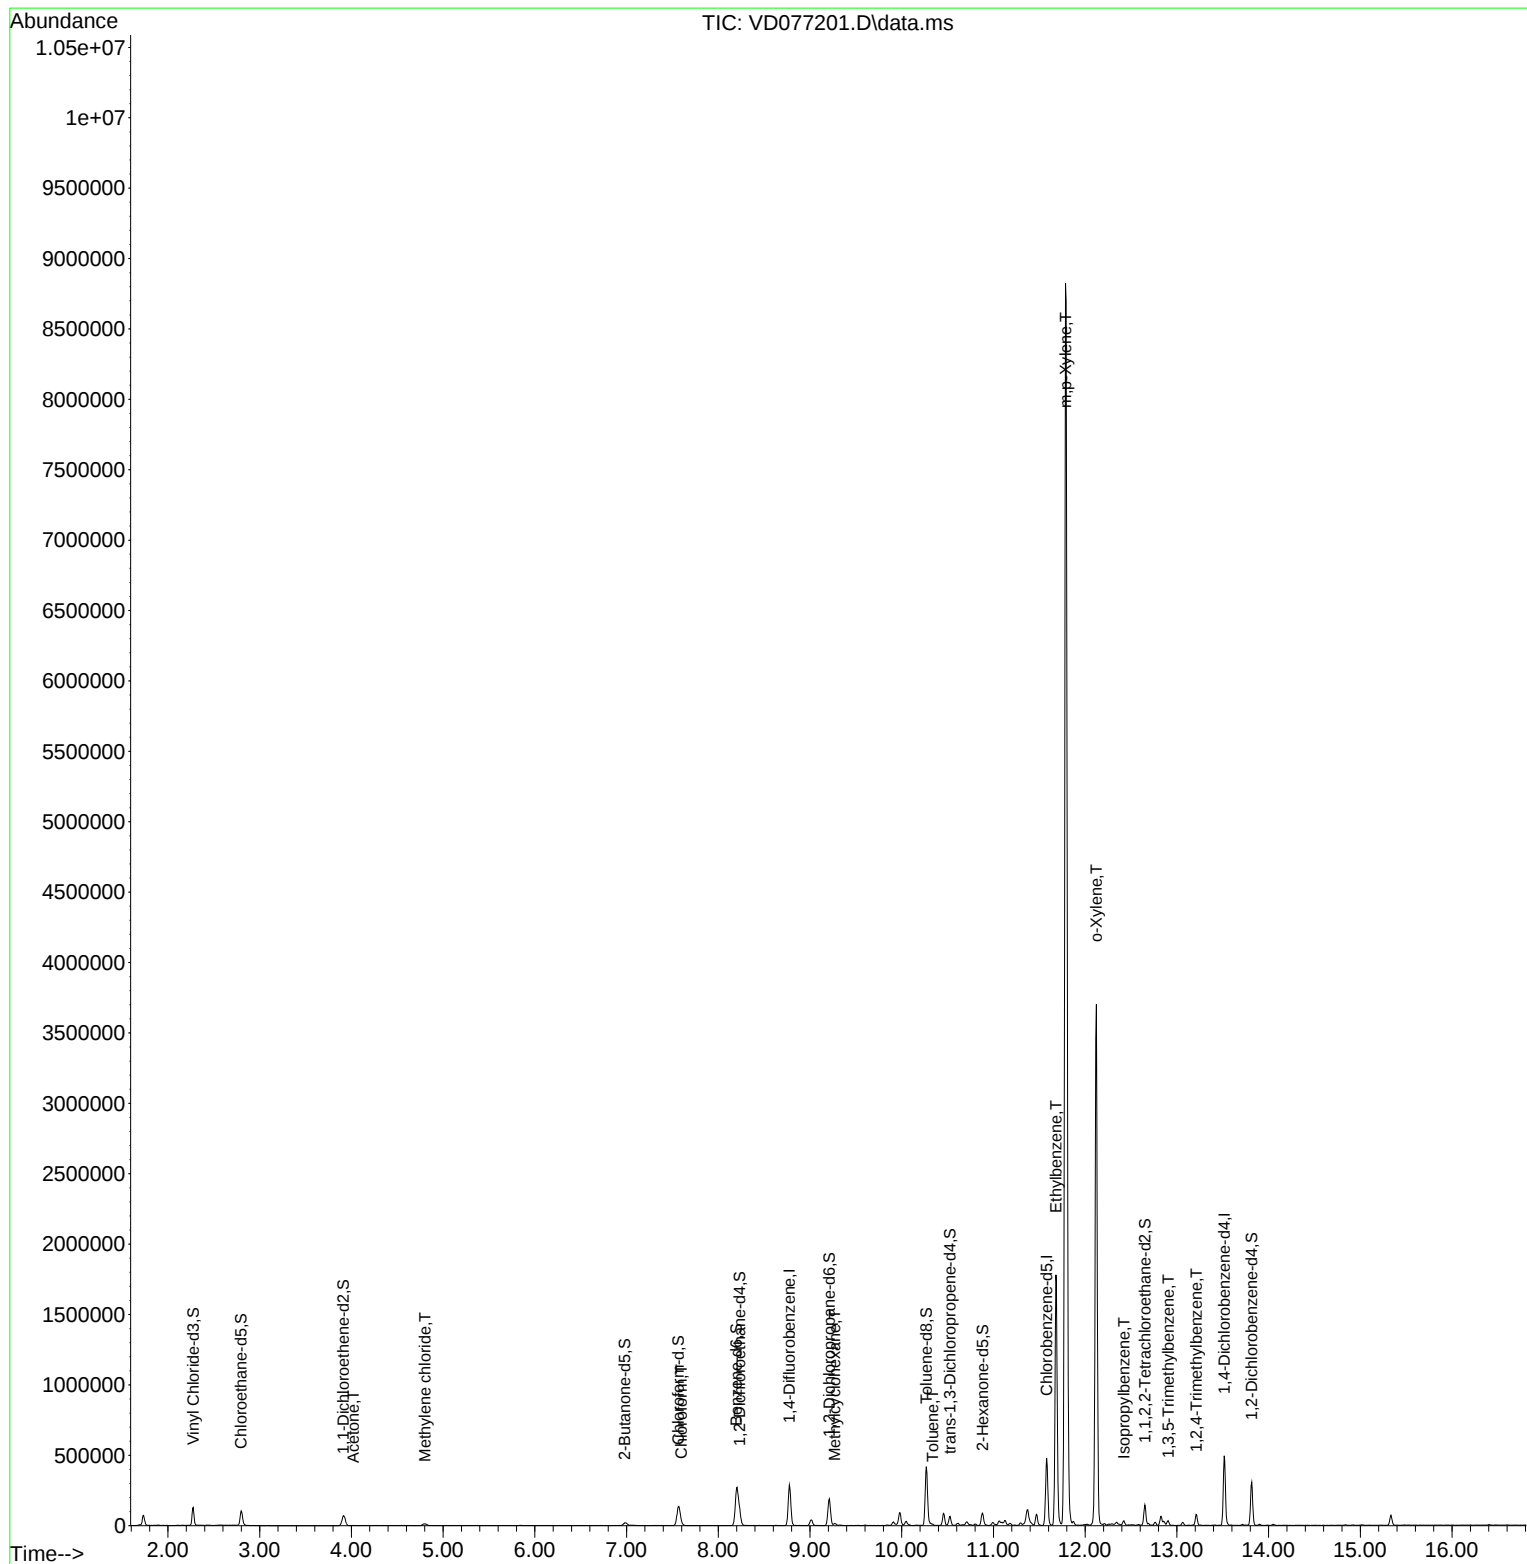

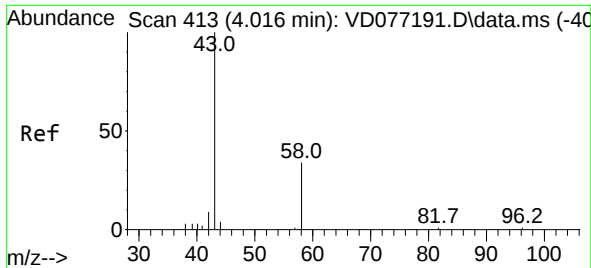

#13

Acetone

Concen: 2.306 ug/L m

RT: 4.022 min Scan# 41

Delta R.T. 0.006 min

Lab File: VD077201.D

Acq: 22 Sep 2023 16:04

Instrument :

MSVOA_D

ClientSampleId :

EZYY7

Tgt Ion: 43 Resp: 269

Ion Ratio Lower Upper

43 100





58 13.1 0.0 71.8

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 09/25/2023

Supervised By :Semsettin Yesilyurt 09/25/2023

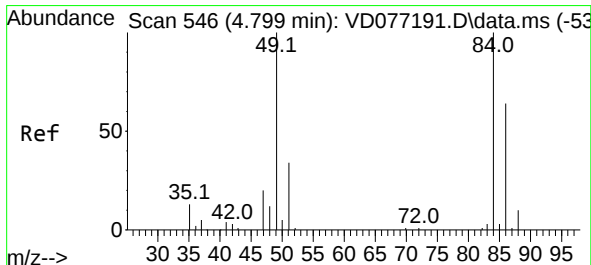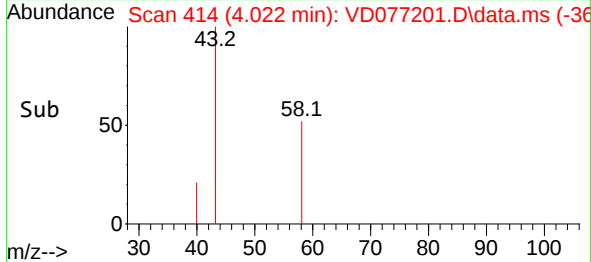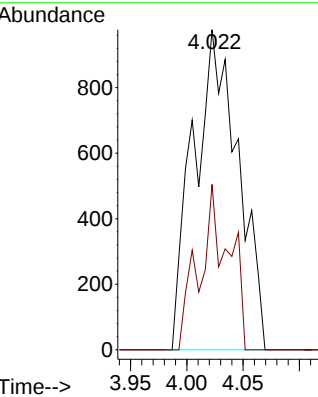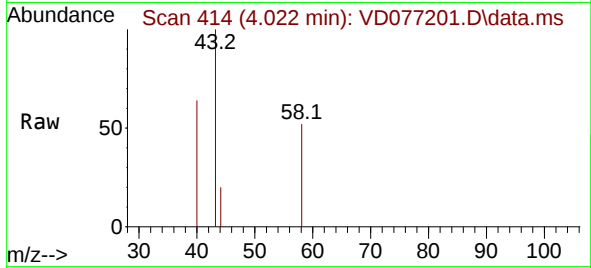

#16

Methylene chloride

Concen: 1.939 ug/L m

RT: 4.805 min Scan# 547

Delta R.T. 0.006 min

Lab File: VD077201.D

Acq: 22 Sep 2023 16:04




Tgt Ion: 84 Resp: 10357


Ion Ratio Lower Upper

84 100

86 69.9 45.3 84.1

49 98.8 69.2 128.6

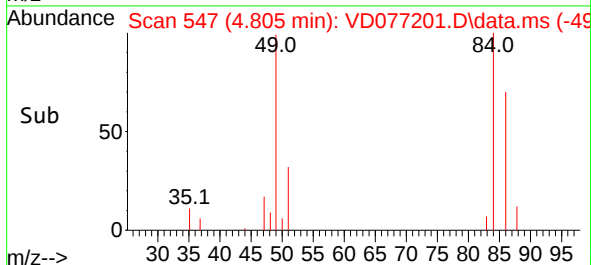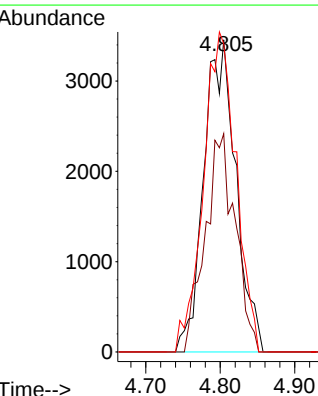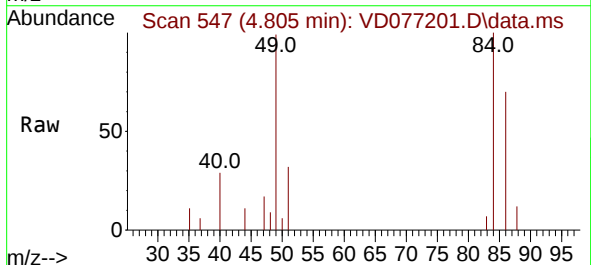

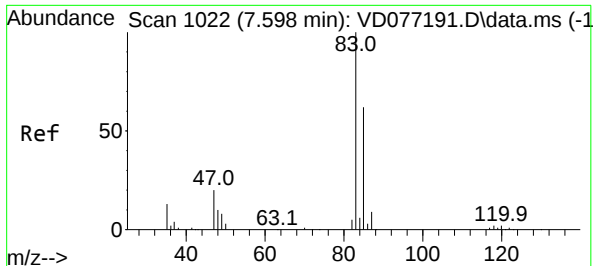





#25
Chloroform
Concen: 1.654 ug/L
RT: 7.599 min Scan# 1022
Delta R.T. 0.000 min
Lab File: VD077201.D
Acq: 22 Sep 2023 16:04

Instrument :
MSVOA_D
ClientSampleId :
EZY7

Tgt Ion: 83 Resp: 11948
Ion Ratio Lower Upper
83 100
85 60.6 46.2 85.8




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 09/25/2023
Supervised By :Semsettin Yesilyurt 09/25/2023

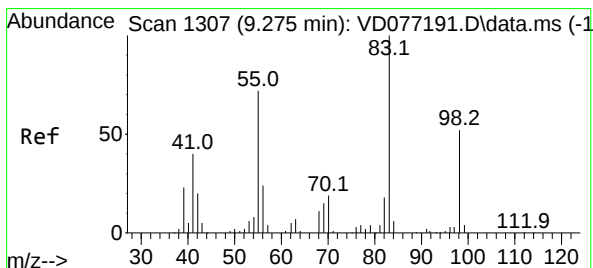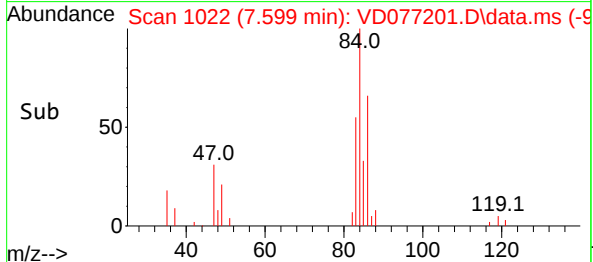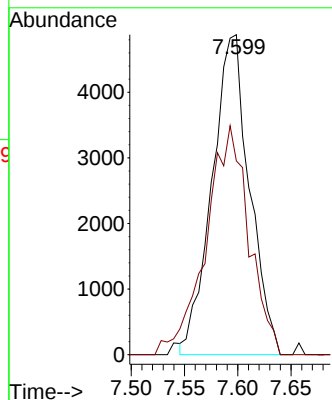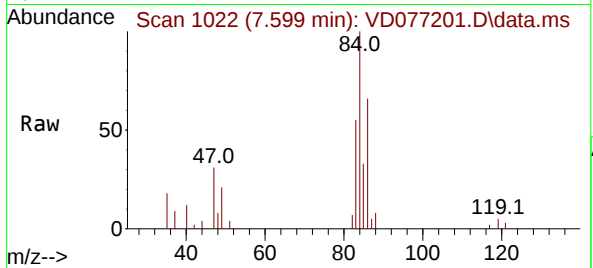

#35
Methylcyclohexane
Concen: 0.669 ug/L
RT: 9.269 min Scan# 1306
Delta R.T. -0.006 min
Lab File: VD077201.D
Acq: 22 Sep 2023 16:04

Tgt Ion: 83 Resp: 4796
Ion Ratio Lower Upper
83 100
55 78.3 51.5 77.3#
98 32.1 40.7 61.1#

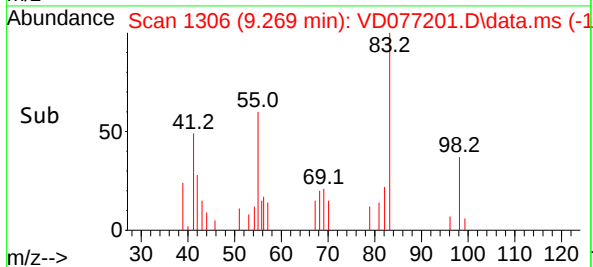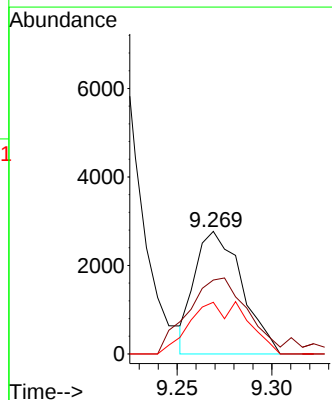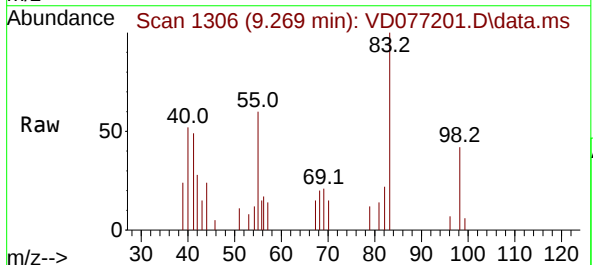

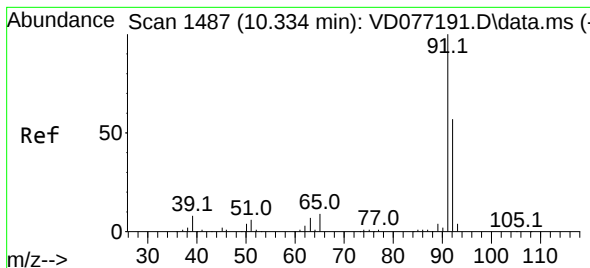

#42

Toluene

Concen: 0.409 ug/L

RT: 10.340 min Scan# 1487

Delta R.T. 0.006 min

Lab File: VD077201.D

Acq: 22 Sep 2023 16:04

Instrument :

MSVOA_D

ClientSampleId :

EZYY7

Tgt Ion: 91 Resp: 776

Ion Ratio Lower Upper

91 100





92 60.5 40.8 75.8

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 09/25/2023

Supervised By :Semsettin Yesilyurt 09/25/2023

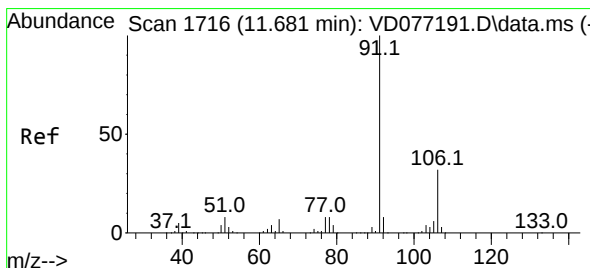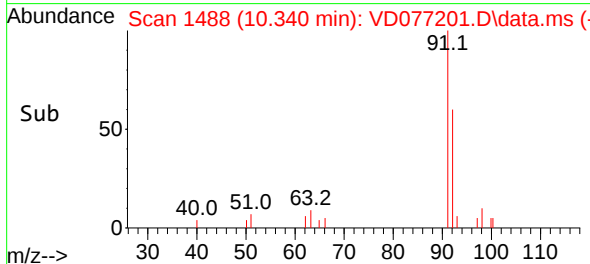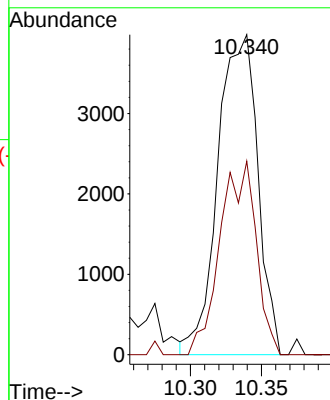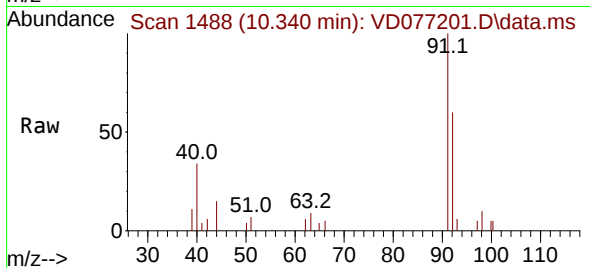

#52

Ethylbenzene

Concen: 63.096 ug/L

RT: 11.681 min Scan# 1716

Delta R.T. 0.000 min

Lab File: VD077201.D




Acq: 22 Sep 2023 16:04


Tgt Ion: 91 Resp: 1297080

Ion Ratio Lower Upper

91 100


106 31.9 22.1 41.1

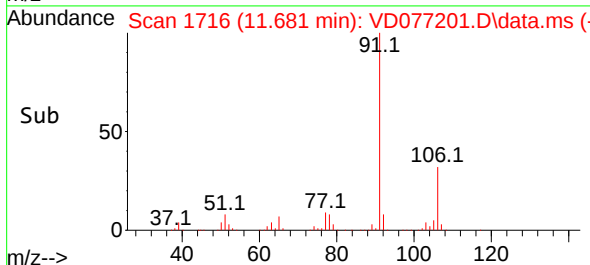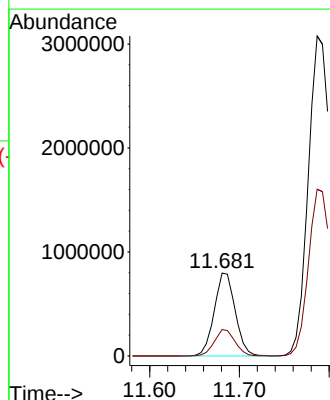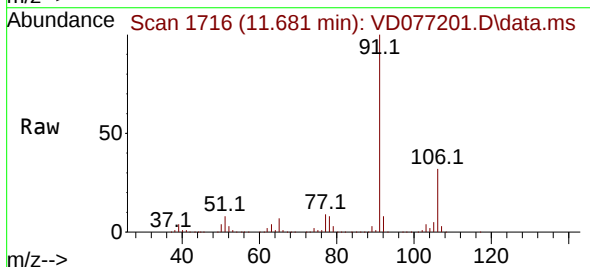

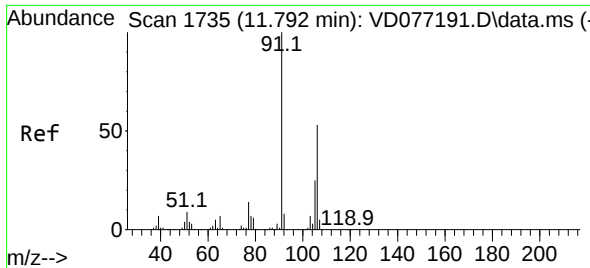

#53
m,p-Xylene
Concen: 364.335 ug/L
RT: 11.787 min Scan# 1734
Delta R.T. -0.006 min
Lab File: VD077201.D
Acq: 22 Sep 2023 16:04




Instrument :
MSVOA_D
ClientSampleId :
EZY7

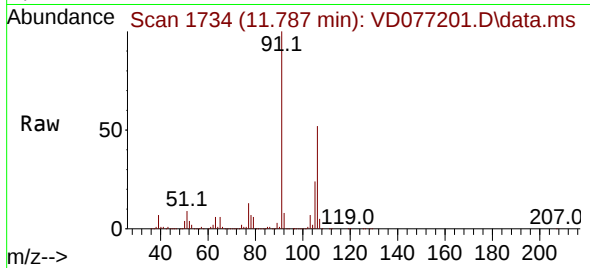

Tgt Ion:106 Resp: 2892049
Ion Ratio Lower Upper
106 100
91 191.9 138.2 256.6




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 09/25/2023
Supervised By :Semsettin Yesilyurt 09/25/2023

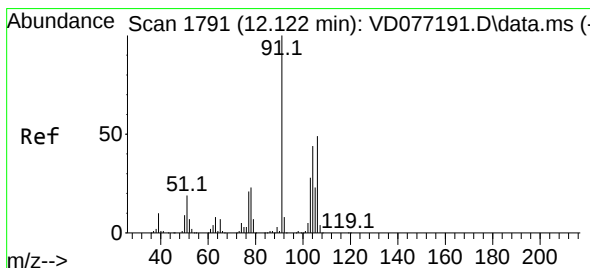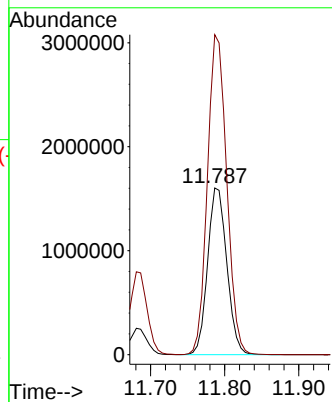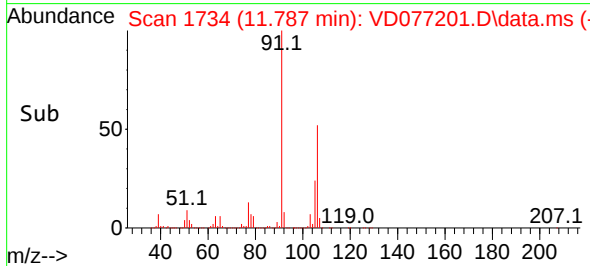

#54
o-Xylene
Concen: 134.966 ug/L
RT: 12.122 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VD077201.D
Acq: 22 Sep 2023 16:04


Tgt Ion:106 Resp: 1034139
Ion Ratio Lower Upper
106 100
91 208.7 146.9 272.7

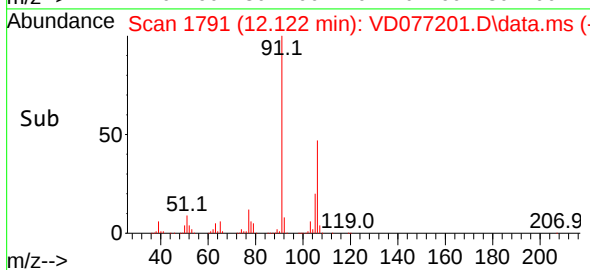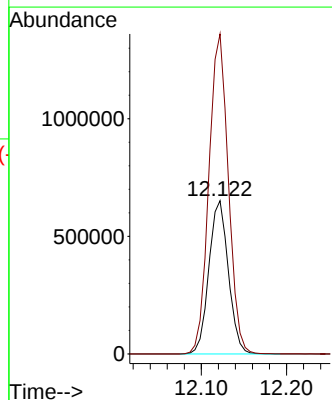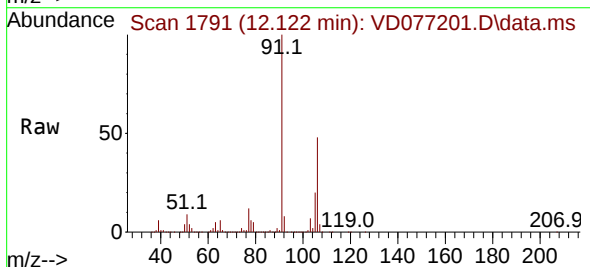

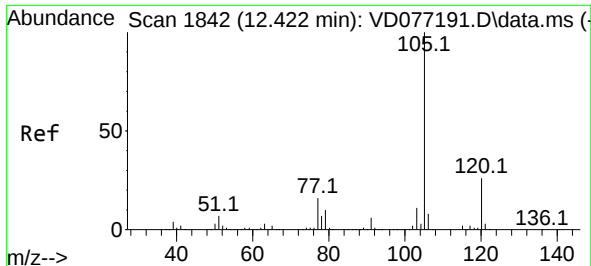

#60
Isopropylbenzene
Concen: 1.138 ug/L
RT: 12.422 min Scan# 1842
Delta R.T. 0.000 min
Lab File: VD077201.D
Acq: 22 Sep 2023 16:04




Instrument :
MSVOA_D
ClientSampleId :
EZY7

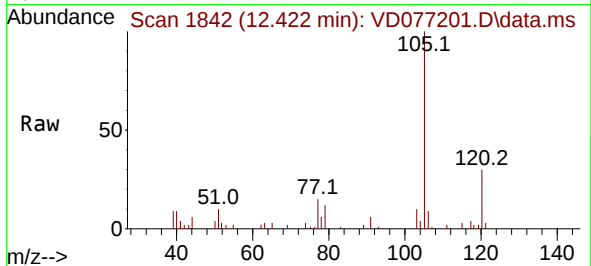


Tgt Ion:105 Resp: 2085
Ion Ratio Lower Upper
105 100
120 28.3 21.8 32.6
77 15.7 11.9 17.9

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 09/25/2023
Supervised By :Semsettin Yesilyurt 09/25/2023

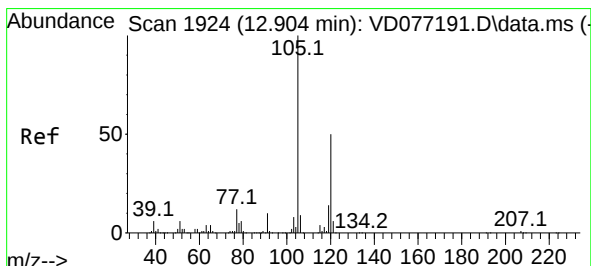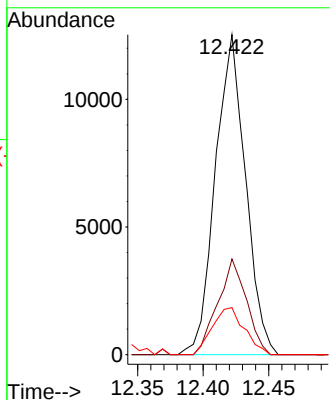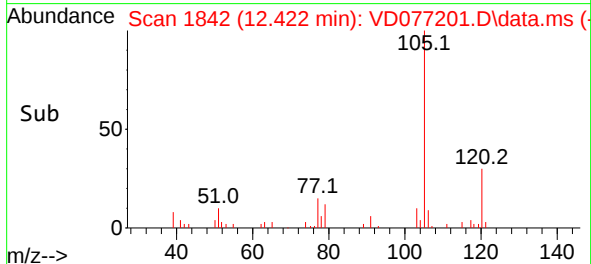


#62
1,3,5-Trimethylbenzene
Concen: 1.107 ug/L
RT: 12.904 min Scan# 1924
Delta R.T. 0.000 min
Lab File: VD077201.D
Acq: 22 Sep 2023 16:04

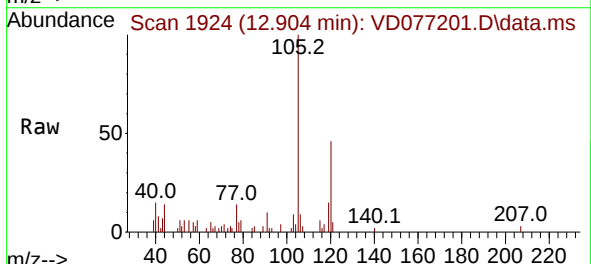


Tgt Ion:105 Resp: 15105
Ion Ratio Lower Upper
105 100
120 51.5 40.2 60.2

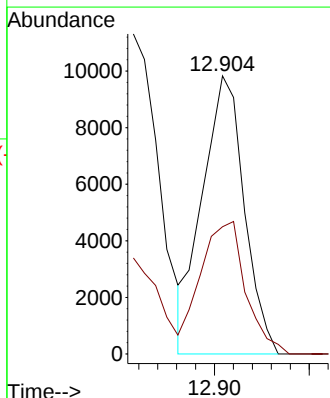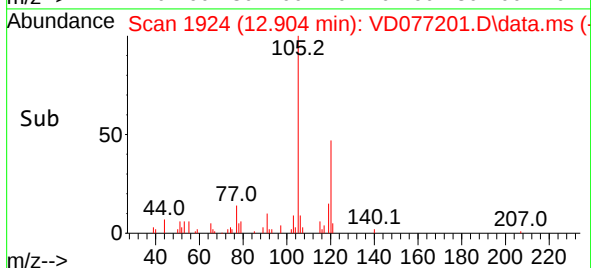

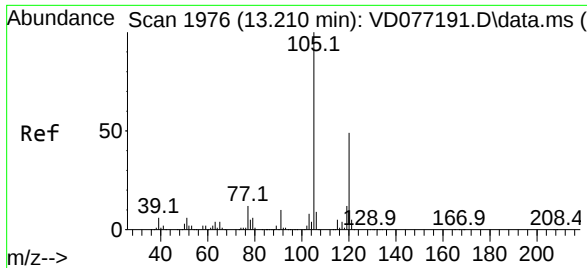

#63
 1,2,4-Trimethylbenzene
 Concen: 3.347 ug/L
 RT: 13.210 min Scan# 1976
 Delta R.T. 0.000 min
 Lab File: VD077201.D
 Acq: 22 Sep 2023 16:04

Instrument : MSVOA_D
 ClientSampleId : EZZY7

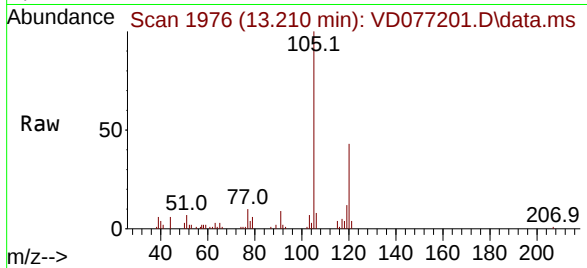

Tgt Ion:105 Resp: 44748
 Ion Ratio Lower Upper
 105 100
 120 43.0 37.8 56.8

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 09/25/2023
 Supervised By :Semsettin Yesilyurt 09/25/2023

