

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD092420\
 Data File : VD066844.D
 Acq On : 24 Sep 2020 12:03
 Operator : VA/SY
 Sample : L4125-01
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CS-19

Quant Time: Sep 25 01:29:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 23 01:34:05 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	417719	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.86	114	736236	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	727018	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	339394	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	219232	53.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.24%	
35) Dibromofluoromethane	7.91	113	236092	50.40	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.80%	
50) Toluene-d8	10.34	98	887927	55.64	ug/l	0.00
Spiked Amount 50.000			Recovery	=	111.28%	
62) 4-Bromofluorobenzene	12.63	95	311200	56.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	113.92%	
Target Compounds						
16) Acetone	4.16	43	36715	42.332	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD092420\
Data File : VD066844.D
Acq On : 24 Sep 2020 12:03
Operator : VA/SY
Sample : L4125-01
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CS-19

Quant Time: Sep 25 01:29:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 23 01:34:05 2020
Response via : Initial Calibration

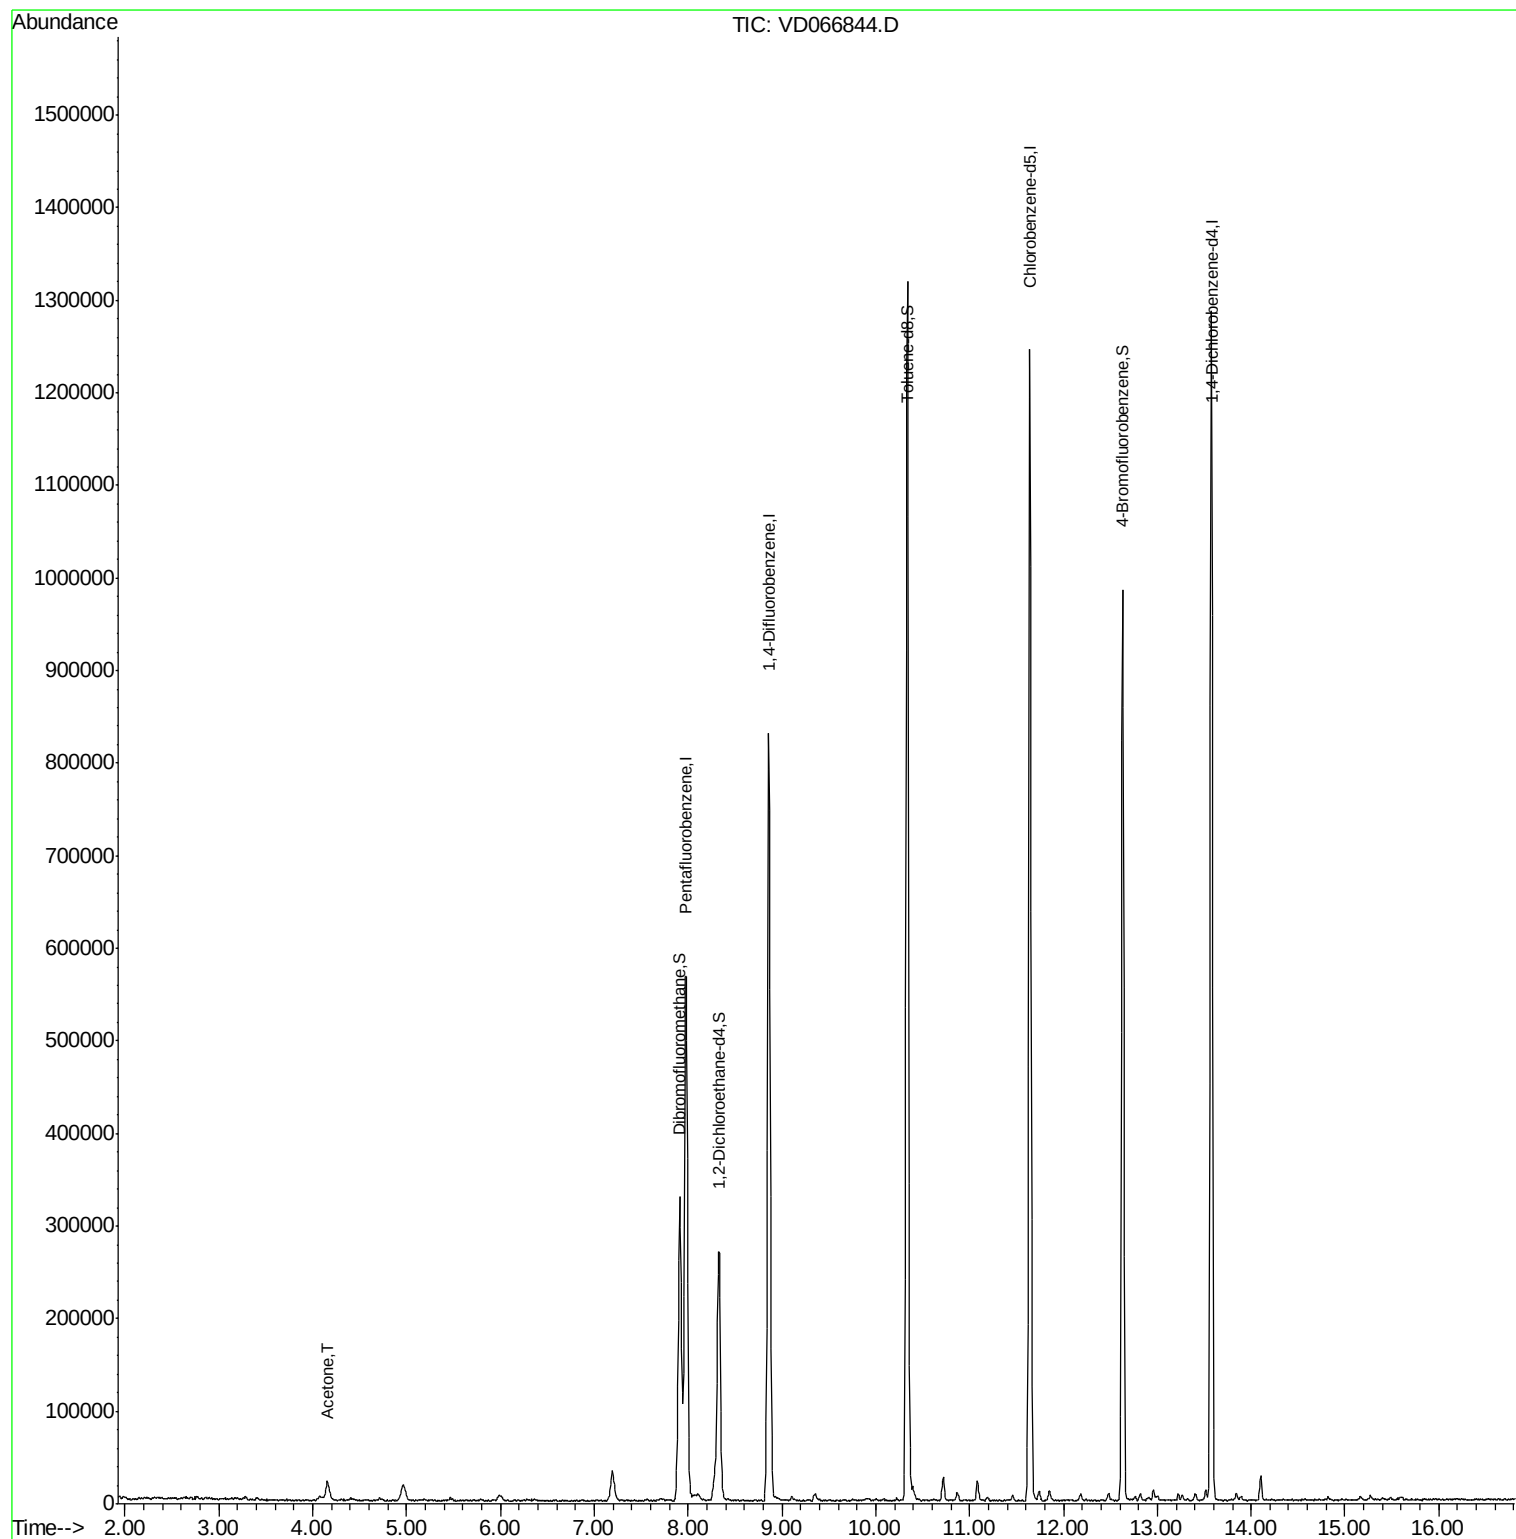

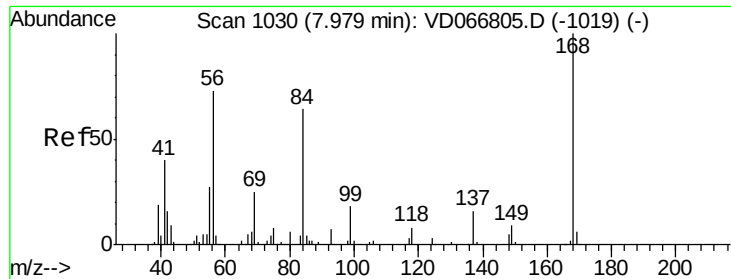

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VD066844.D

Acq: 24 Sep 2020 12:03

Instrument :

MSVOA_D

ClientSampleId :


CS-19

Tot Ion:168 Resp: 417719

Ion Ratio Lower Upper

168 100

99 60.6 46.6 69.8

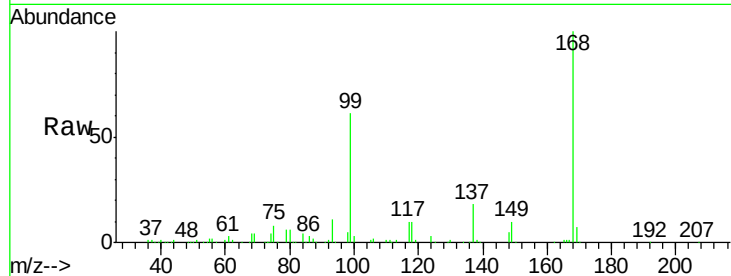

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

200000



150000

100000

50000

0

Time-->

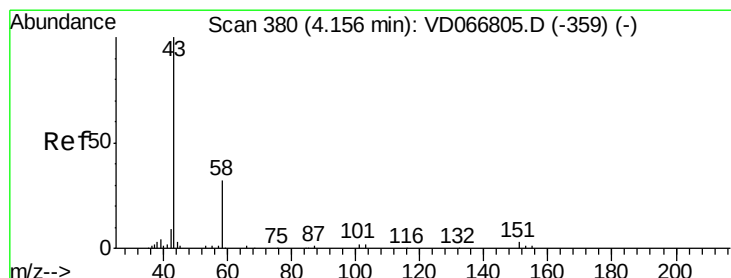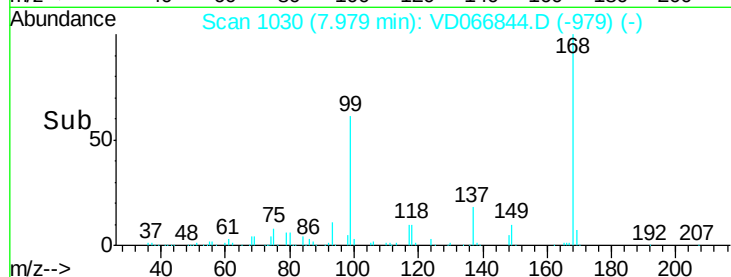

#16

Acetone

Concen: 42.332 ug/l

RT: 4.16 min Scan# 380

Delta R.T. 0.00 min

Lab File: VD066844.D


Acq: 24 Sep 2020 12:03

Tgt Ion: 43 Resp: 36715

Ion Ratio Lower Upper

43 100

58 29.7 25.6 38.4

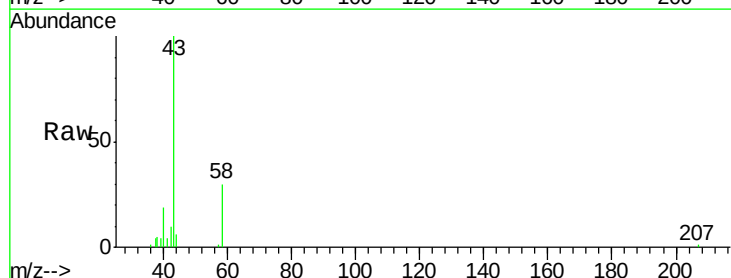

Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 58.00 (57.70 to 58.70): VDC

4.16


15000


10000

5000

0

Time-->




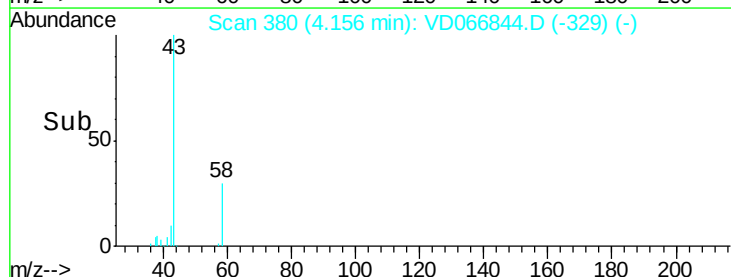


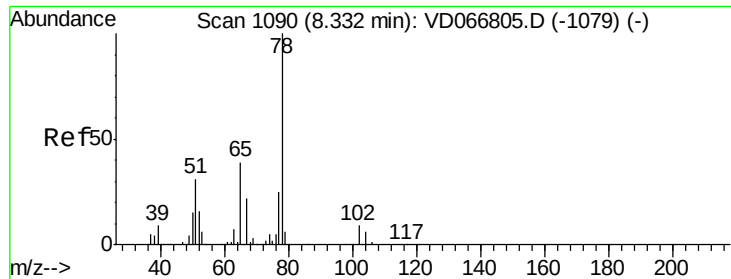

#33
 1,2-Dichloroethane-d4
 Concen: 53.622 ug/l
 RT: 8.33 min Scan# 1090
 Delta R.T. 0.00 min
 Lab File: VD066844.D
 Acq: 24 Sep 2020 12:03




Instrument :
 MSVOA_D
 ClientSampled :
 CS-19


Tot Ion: 65 Resp: 219232
 Ion Ratio Lower Upper
 65 100
 67 52.1 0.0 107.2

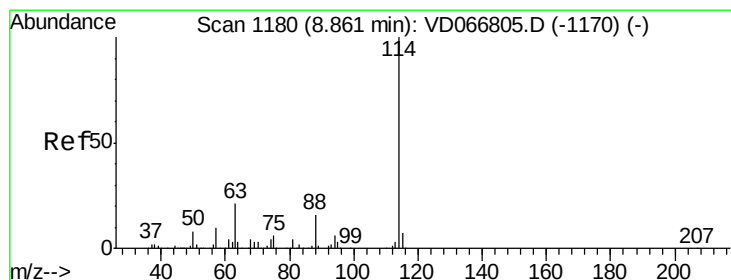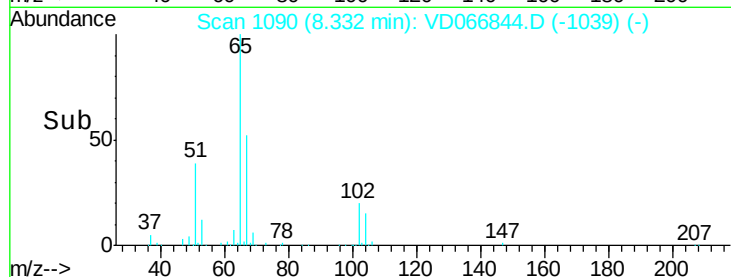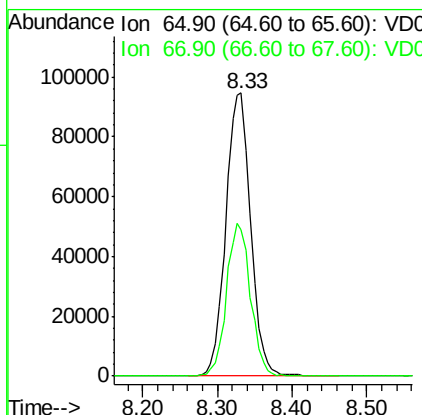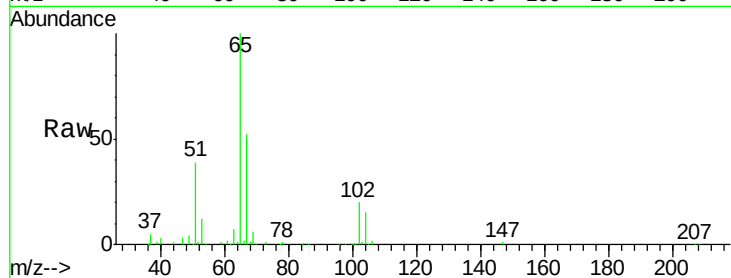

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.86 min Scan# 1180
 Delta R.T. 0.00 min
 Lab File: VD066844.D
 Acq: 24 Sep 2020 12:03

Tgt Ion: 114 Resp: 736236
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 42.6
 88 15.5 0.0 32.6

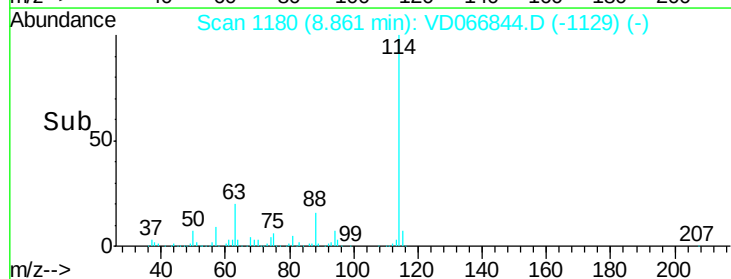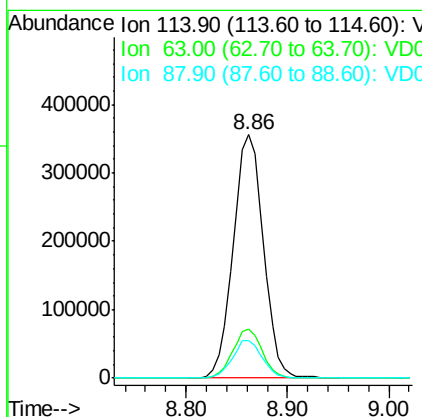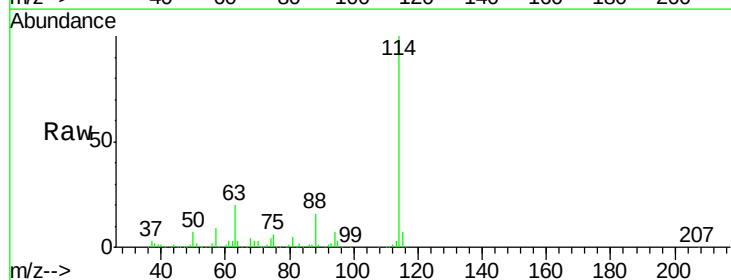


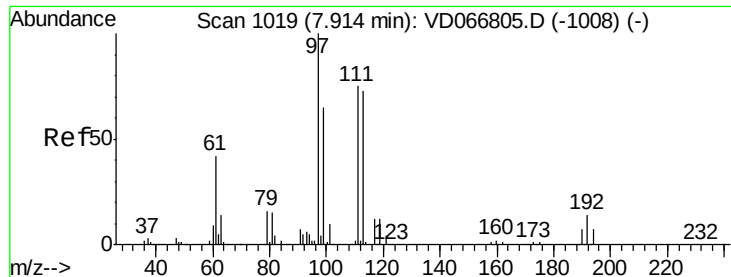




#35
 Dibromofluoromethane
 Concen: 50.405 ug/l
 RT: 7.91 min Scan# 1019
 Delta R.T. 0.00 min
 Lab File: VD066844.D
 Acq: 24 Sep 2020 12:03

Instrument :
 MSVOA_D
 ClientSampleId :
 CS-19

Tot Ion	Ratio	Lower	Upper
113	100		
111	100.8	81.8	122.8
192	18.4	14.4	21.6

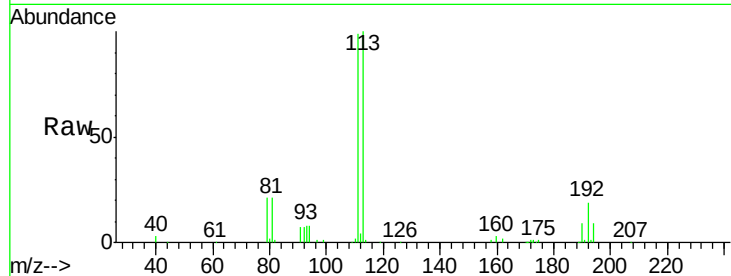


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

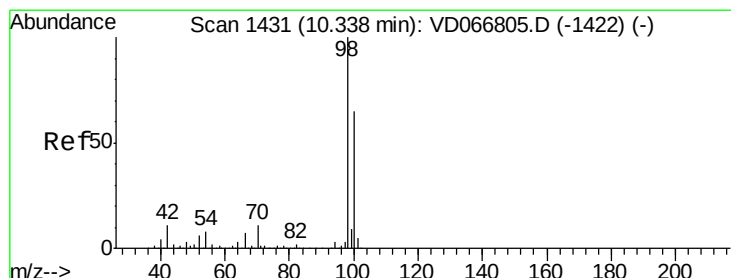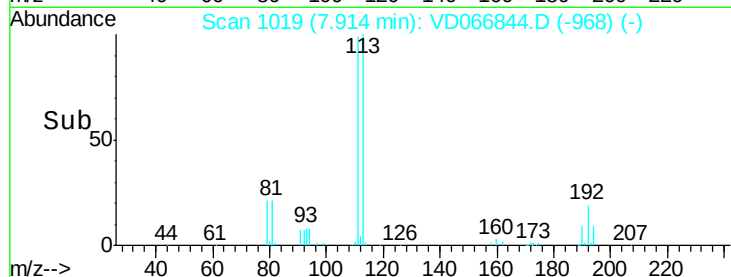
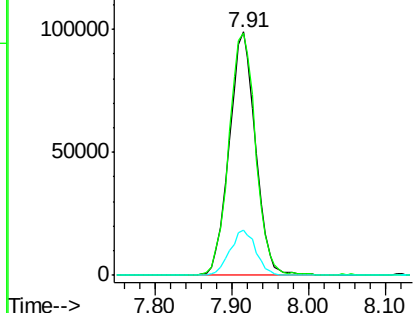



#50
 Toluene-d8
 Concen: 55.638 ug/l
 RT: 10.34 min Scan# 1431
 Delta R.T. 0.00 min
 Lab File: VD066844.D
 Acq: 24 Sep 2020 12:03

Tgt Ion	Ratio	Lower	Upper
98	100		
100	66.0	52.2	78.2

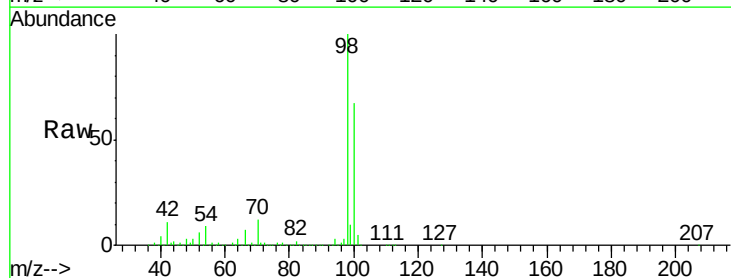

Abundance Ion 98.00 (97.70 to 98.70): VDC
 Ion 100.00 (99.70 to 100.70): VDC



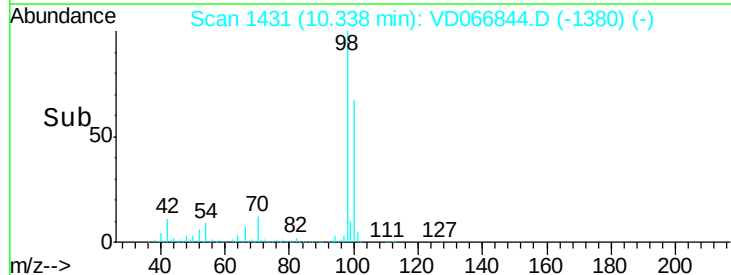
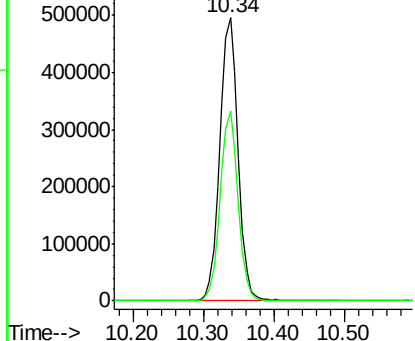


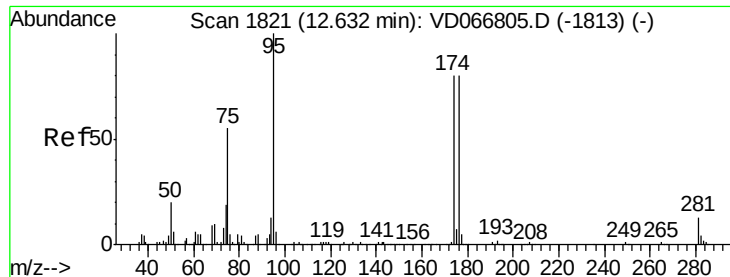

#62
4-Bromofluorobenzene
Concen: 56.962 ug/l
RT: 12.63 min Scan# 1821
Delta R.T. 0.00 min
Lab File: VD066844.D
Acq: 24 Sep 2020 12:03




Instrument :
MSVOA_D
ClientSampleId :
CS-19


Tot Ion: 95 Resp: 311200
Ion Ratio Lower Upper
95 100
174 79.7 0.0 159.8
176 76.3 0.0 154.4

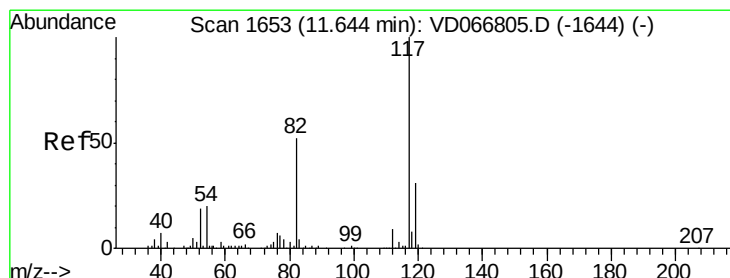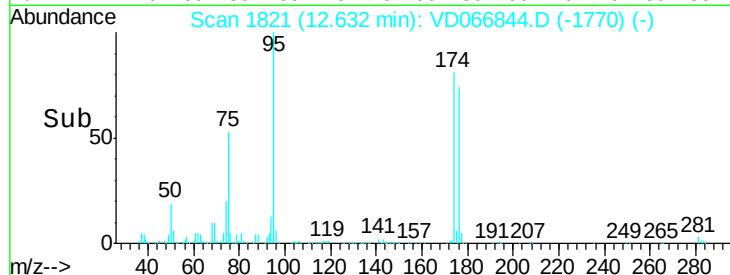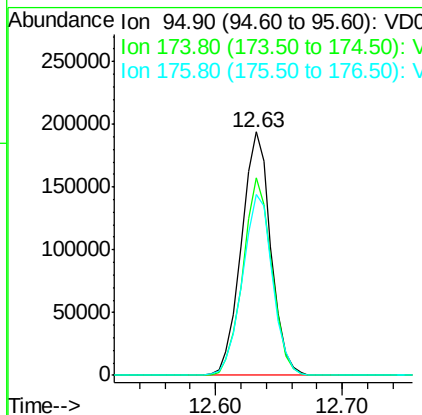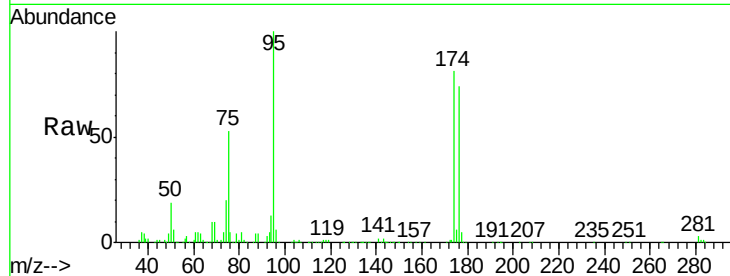

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.64 min Scan# 1653
Delta R.T. 0.00 min
Lab File: VD066844.D
Acq: 24 Sep 2020 12:03

Tgt Ion: 117 Resp: 727018
Ion Ratio Lower Upper
117 100
82 54.5 41.8 62.6
119 32.1 24.6 37.0

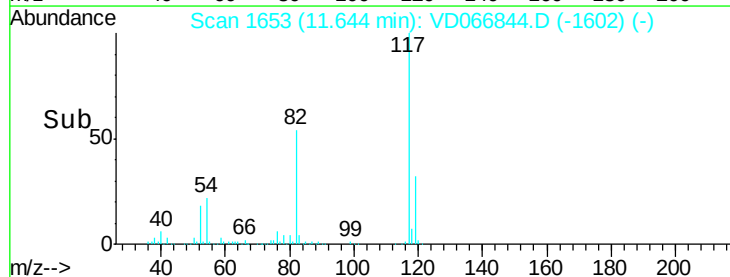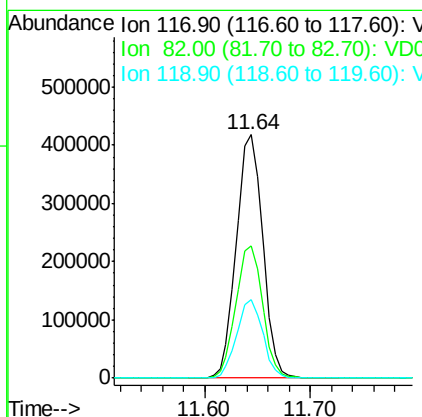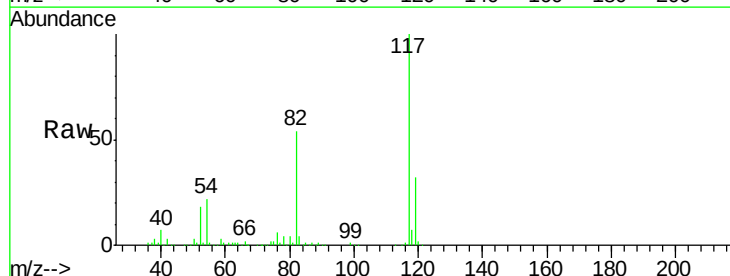

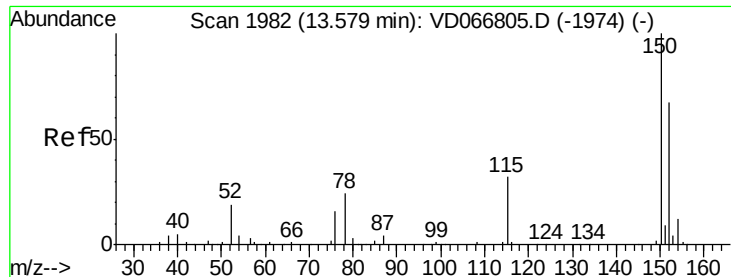

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1982

Delta R.T. 0.00 min

Lab File: VD066844.D

Acq: 24 Sep 2020 12:03

Instrument :

MSVOA_D

ClientSampleId :

CS-19


Tot Ion:152 Resp: 339394

Ion Ratio Lower Upper

152 100

115 58.9 30.3 91.0

150 156.6 0.0 346.2

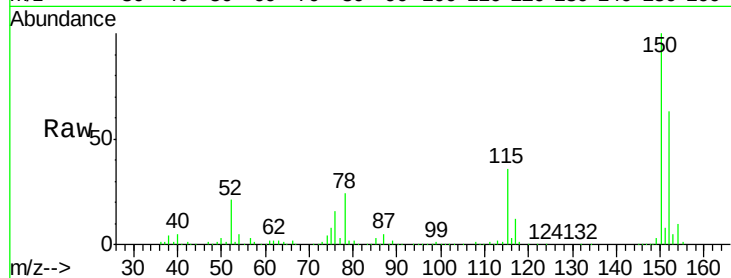

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

