

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD092420\
 Data File : VD066848.D
 Acq On : 24 Sep 2020 13:53
 Operator : VA/SY
 Sample : L4125-05
 Misc : 5.02G/5.00ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CS-23

Quant Time: Sep 25 01:47:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 23 01:34:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	403180	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.86	114	732083	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	730434	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	336414	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	220551	55.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.78%	
35) Dibromofluoromethane	7.91	113	237659	51.03	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.06%	
50) Toluene-d8	10.34	98	886767	55.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.76%	
62) 4-Bromofluorobenzene	12.63	95	307692	56.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	113.28%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD092420\
Data File : VD066848.D
Acq On : 24 Sep 2020 13:53
Operator : VA/SY
Sample : L4125-05
Misc : 5.02G/5.00ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CS-23

Quant Time: Sep 25 01:47:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 23 01:34:05 2020
Response via : Initial Calibration

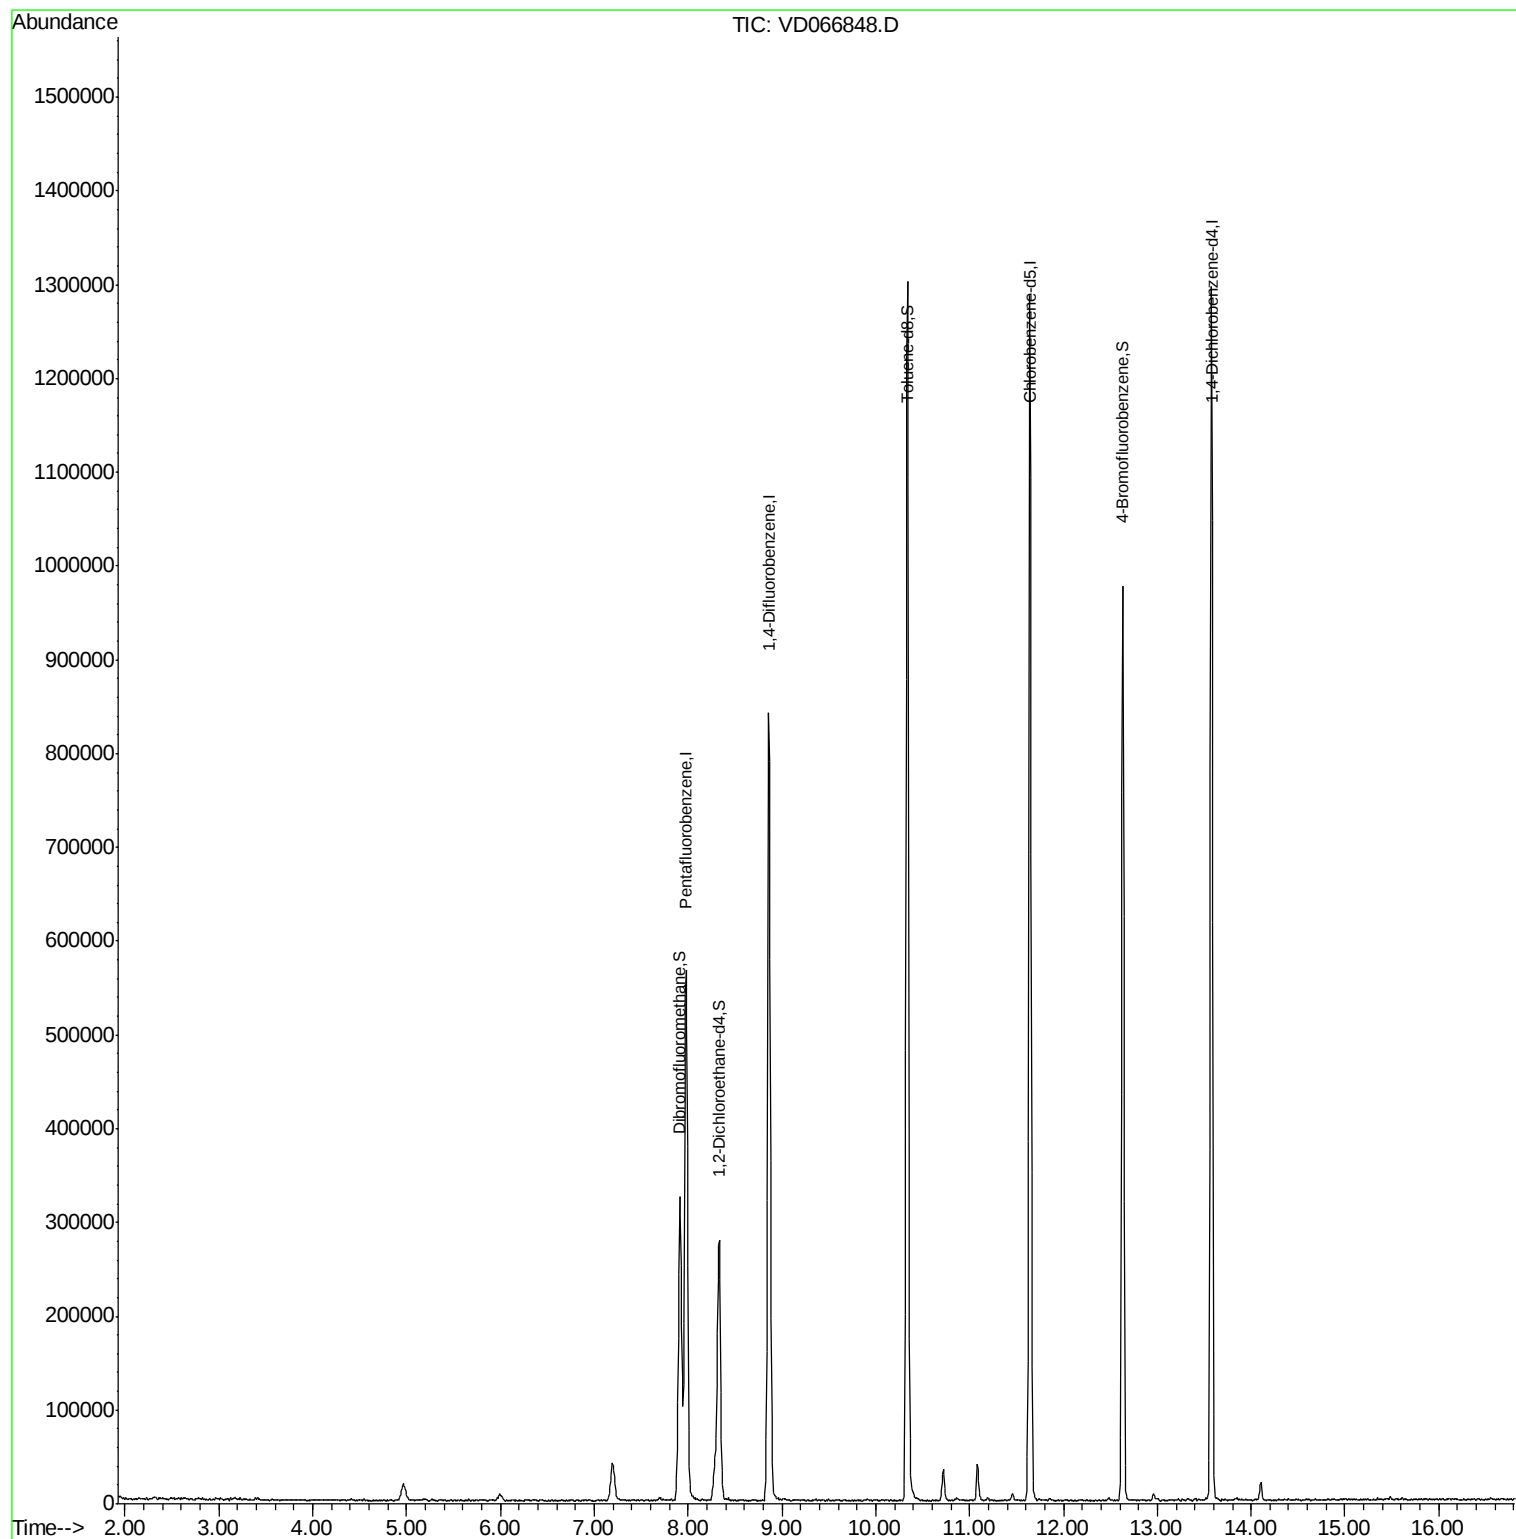

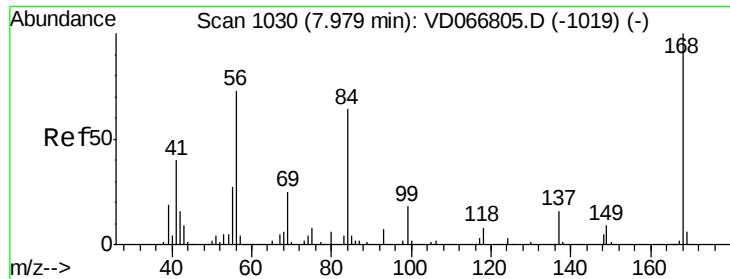

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VD066848.D

Acq: 24 Sep 2020 13:53

Instrument :

MSVOA_D

ClientSampled :


CS-23

Tot Ion:168 Resp: 403180

Ion Ratio Lower Upper

168 100

99 58.6 46.6 69.8

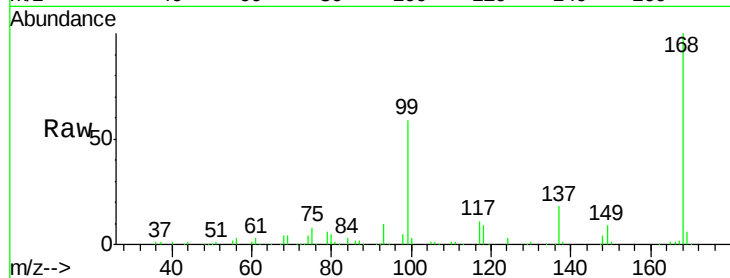

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

200000

150000



100000

50000

0

Time-->

7.90 8.00 8.10

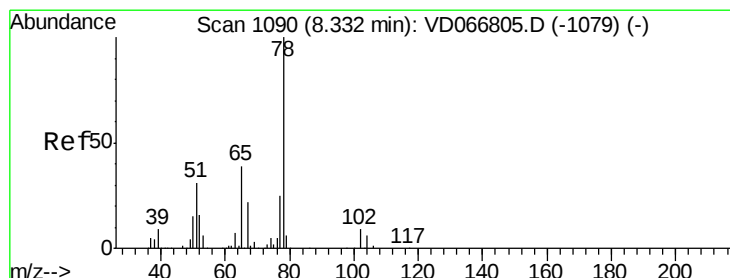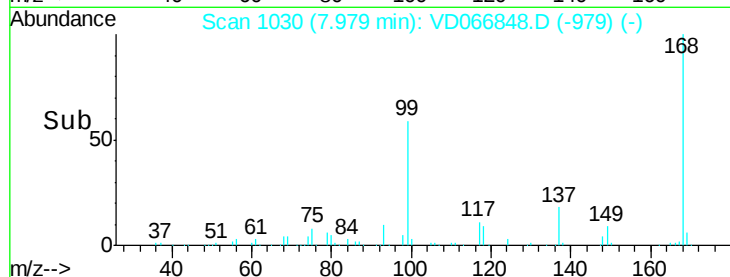

#33

1,2-Dichloroethane-d4

Concen: 55.890 ug/l

RT: 8.33 min Scan# 1089

Delta R.T. -0.01 min

Lab File: VD066848.D


Acq: 24 Sep 2020 13:53

Tgt Ion: 65 Resp: 220551

Ion Ratio Lower Upper

65 100

67 53.4 0.0 107.2

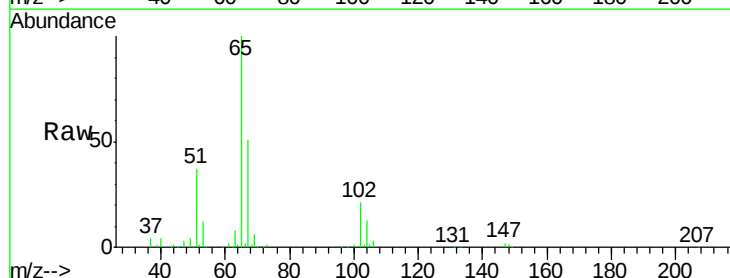

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

100000

80000

60000


40000


20000

0

Time-->

8.25 8.30 8.35 8.40

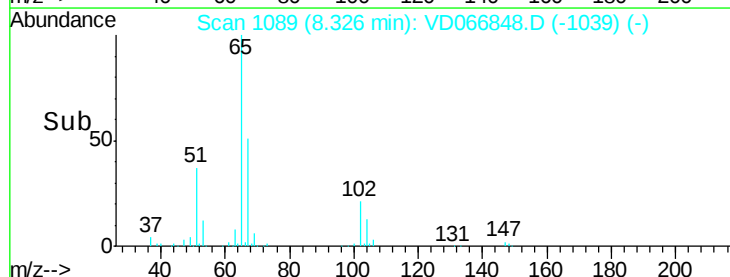


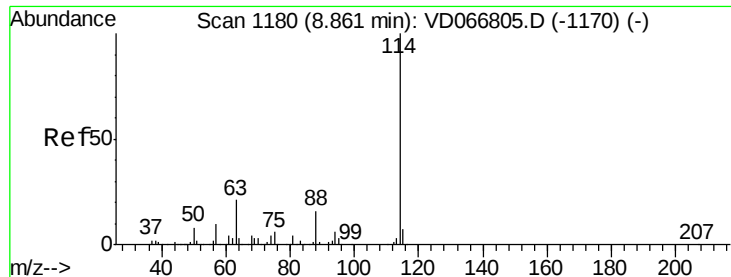




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.86 min Scan# 1180
Delta R.T. -0.00 min
Lab File: VD066848.D
Acq: 24 Sep 2020 13:53

Instrument :
MSVOA_D
ClientSampleId :
CS-23

Tot Ion	Ratio	Lower	Upper
114	100		
63	20.5	0.0	42.6
88	15.1	0.0	32.6

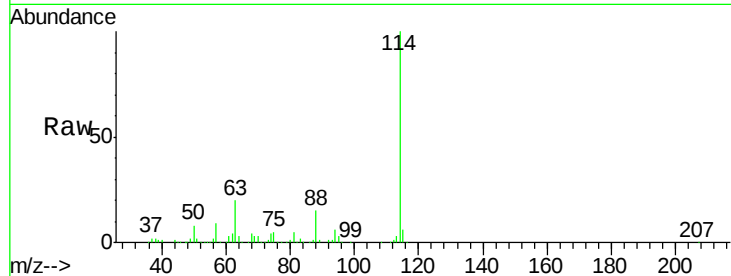


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): V
Ion 87.90 (87.60 to 88.60): V

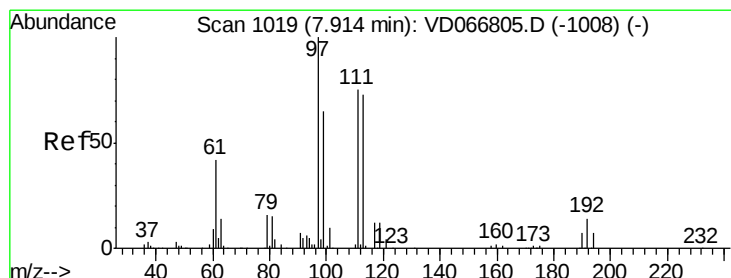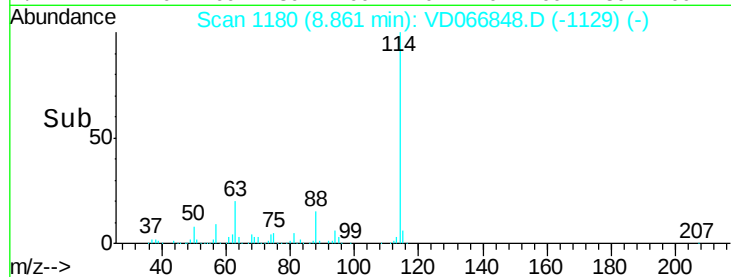
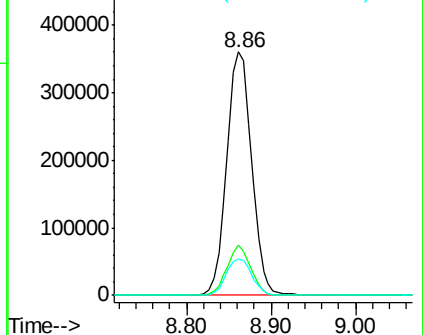



#35
Dibromofluoromethane
Concen: 51.027 ug/l
RT: 7.91 min Scan# 1019
Delta R.T. 0.00 min
Lab File: VD066848.D
Acq: 24 Sep 2020 13:53

Tgt Ion	Ratio	Lower	Upper
113	100		
111	100.5	81.8	122.8
192	18.2	14.4	21.6

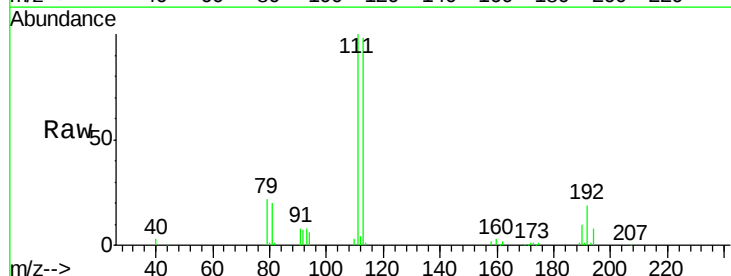

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



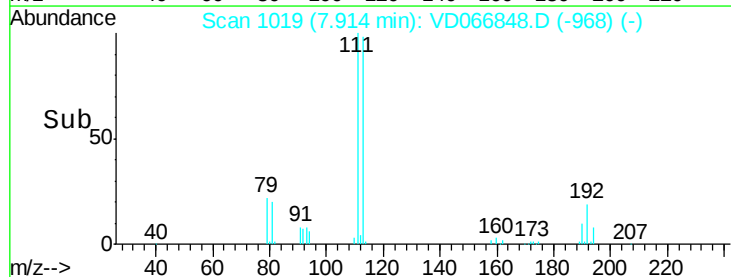
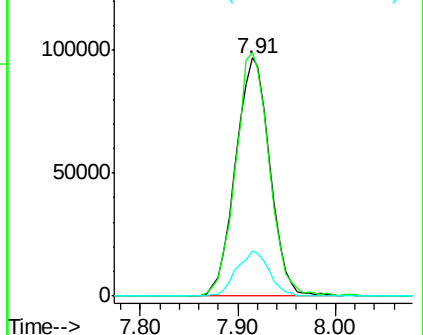


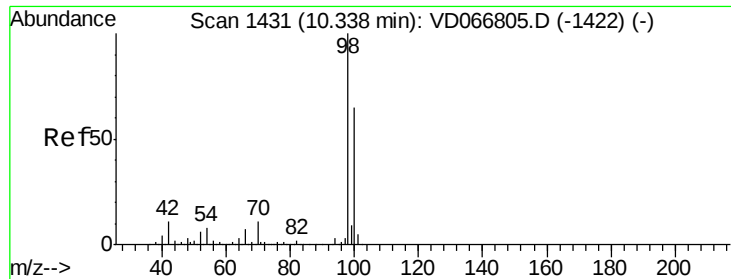

#50
Toluene-d8
Concen: 55.881 ug/l
RT: 10.34 min Scan# 1431
Delta R.T. 0.00 min
Lab File: VD066848.D
Acq: 24 Sep 2020 13:53




Instrument :
MSVOA_D
ClientSampled :
CS-23


Tot Ion: 98 Resp: 886767
Ion Ratio Lower Upper
98 100
100 65.4 52.2 78.2

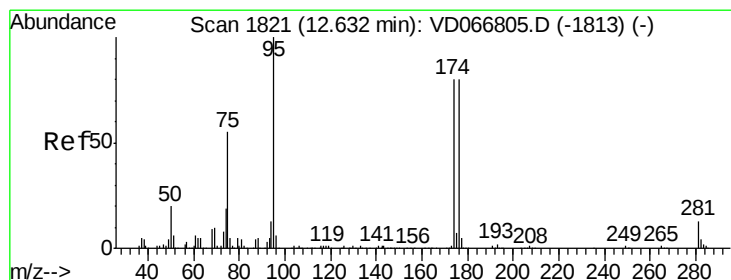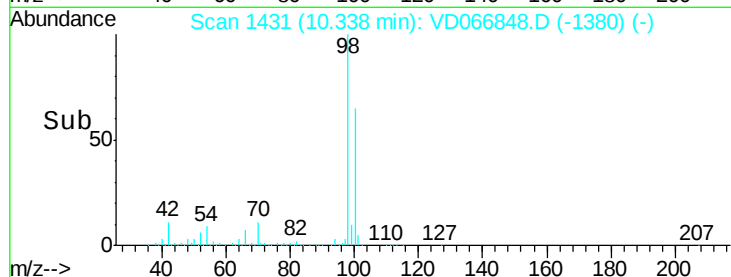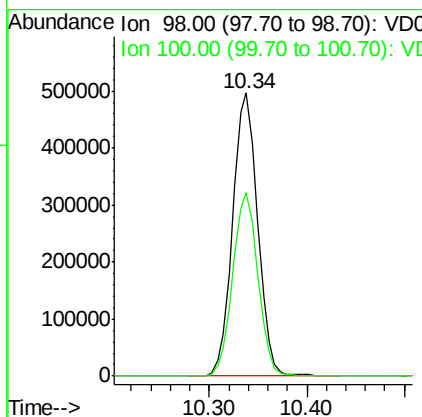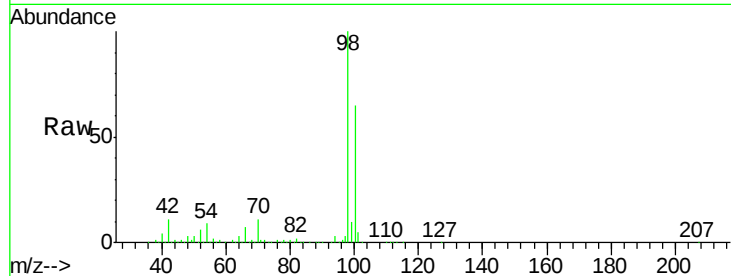

#62
4-Bromofluorobenzene
Concen: 56.639 ug/l
RT: 12.63 min Scan# 1821
Delta R.T. 0.00 min
Lab File: VD066848.D
Acq: 24 Sep 2020 13:53

Tgt Ion: 95 Resp: 307692
Ion Ratio Lower Upper
95 100
174 79.8 0.0 159.8
176 78.0 0.0 154.4


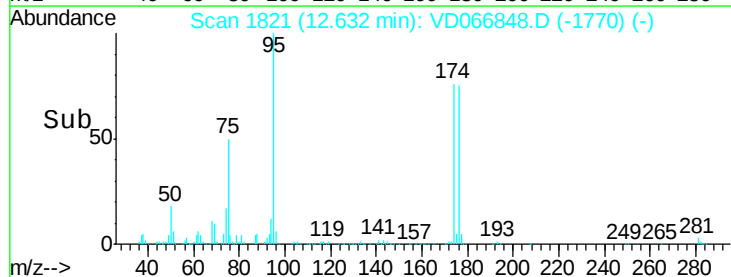
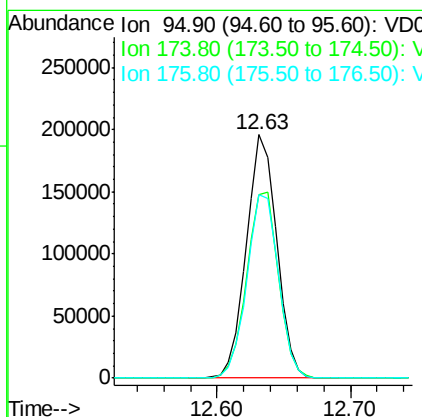
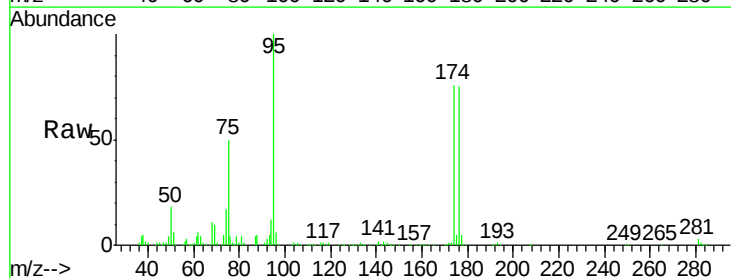


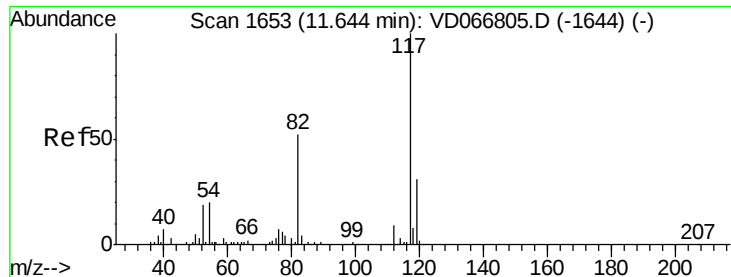

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.64 min Scan# 1653
Delta R.T. 0.00 min
Lab File: VD066848.D
Acq: 24 Sep 2020 13:53

Instrument :
MSVOA_D
ClientSampled :
CS-23

Tot Ion:117 Resp: 730434
Ion Ratio Lower Upper
117 100
82 53.2 41.8 62.6
119 32.4 24.6 37.0

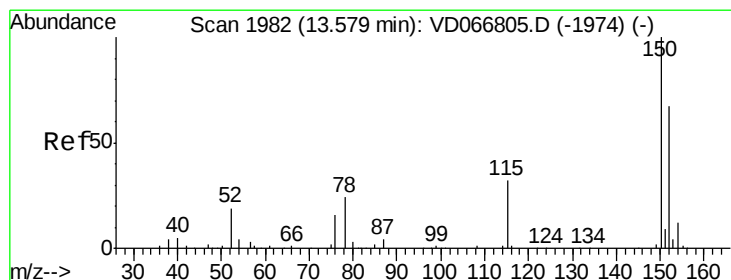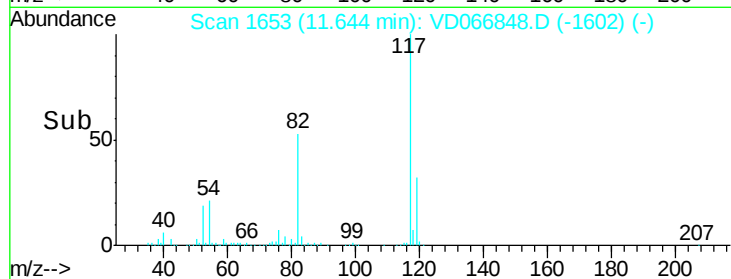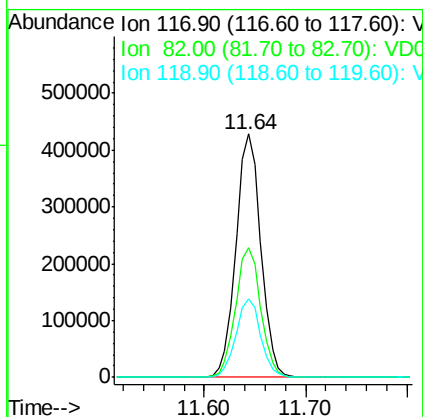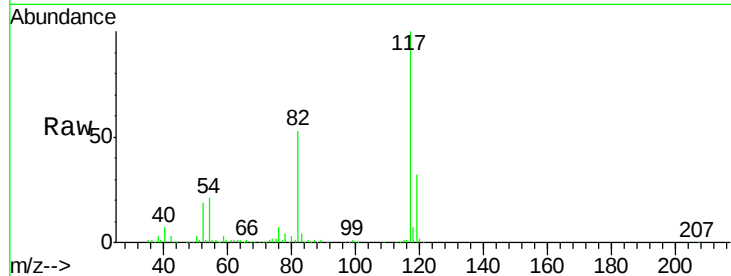

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.00 min
Lab File: VD066848.D
Acq: 24 Sep 2020 13:53

Tgt Ion:152 Resp: 336414
Ion Ratio Lower Upper
152 100
115 60.3 30.3 91.0
150 155.4 0.0 346.2

