


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD092420\
 Data File : VD066839.D
 Acq On : 24 Sep 2020 09:32
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
 Title : SW846 8260
 Last Update : Wed Sep 23 01:34:05 2020

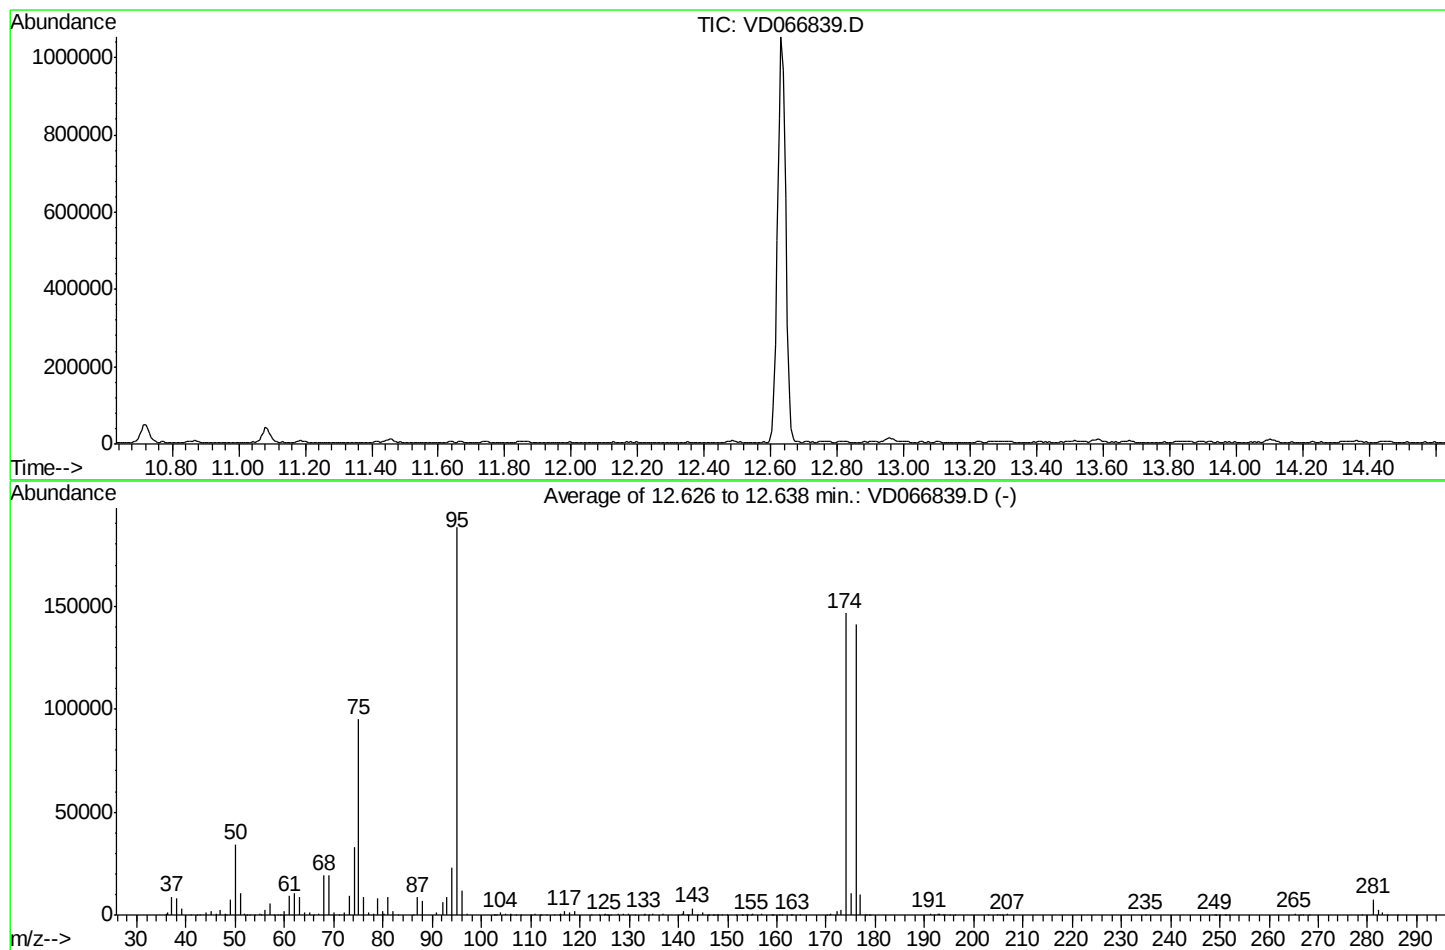

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	33922	PASS
75	95	30	60	50.4	94925	PASS
95	95	100	100	100.0	188266	PASS
96	95	5	9	6.3	11889	PASS
173	174	0.00	2	1.6	2416	PASS
174	95	50	100	77.9	146645	PASS
175	174	5	9	7.1	10391	PASS
176	174	95	101	96.1	140970	PASS
177	176	5	9	7.2	10106	PASS