


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD092519\
 Data File : VD063825.D
 Acq On : 25 Sep 2019 15:05
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00µ/5.00mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D092519S.M
 Title : SW846 8260
 Last Update : Thu Sep 26 12:03:05 2019

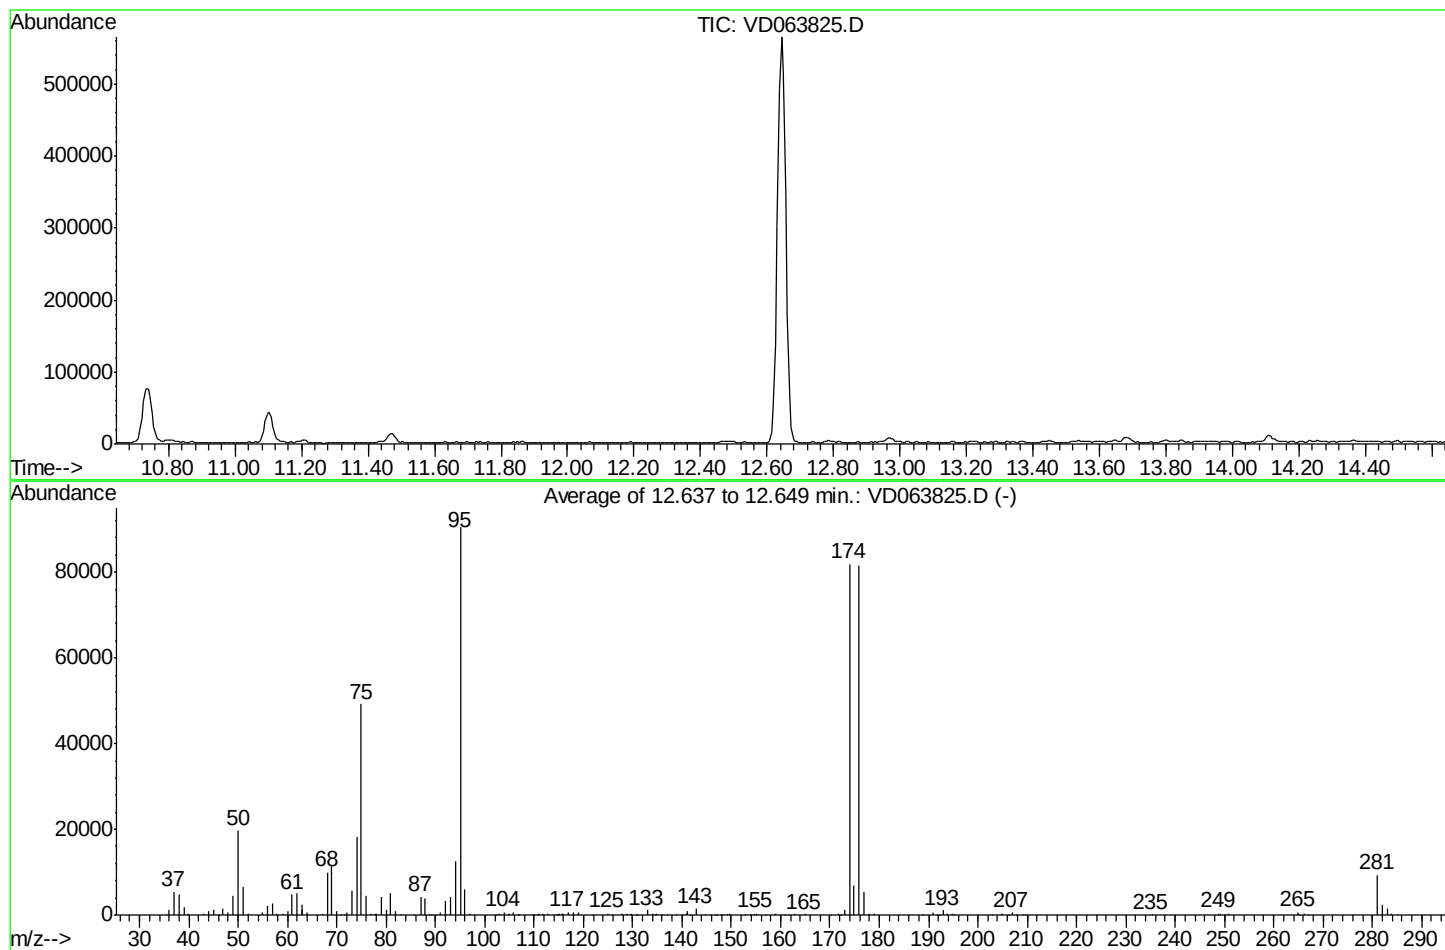

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	19626	PASS
75	95	30	60	54.4	49224	PASS
95	95	100	100	100.0	90482	PASS
96	95	5	9	6.6	5997	PASS
173	174	0.00	2	1.4	1113	PASS
174	95	50	100	90.6	81970	PASS
175	174	5	9	8.6	7017	PASS
176	174	95	101	99.4	81514	PASS
177	176	5	9	6.6	5381	PASS