

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD092520\
 Data File : VD066884.D
 Acq On : 25 Sep 2020 19:50
 Operator : VA/SY
 Sample : L4129-18
 Misc : 11.39G/5.00ml/MSVOA D/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DRUM-COMP-3

Quant Time: Sep 26 05:02:49 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 23 01:34:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.98
34) 1,4-Difluorobenzene	0.00	114	0m	50.00	ug/l	-8.86
63) Chlorobenzene-d5	0.00	117	0m	50.00	ug/l	-11.64
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.58

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0d	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD092520\
Data File : VD066884.D
Acq On : 25 Sep 2020 19:50
Operator : VA/SY
Sample : L4129-18
Misc : 11.39G/5.00ml/MSVOA D/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DRUM-COMP-3

Quant Time: Sep 26 05:02:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 23 01:34:05 2020
Response via : Initial Calibration

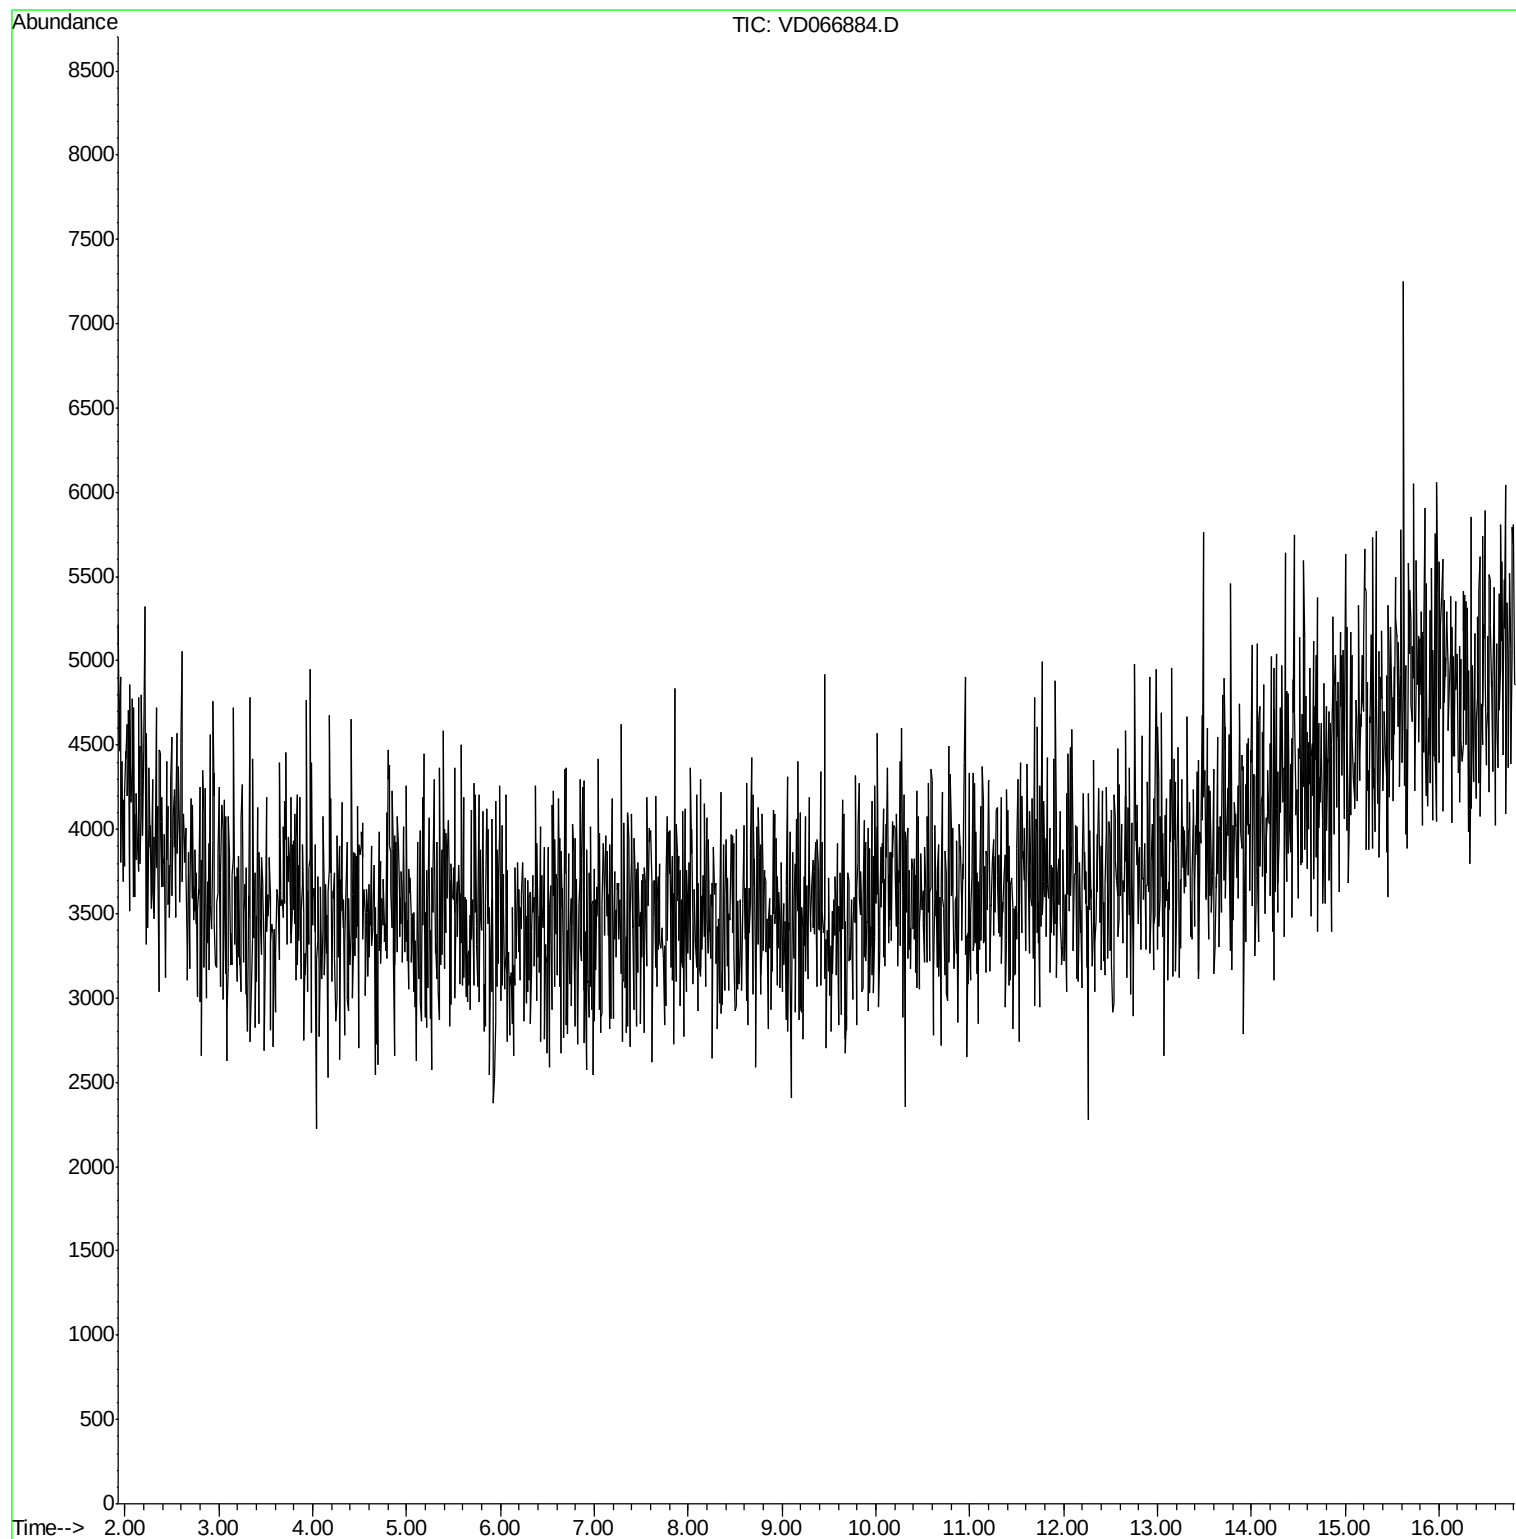

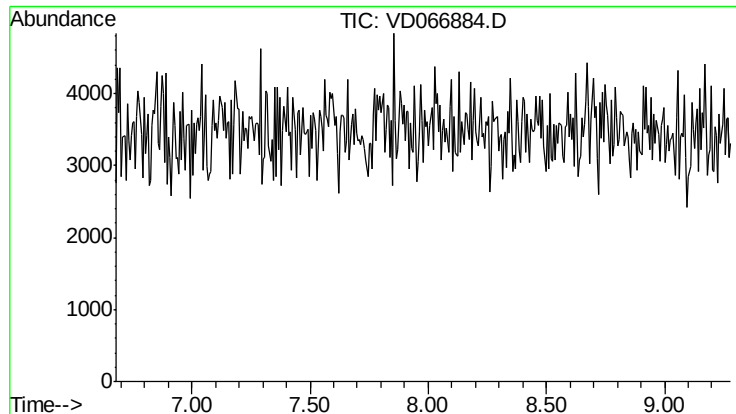

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.98 min

Lab File: VD066884.D

Acq: 25 Sep 2020 19:50

Tot Ion: 168

Sig	Exp Ratio
168	100
99	58.2

168 100



99 58.2

Instrument :

MSVOA_D

ClientSampleId :

DRUM-COMP-3

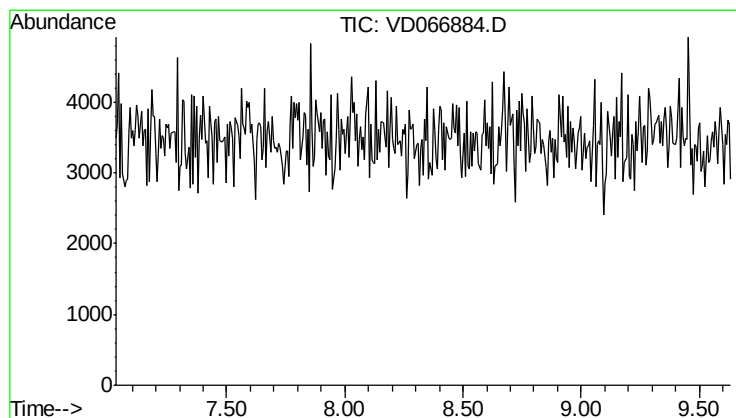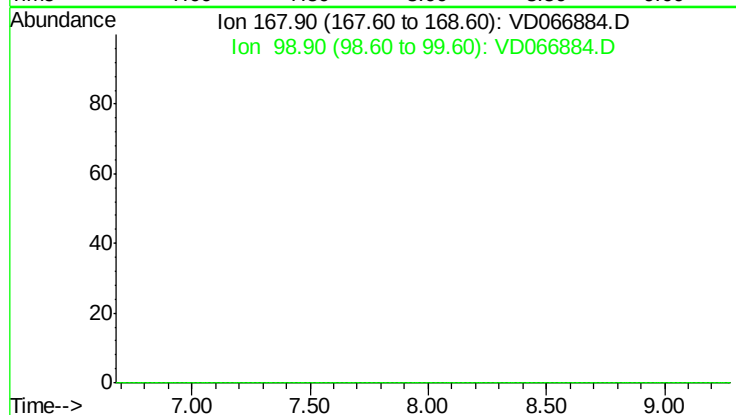

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.33 min

Lab File: VD066884.D


Acq: 25 Sep 2020 19:50


Tgt Ion: 65

Sig	Exp Ratio
65	100
67	53.6

65 100

67 53.6


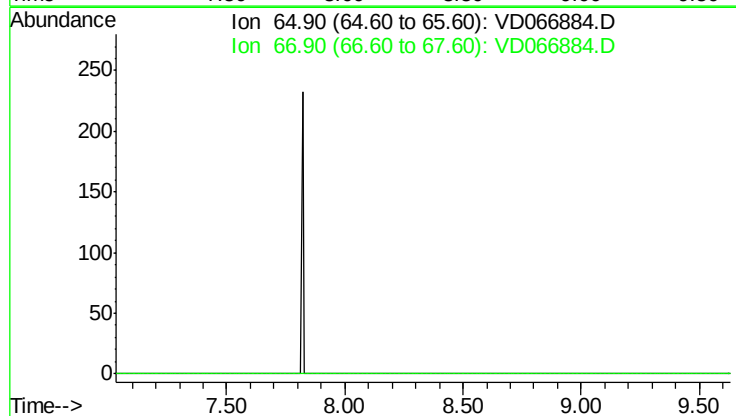


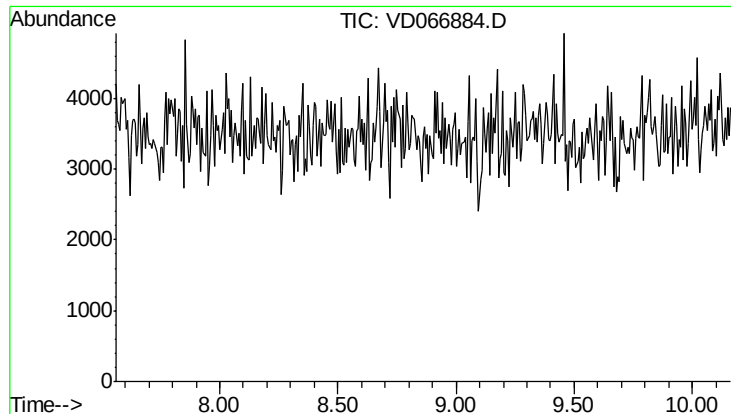

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.86 min
 Lab File: VD066884.D
 Acq: 25 Sep 2020 19:50


Instrument :
 MSVOA_D
 ClientSampleId :
 DRUM-COMP-3


Tot Ion	114
Sig	Exp Ratio
114	100
63	21.3
88	16.3

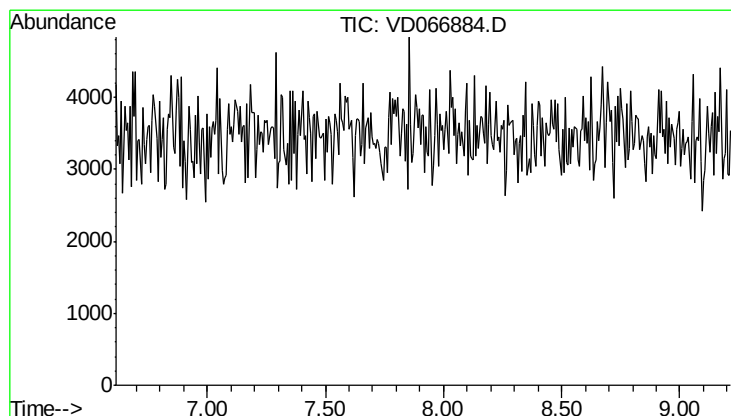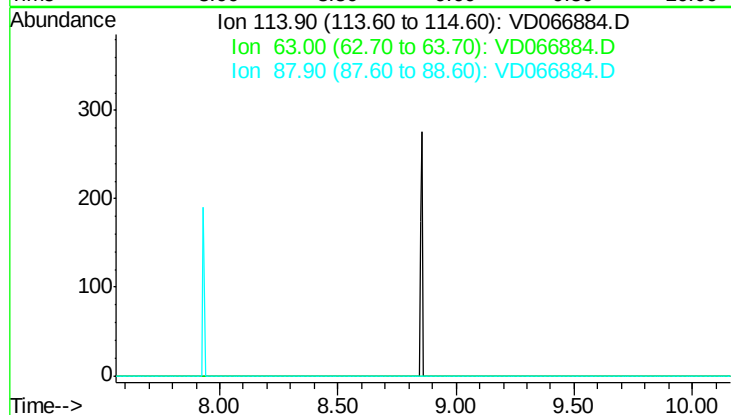

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.91 min
 Lab File: VD066884.D
 Acq: 25 Sep 2020 19:50

Tgt Ion	113
Sig	Exp Ratio
113	100
111	102.3
192	18.0

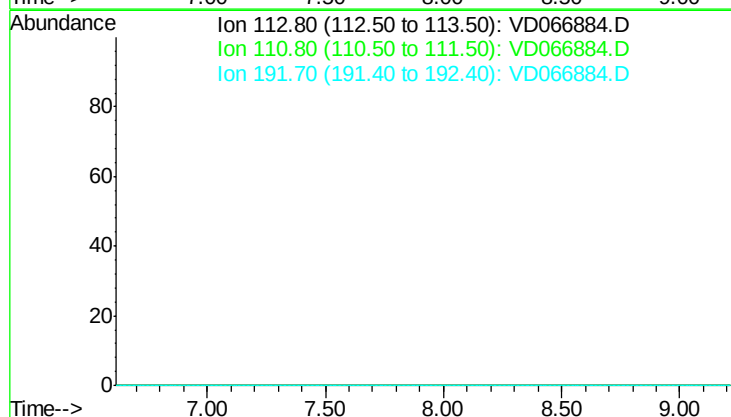


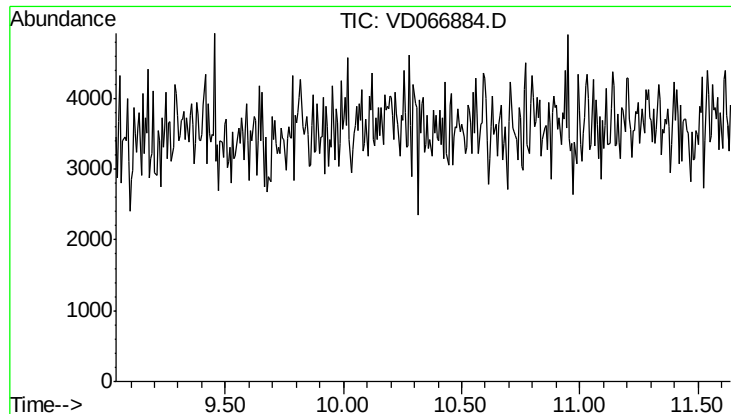


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.34 min

Lab File: VD066884.D
Acq: 25 Sep 2020 19:50

Instrument :
MSVOA_D
ClientSampleId :
DRUM-COMP-3


Tot Ion: 98
Sig Exp Ratio
98 100
100 65.2

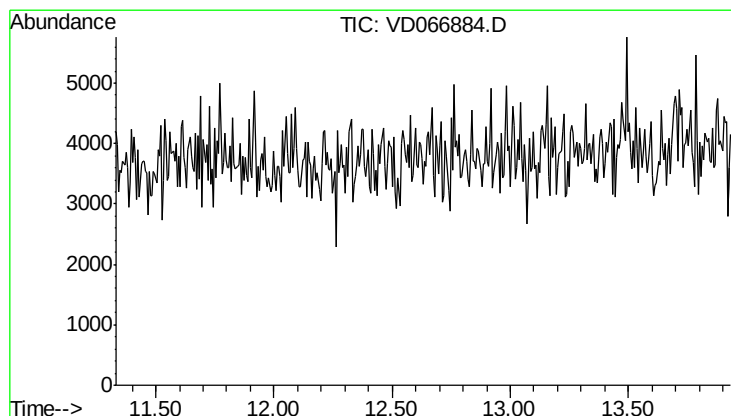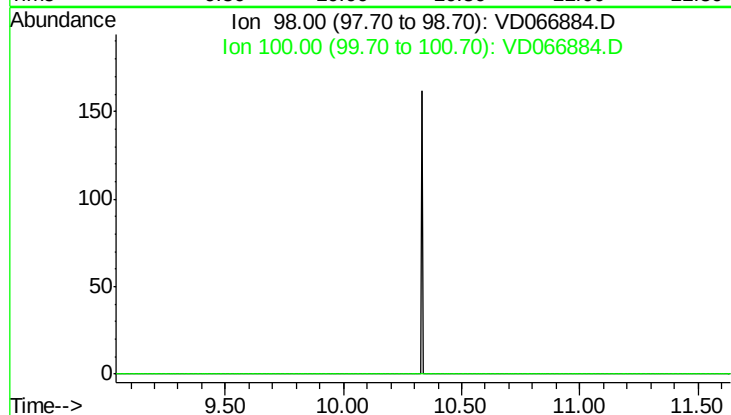


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.63 min

Lab File: VD066884.D
Acq: 25 Sep 2020 19:50

Tgt Ion: 95
Sig Exp Ratio
95 100
174 79.9
176 77.2

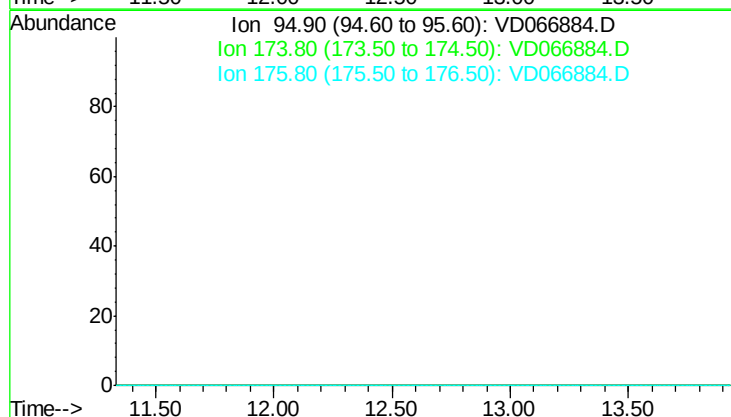


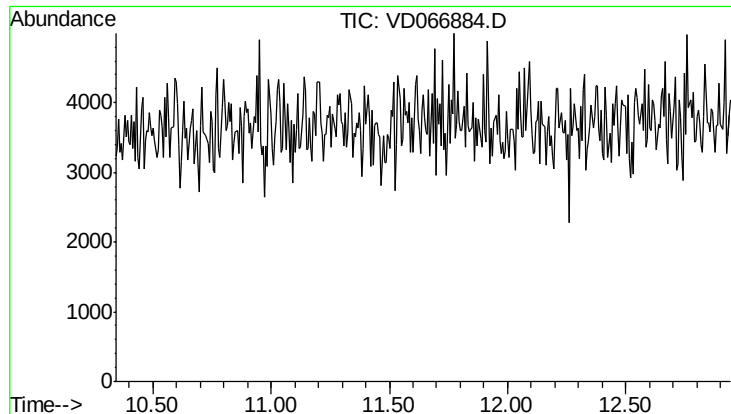


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.64 min
 Lab File: VD066884.D
 Acq: 25 Sep 2020 19:50

Instrument :
 MSVOA_D
 ClientSampleId :
 DRUM-COMP-3

Tot Ion: 117

Sig	Exp Ratio
117	100
82	52.2
119	30.8

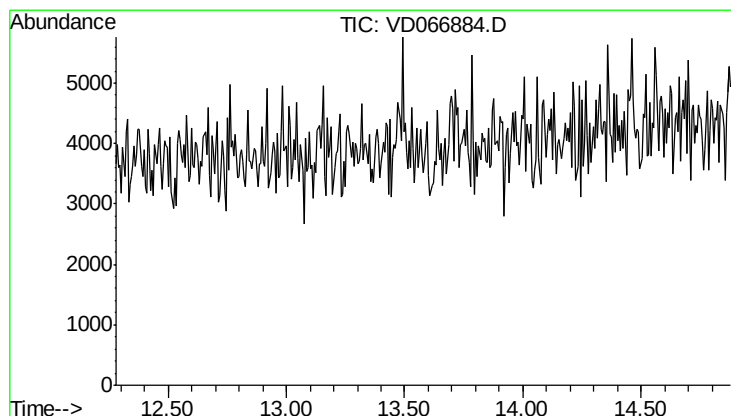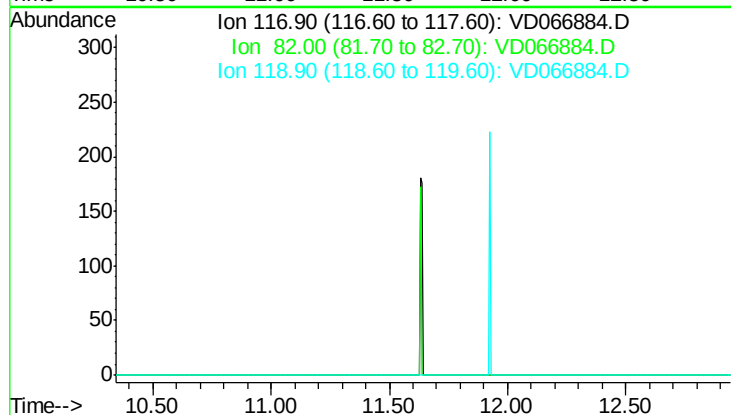

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.58 min
 Lab File: VD066884.D
 Acq: 25 Sep 2020 19:50

Tgt Ion: 152

Sig	Exp Ratio
152	100
115	60.7
150	173.1

