


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD092619\
Data File : VD063833.D
Acq On : 26 Sep 2019 09:32
Operator : VA/SY
Sample : BFB
Misc : 5.00µ/5.00mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D092519S.M
Title : SW846 8260
Last Update : Thu Sep 26 12:03:05 2019

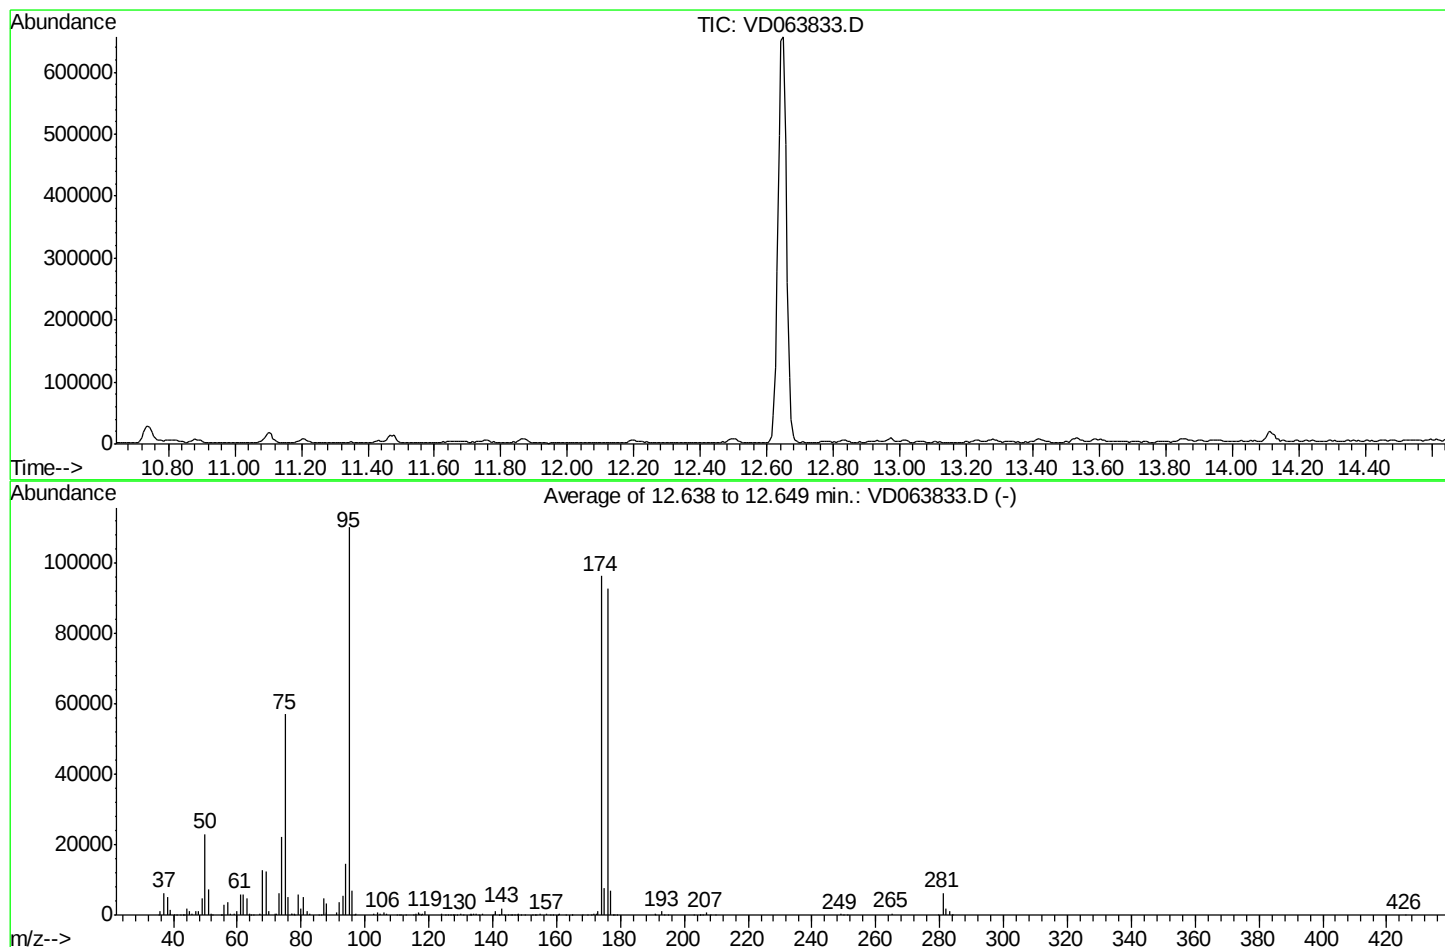

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	23064	PASS
75	95	30	60	51.7	57056	PASS
95	95	100	100	100.0	110258	PASS
96	95	5	9	6.4	7110	PASS
173	174	0.00	2	1.1	1092	PASS
174	95	50	100	87.4	96389	PASS
175	174	5	9	8.1	7805	PASS
176	174	95	101	96.3	92824	PASS
177	176	5	9	7.5	6952	PASS