
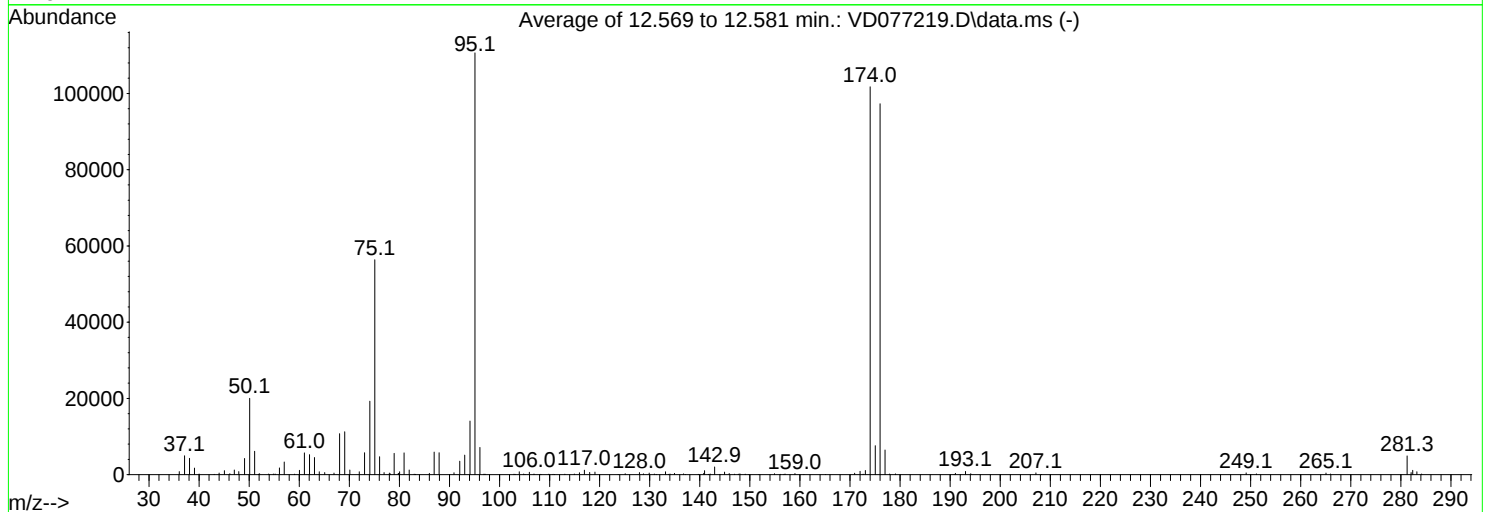


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092623\
Data File : VD077219.D
Acq On : 26 Sep 2023 10:12
Operator : JC/SY
Sample : BFB166
Misc : 5.00G/10.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB166

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM092523SMA.M
Title : SFAM01.0
Last Update : Mon Sep 25 23:07:59 2023

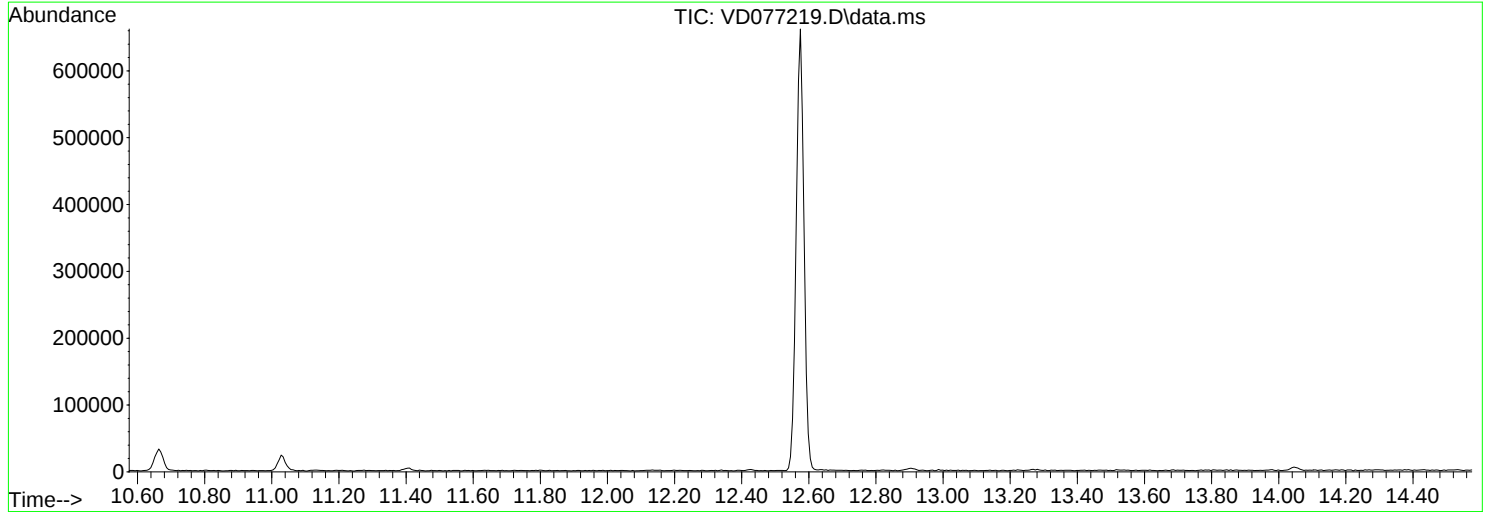

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	20024	PASS
75	95	30	80	50.9	56371	PASS
95	95	100	100	100.0	110656	PASS
96	95	5	9	6.5	7152	PASS
173	174	0.00	2	1.1	1078	PASS
174	95	50	120	92.0	101771	PASS
175	174	5	9	7.5	7586	PASS
176	174	95	105	95.6	97296	PASS
177	176	5	10	6.7	6478	PASS

m/z	Abundance
40.10	1205.0
44.10	971.0

Instrument :
MSVOA_D
ClientSampleId :
BFB166

m/z	Abundance
36.00	818.0
37.10	4754.0
38.10	4253.0
39.10	1980.0
40.00	1301.0
44.00	1649.0
45.00	1101.0
46.10	230.0
47.00	910.0
48.00	723.0
49.10	3985.0
50.10	18968.0
51.10	6616.0
51.90	411.0
53.90	330.0
55.20	290.0
56.10	1768.0
57.00	2971.0
59.20	200.0
60.00	1158.0
61.00	5370.0
62.10	5640.0
63.10	4457.0
64.00	622.0
65.10	581.0
67.00	525.0
68.00	10696.0
69.10	11914.0
70.10	1271.0
72.00	813.0
73.00	5686.0
74.10	19664.0
75.10	56608.0
76.10	5025.0
77.00	664.0
78.00	730.0
78.90	5828.0
79.80	1077.0
80.10	985.0
80.90	5830.0
81.90	1463.0
83.00	261.0
86.00	353.0
86.90	5326.0
88.00	6229.0
90.90	409.0
92.00	3844.0
93.10	4236.0
94.10	13573.0
95.10	111104.0
96.10	7415.0
96.90	177.0
103.90	524.0
104.90	265.0
106.00	347.0
106.90	153.0
109.80	171.0
113.00	199.0
115.00	296.0
116.10	411.0
117.00	1012.0
118.00	713.0
119.10	862.0
123.70	176.0
125.10	268.0
128.00	514.0
128.80	443.0
130.00	425.0
133.10	817.0
133.80	227.0
134.90	243.0
136.80	392.0
140.80	1010.0
142.00	305.0
142.90	1949.0
145.00	706.0
145.80	232.0
148.00	338.0
154.90	201.0
156.80	224.0
159.00	338.0
170.90	552.0
172.00	892.0
172.60	451.0
173.10	660.0
174.00	97984.0
175.00	7564.0
176.00	94400.0
177.00	6981.0
178.00	251.0
179.00	176.0
190.80	281.0

Instrument :
MSVOA_D
ClientSampleId :
BFB166

192.10	186.0
193.00	503.0
194.10	213.0
207.10	540.0
249.10	325.0
265.20	194.0
281.30	3709.0
282.10	601.0
282.40	608.0
283.20	648.0
284.20	163.0

Instrument :
MSVOA_D
ClientSampleId :
BFB166

m/z	Abundance
36.10	946.0
37.10	5937.0
38.10	4809.0
39.10	1511.0
40.00	1173.0
44.00	1361.0
45.10	1349.0
46.20	347.0
47.10	1258.0
48.00	843.0
49.10	4487.0
50.10	22704.0
51.10	7011.0
52.10	313.0
54.10	167.0
54.80	225.0
55.20	204.0
56.00	2072.0
57.00	3932.0
59.00	202.0
60.10	1252.0
61.10	6681.0
62.10	5804.0
63.00	4699.0
64.00	990.0
65.00	655.0
66.80	282.0
67.10	264.0
68.10	12693.0
69.10	12435.0
70.10	1132.0
72.10	949.0
73.00	6849.0
74.10	21264.0
75.10	62656.0
76.00	5138.0
76.90	657.0
78.20	595.0
79.00	6368.0
80.00	1311.0
81.00	6653.0
82.00	1359.0
83.20	233.0
85.90	342.0
87.00	7089.0
88.00	5743.0
90.90	651.0
92.10	3731.0
93.00	5724.0
94.10	16181.0
95.10	123320.0
96.10	8235.0
97.10	341.0
102.90	342.0
104.00	1065.0
104.80	261.0
106.00	946.0
106.80	185.0
108.10	255.0
110.70	265.0
114.90	205.0
115.90	654.0
116.90	1468.0
118.00	596.0
119.00	732.0
125.10	219.0
127.90	723.0
129.80	511.0
131.00	269.0
133.10	828.0
134.00	387.0
135.00	417.0
137.10	202.0
139.70	262.0
141.00	1732.0
142.10	161.0
143.00	2447.0
145.00	649.0
145.80	311.0
146.90	244.0
147.70	354.0
149.10	192.0
149.80	180.0
154.80	335.0
156.10	155.0
157.00	265.0
159.00	185.0
165.10	155.0
170.90	365.0
172.10	999.0
173.10	1555.0
174.00	112480.0

Instrument :
MSVOA_D
ClientSampleId :
BFB166

175.10	8431.0
176.00	107416.0
177.00	7149.0
177.80	224.0
179.10	248.0
191.00	654.0
193.10	1104.0
194.10	202.0
207.10	451.0
249.10	654.0
251.10	206.0
265.00	600.0
266.00	233.0
281.20	5082.0
282.00	1042.0
282.40	1141.0
283.30	850.0
284.10	299.0

Instrument :
MSVOA_D
ClientSampleId :
BFB166

m/z	Abundance
36.00	621.0
37.10	4211.0
38.10	3743.0
39.10	1636.0
40.00	1596.0
43.00	217.0
44.00	1126.0
45.00	716.0
46.10	194.0
47.00	1520.0
47.90	816.0
49.10	4250.0
50.10	18400.0
51.10	4742.0
52.10	510.0
53.90	189.0
54.90	257.0
56.00	1522.0
57.00	3078.0
60.00	1024.0
61.00	5032.0
62.00	4335.0
63.10	4274.0
64.00	596.0
65.20	347.0
67.00	243.0
68.00	8864.0
69.10	9393.0
70.10	1289.0
71.90	523.0
73.10	4778.0
74.10	16928.0
75.10	49848.0
76.10	3899.0
76.90	339.0
78.00	553.0
78.90	4621.0
79.90	950.0
81.00	4611.0
81.90	857.0
82.90	192.0
86.10	324.0
87.00	5349.0
87.90	5354.0
90.90	504.0
92.00	3042.0
93.00	5457.0
94.10	12416.0
95.10	97544.0
96.10	5805.0
96.90	217.0
103.10	307.0
104.00	740.0
105.10	155.0
105.90	600.0
107.00	173.0
108.30	157.0
109.90	230.0
111.00	163.0
113.10	245.0
115.80	456.0
117.00	1013.0
118.00	490.0
119.10	455.0
125.10	302.0
127.90	387.0
128.70	169.0
129.90	356.0
130.80	207.0
131.30	154.0
133.20	656.0
134.10	152.0
135.00	372.0
136.70	187.0
140.90	1466.0
141.70	279.0
143.00	1648.0
144.00	204.0
144.90	621.0
145.90	356.0
147.00	167.0
148.00	286.0
149.00	159.0
151.80	165.0
155.00	218.0
156.10	165.0
157.00	202.0
159.00	342.0
160.80	180.0
171.00	283.0
171.90	816.0
172.90	1019.0

Instrument :
MSVOA_D
ClientSampleId :
BFB166

174.00	94848.0
175.00	6764.0
176.00	90072.0
177.00	5303.0
179.10	278.0
191.10	329.0
193.00	937.0
193.90	163.0
194.20	172.0
207.10	432.0
208.20	154.0
249.10	471.0
250.00	166.0
251.20	405.0
265.10	530.0
265.90	291.0
281.20	5911.0
282.30	1681.0
283.10	786.0

Instrument :
MSVOA_D
ClientSampleId :
BFB166