


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD092920\
 Data File : VD066949.D
 Acq On : 29 Sep 2020 20:26
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D092220S.M
 Title : SW846 8260
 Last Update : Wed Sep 23 01:34:05 2020

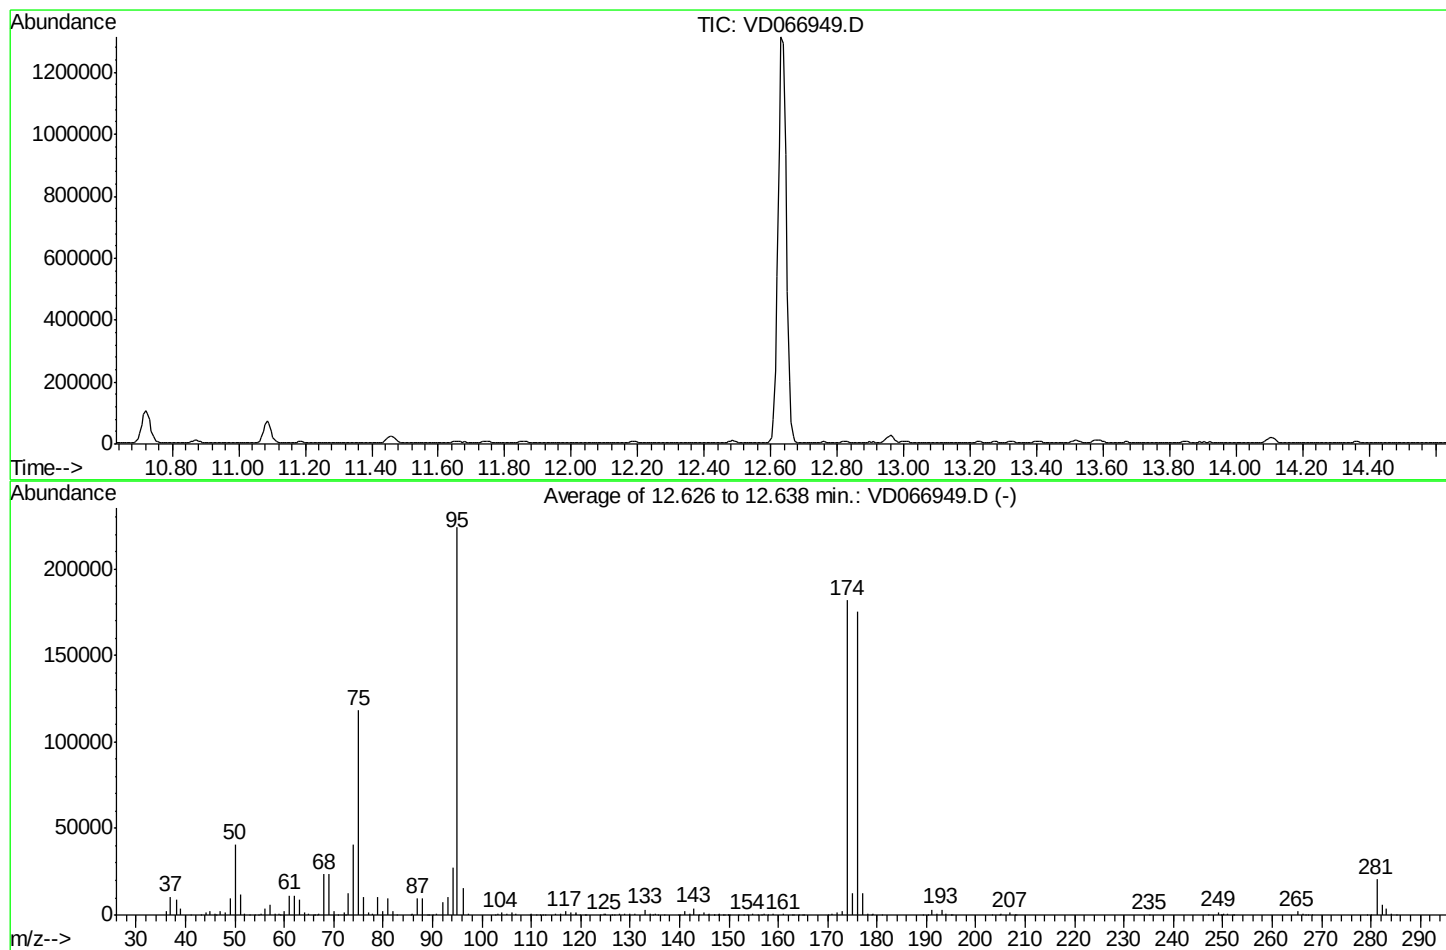

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	40461	PASS
75	95	30	60	52.7	118112	PASS
95	95	100	100	100.0	223957	PASS
96	95	5	9	7.0	15750	PASS
173	174	0.00	2	1.4	2511	PASS
174	95	50	100	81.1	181589	PASS
175	174	5	9	7.0	12630	PASS
176	174	95	101	96.6	175488	PASS
177	176	5	9	7.0	12250	PASS