
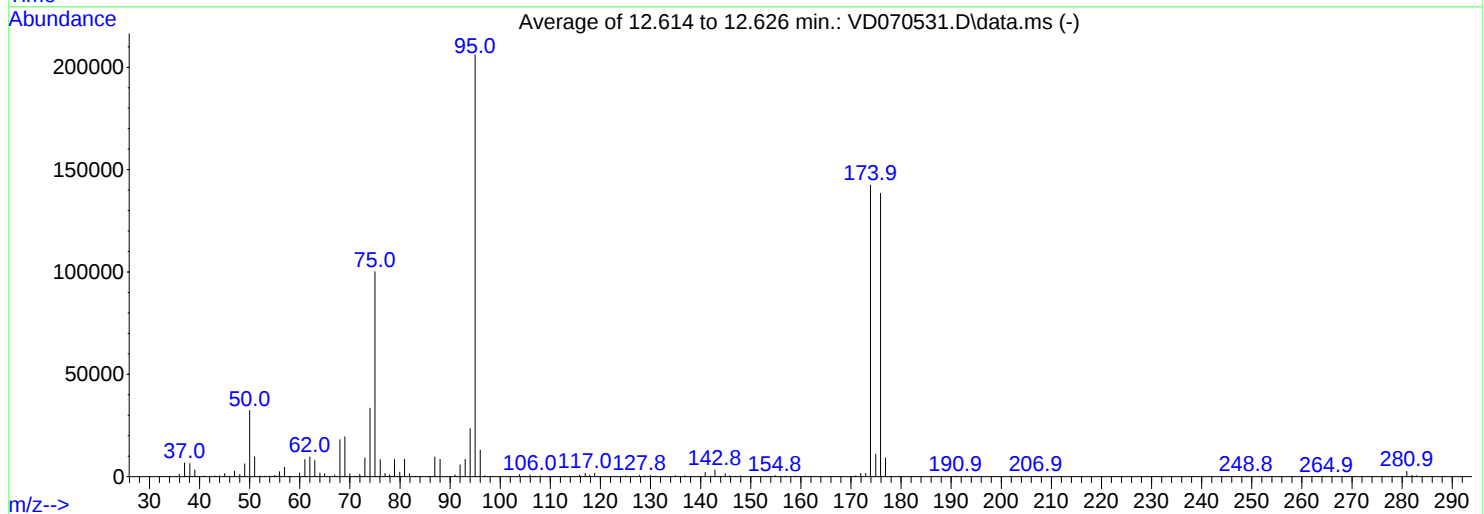


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD093021\
Data File : VD070531.D
Acq On : 30 Sep 2021 08:59
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Title : SW846 8260
Last Update : Thu Sep 09 03:07:09 2021

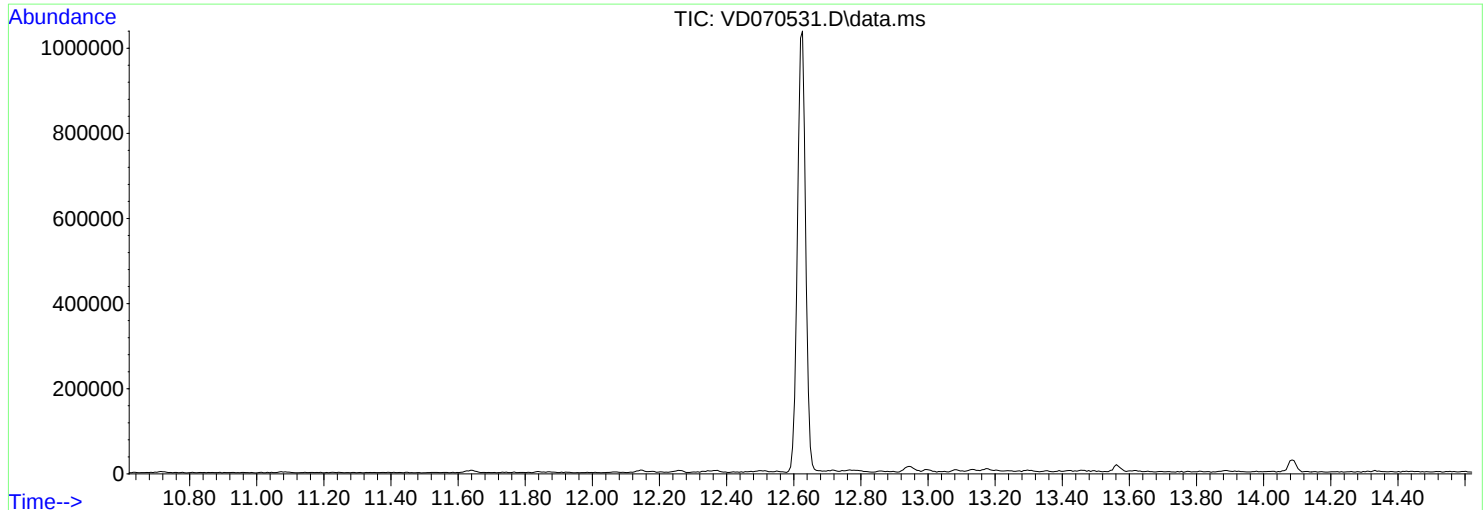

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	32269	PASS
75	95	30	60	48.6	100117	PASS
95	95	100	100	100.0	206080	PASS
96	95	5	9	6.3	13010	PASS
173	174	0.00	2	1.1	1532	PASS
174	95	50	100	69.1	142475	PASS
175	174	5	9	7.7	10912	PASS
176	174	95	101	97.2	138445	PASS
177	176	5	9	6.6	9152	PASS