



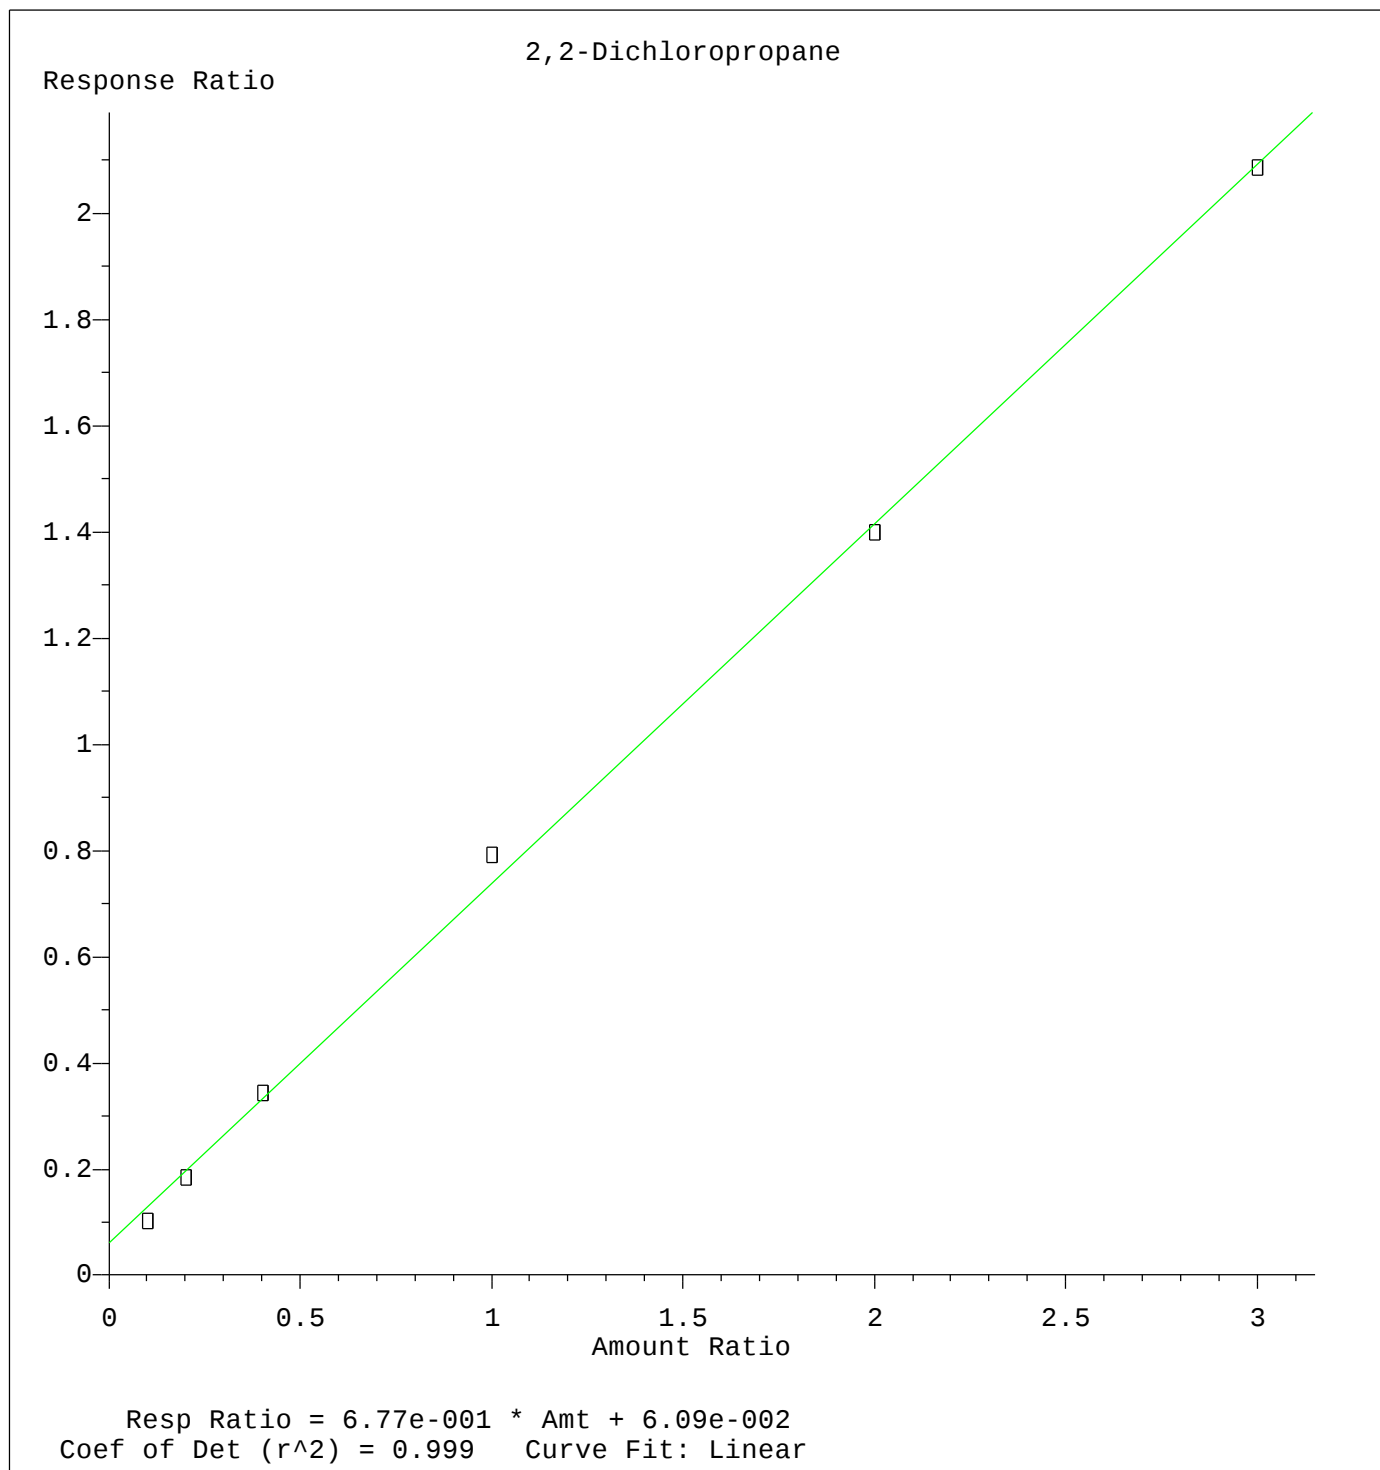

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Calibration Table Last Updated: Thu Oct 01 15:19:17 2020


Methylene Chloride

Response Ratio

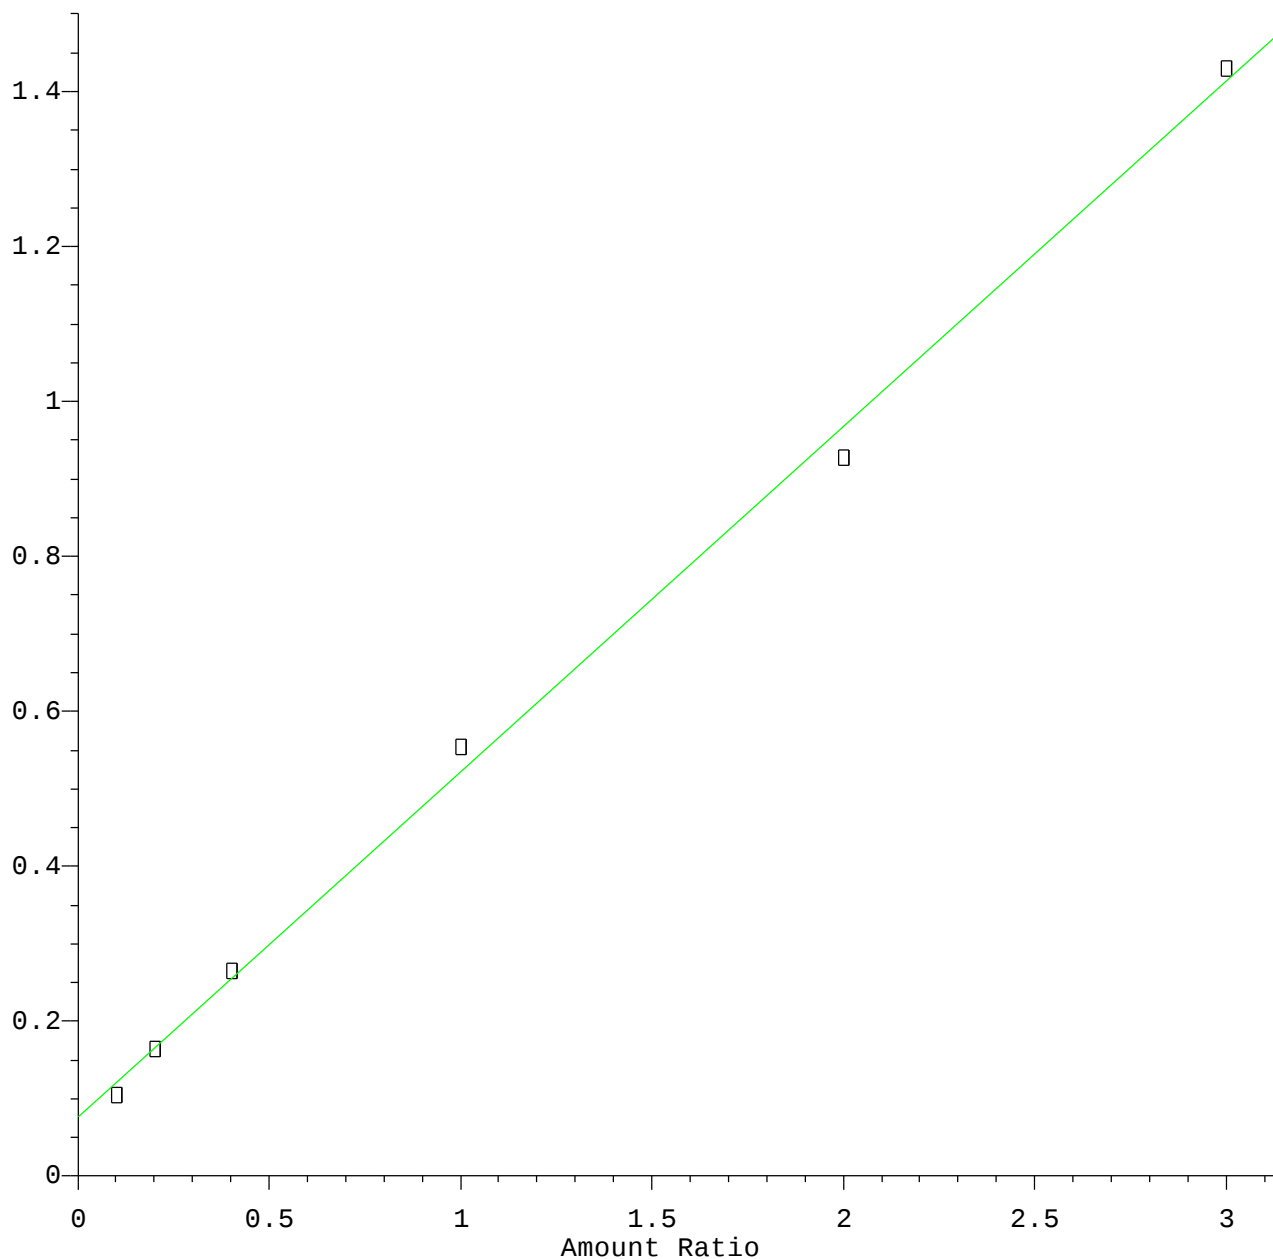


Resp Ratio = $4.46 \times 10^{-1} \times \text{Amt} + 7.59 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Calibration Table Last Updated: Thu Oct 01 15:19:17 2020

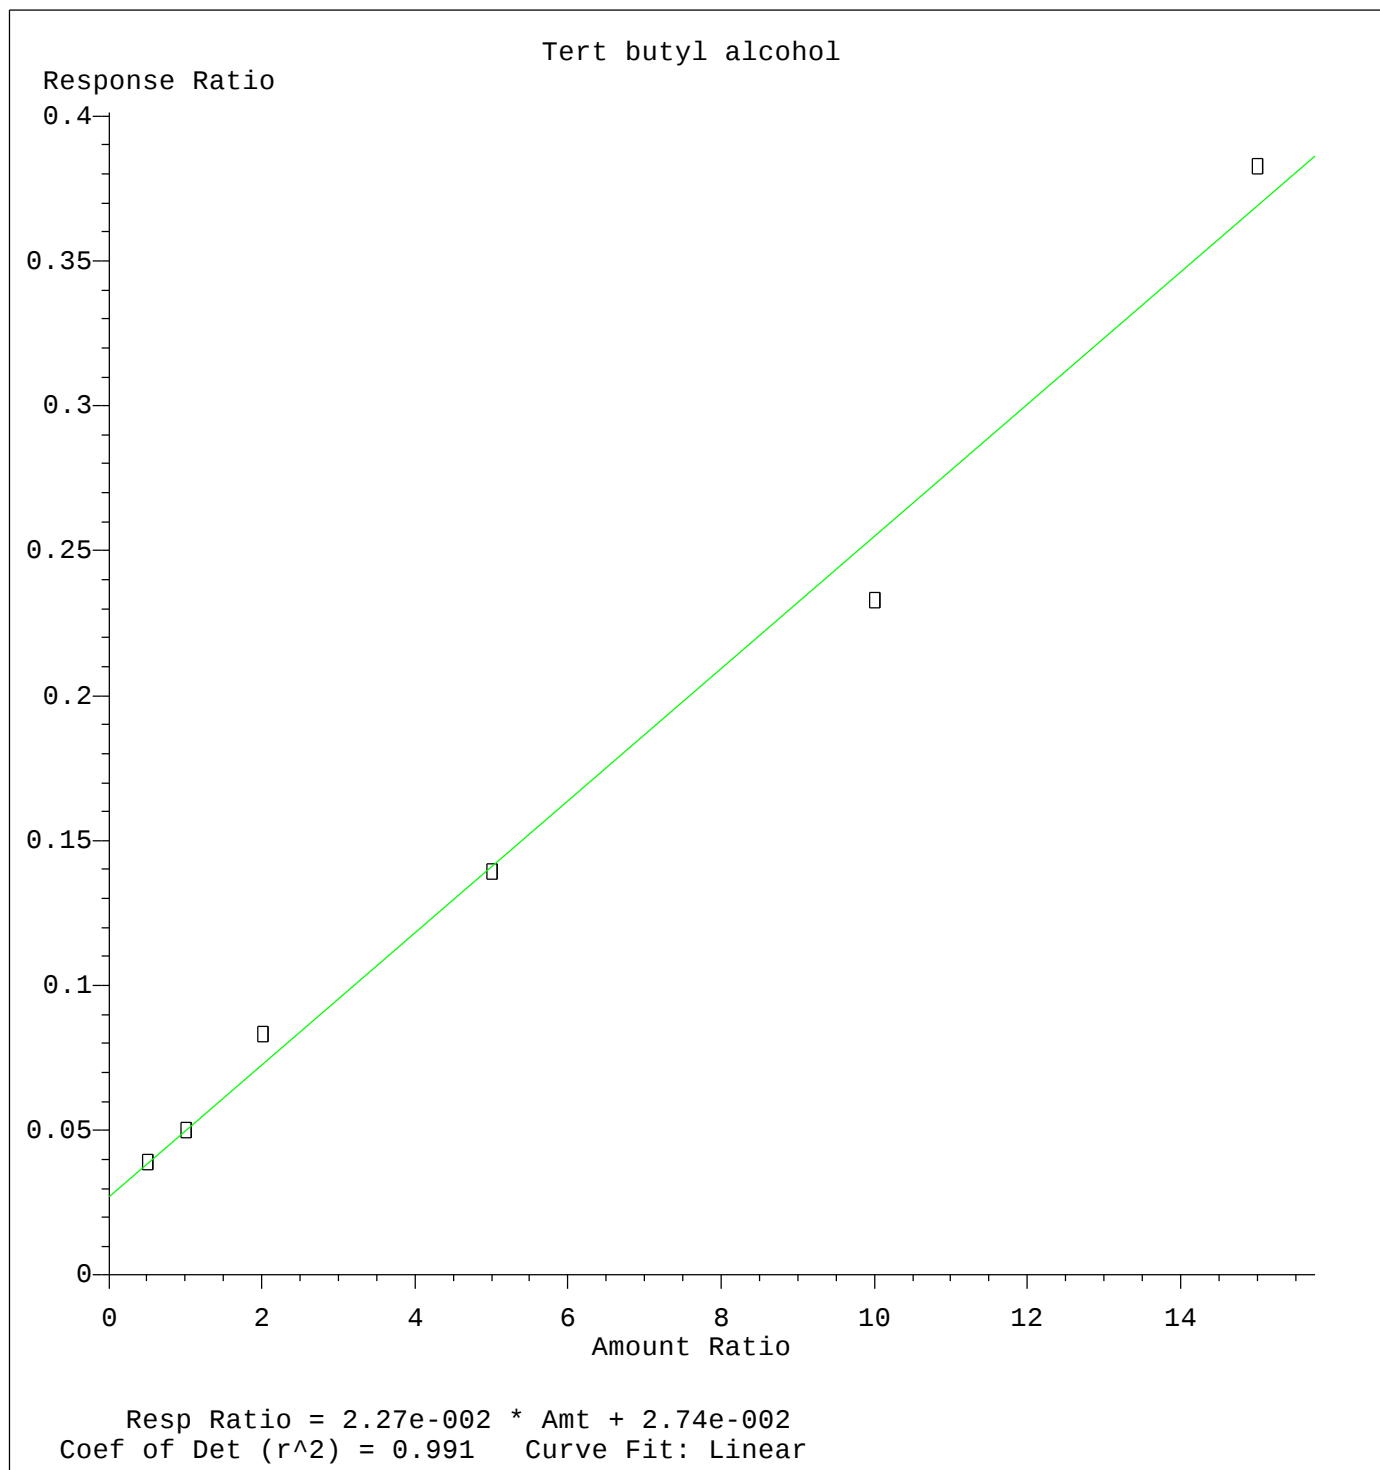


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Calibration Table Last Updated: Thu Oct 01 15:19:17 2020

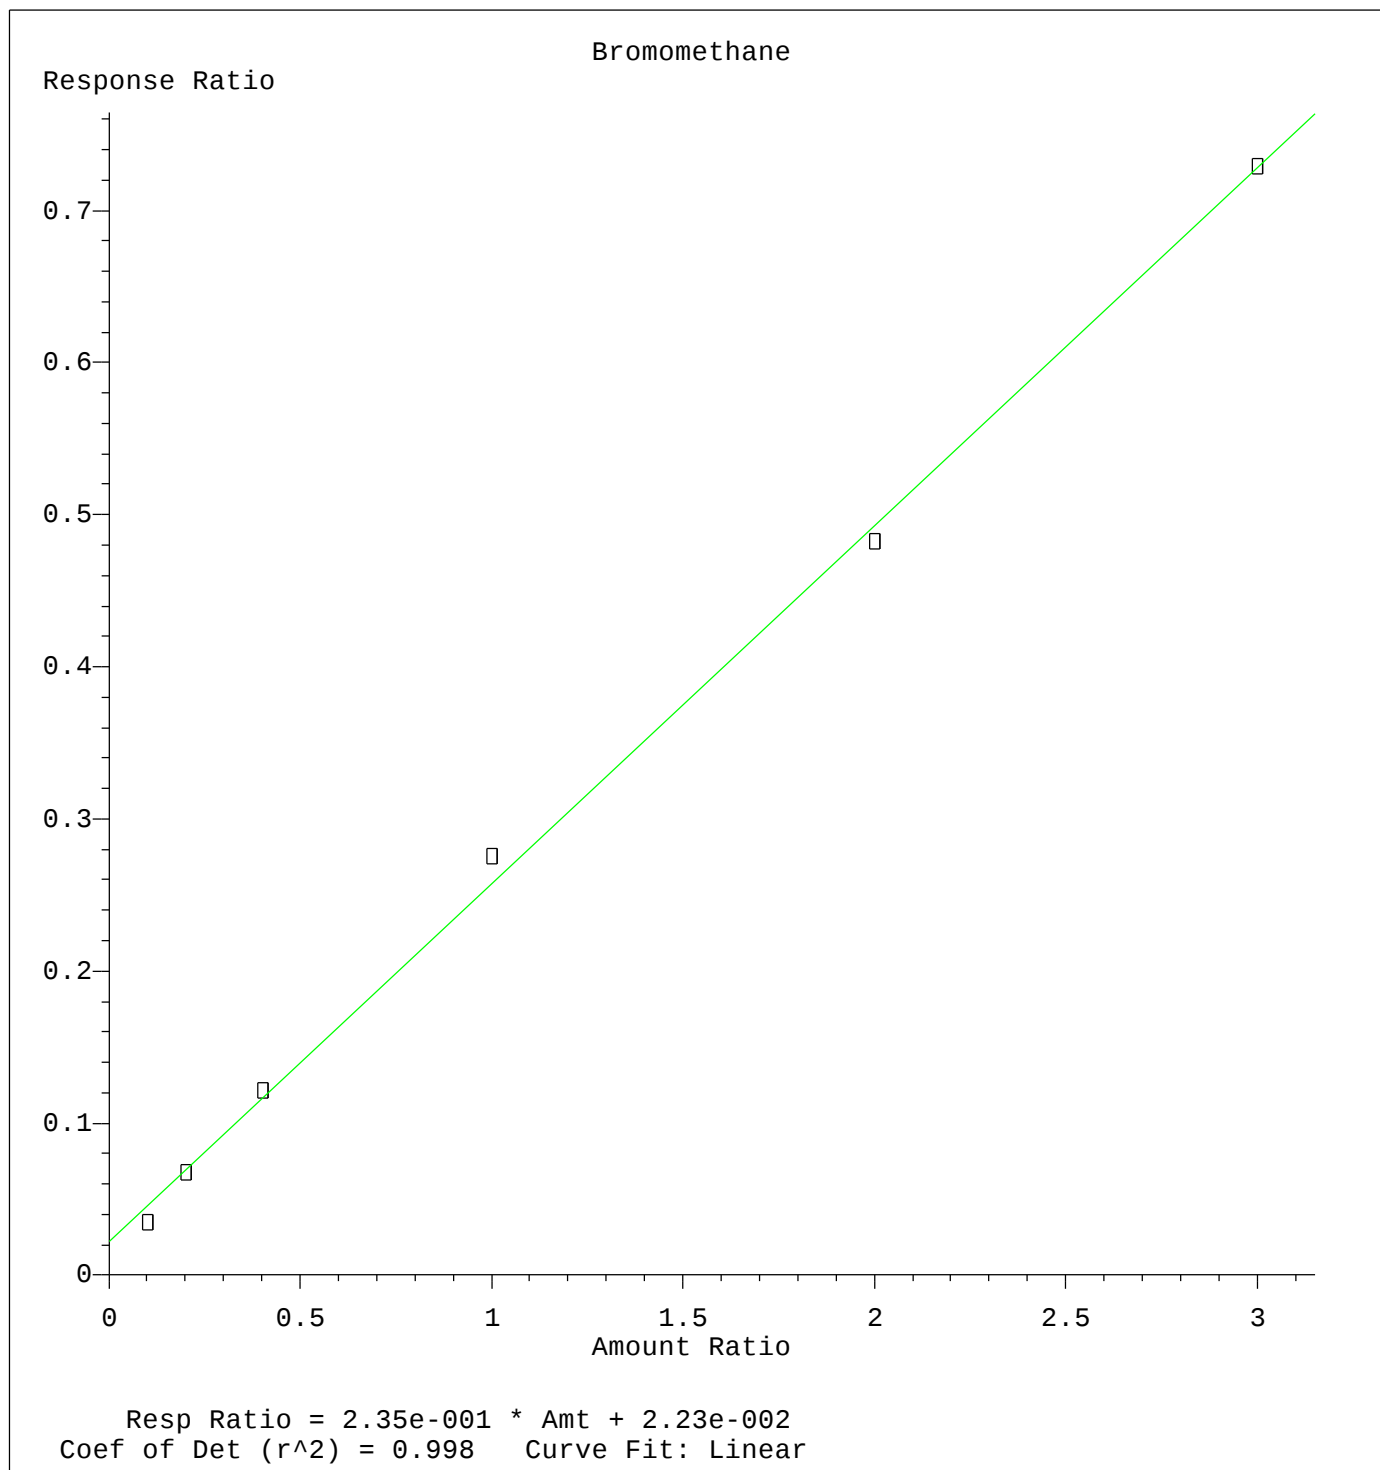

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Calibration Table Last Updated: Thu Oct 01 15:19:17 2020

Dichlorodifluoromethane

Response Ratio

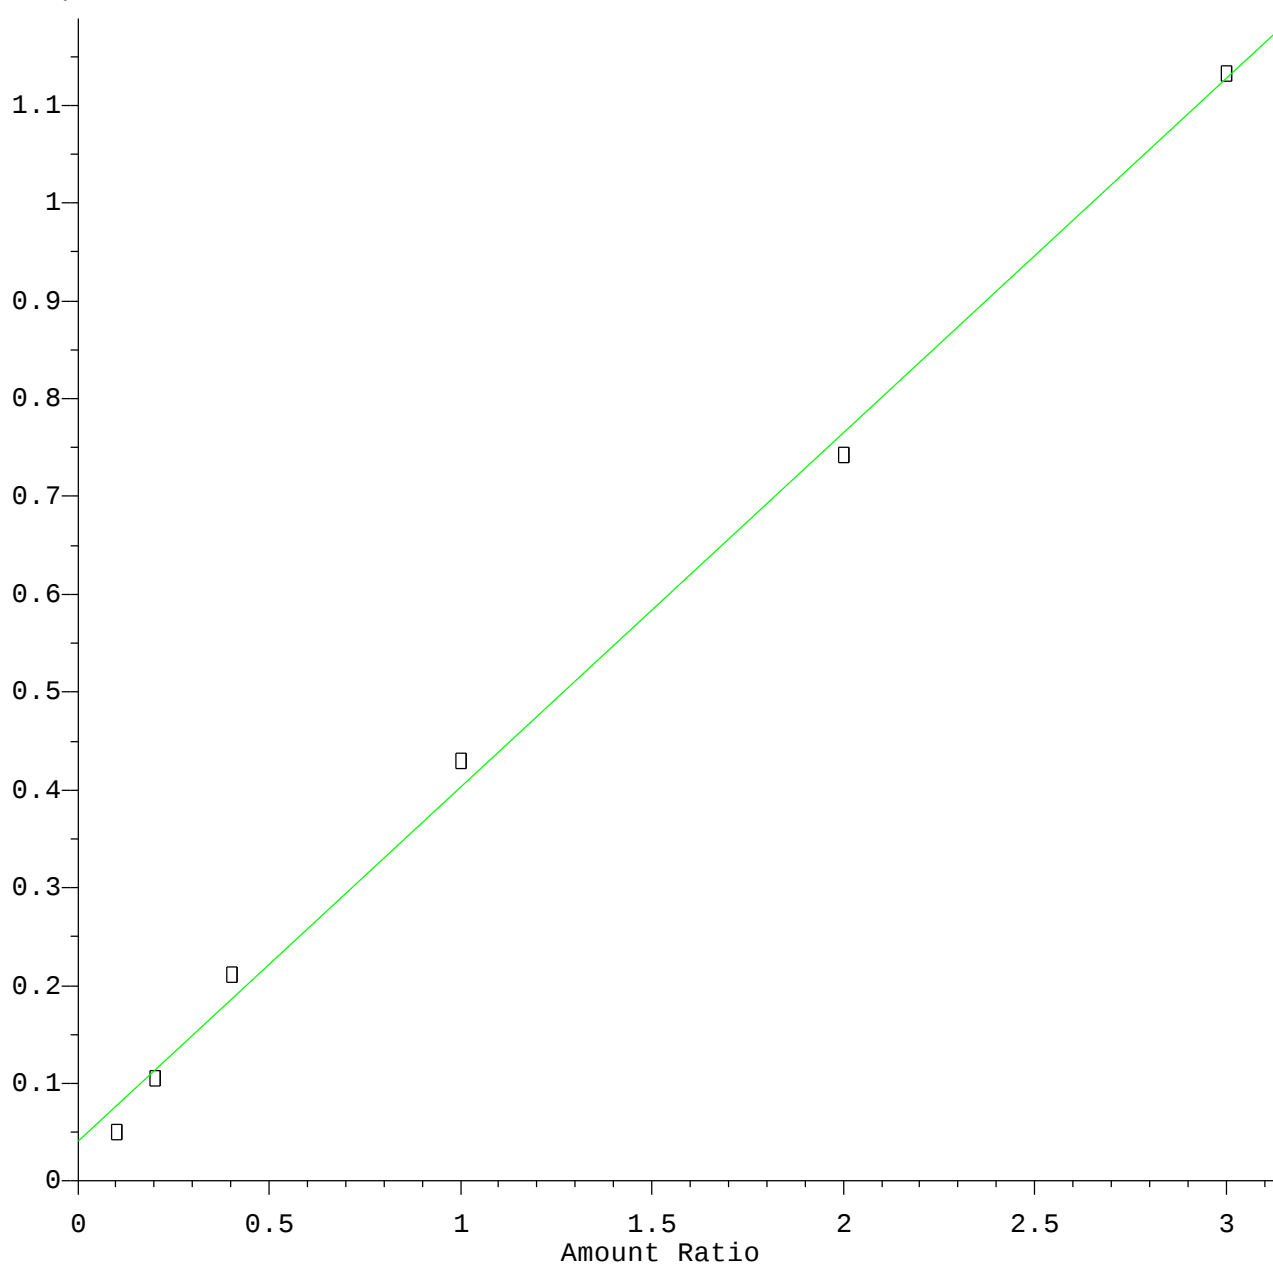

Resp Ratio = $3.63 \times 10^{-1} \times \text{Amt} + 3.99 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Calibration Table Last Updated: Thu Oct 01 15:19:17 2020