

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD100120\
 Data File : VD066992.D
 Acq On : 01 Oct 2020 15:03
 Operator : VA/SY
 Sample : VD1001SBL01
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1001SBL01

Quant Time: Oct 02 00:52:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 15:19:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	540836	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.86	114	883280	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	845128	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	395308	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	255894	49.12	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.24%	
35) Dibromofluoromethane	7.91	113	274204	47.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.84%	
50) Toluene-d8	10.34	98	1033664	49.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.12%	
62) 4-Bromofluorobenzene	12.63	95	365530	51.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.20%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD100120\
Data File : VD066992.D
Acq On : 01 Oct 2020 15:03
Operator : VA/SY
Sample : VD1001SBL01
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1001SBL01

Quant Time: Oct 02 00:52:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 15:19:17 2020
Response via : Initial Calibration

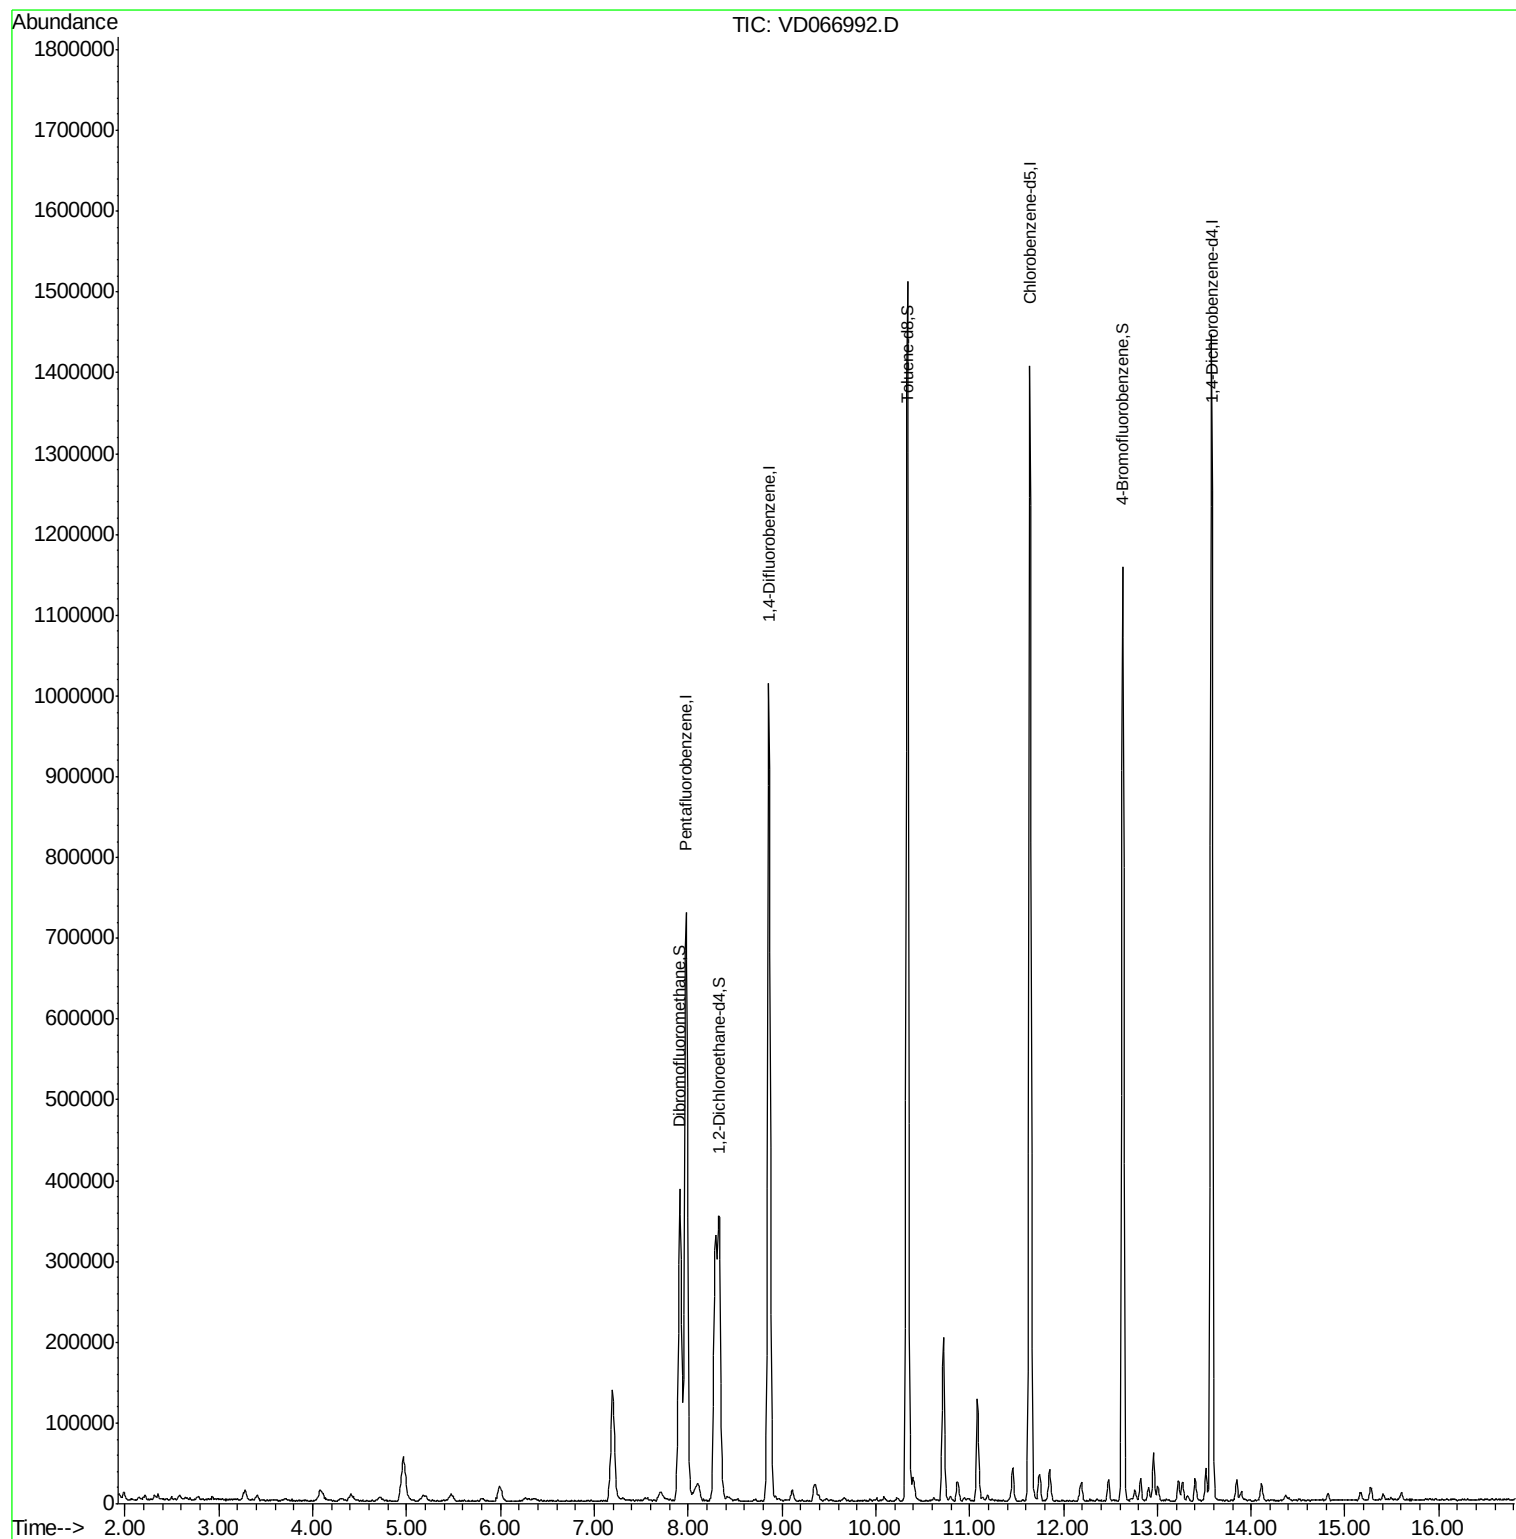

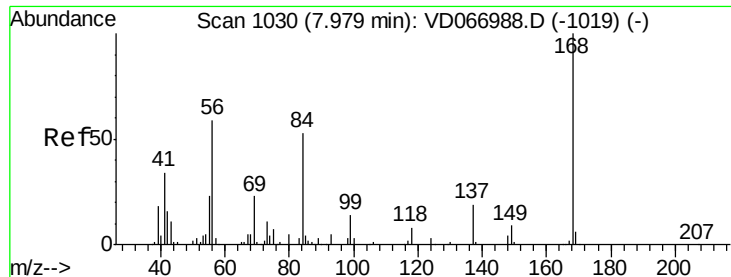

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VD066992.D

Acq: 01 Oct 2020 15:03

Instrument :

MSVOA_D

ClientSampleId :


VD1001SBL01

Tot Ion:168 Resp: 540836

Ion Ratio Lower Upper




168 100

99 59.0 44.1 66.1

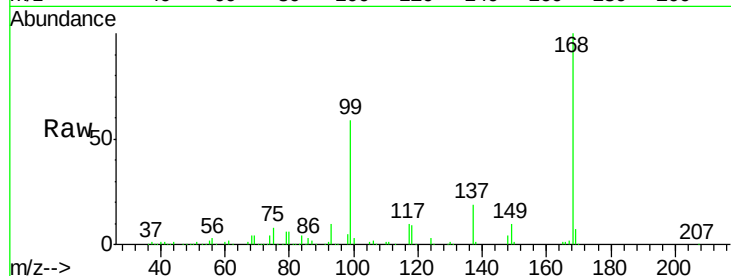

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

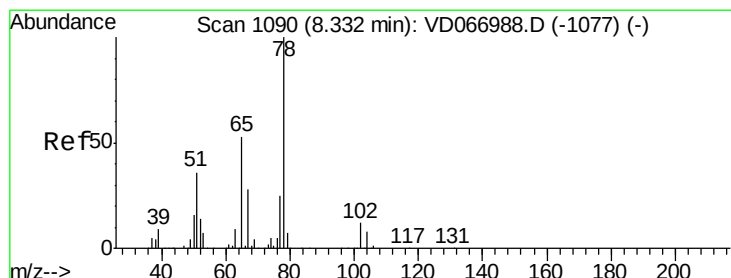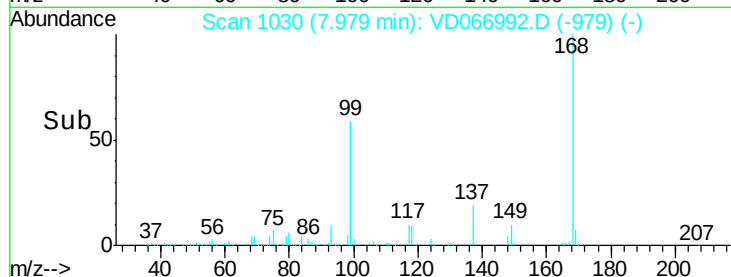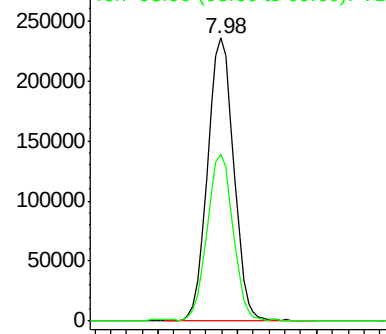

#33

1,2-Dichloroethane-d4

Concen: 49.122 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. 0.00 min

Lab File: VD066992.D


Acq: 01 Oct 2020 15:03

Tgt Ion: 65 Resp: 255894

Ion Ratio Lower Upper



65 100


67 54.8 0.0 106.8

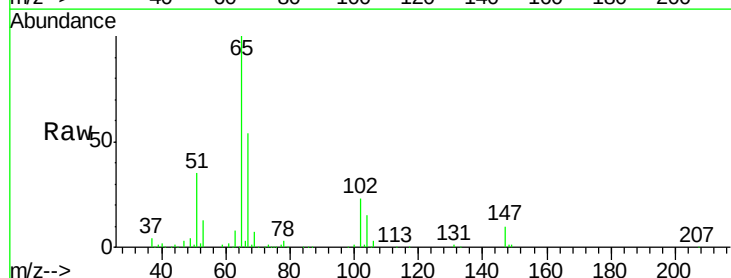

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

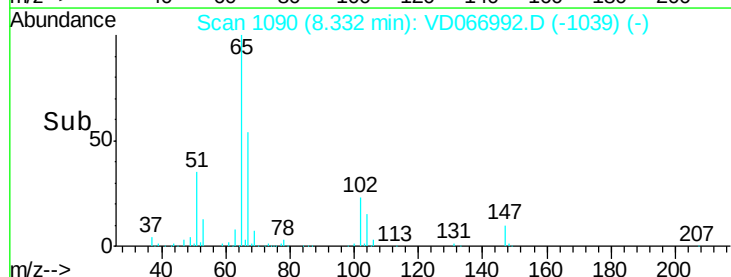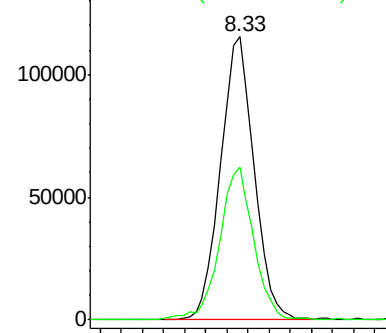

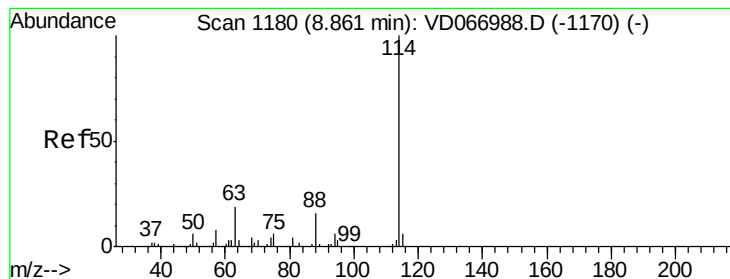

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.86 min Scan# 1180

Delta R.T. 0.00 min

Lab File: VD066992.D

Acq: 01 Oct 2020 15:03

Instrument :

MSVOA_D

ClientSampleId :

VD1001SBL01


Tot Ion:114 Resp: 883280

Ion Ratio Lower Upper

114 100

63 18.3 0.0 38.4




88 15.6 0.0 31.2

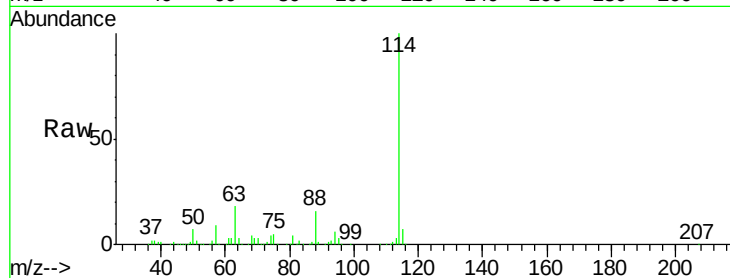

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

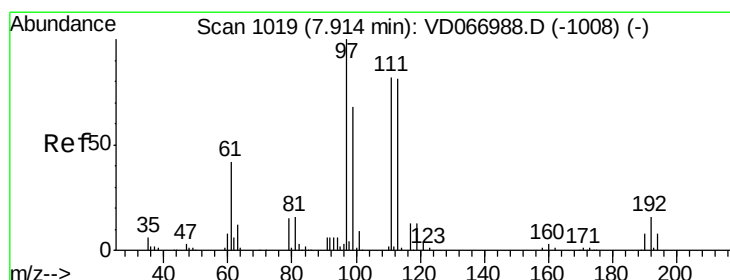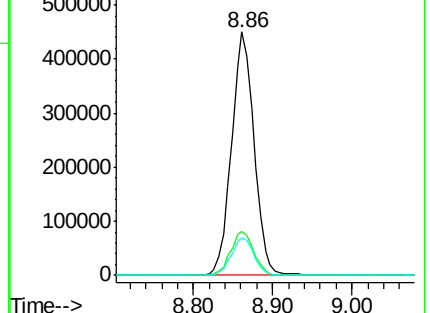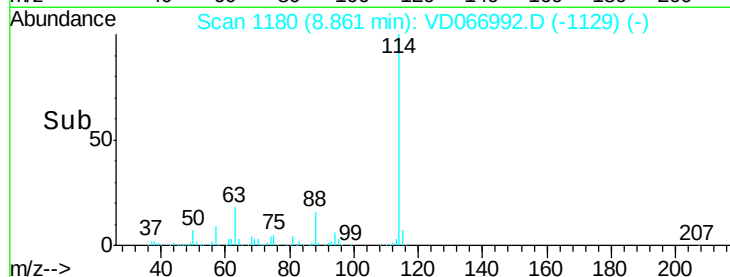

#35

Dibromofluoromethane

Concen: 47.418 ug/l

RT: 7.91 min Scan# 1019

Delta R.T. 0.00 min

Lab File: VD066992.D

Acq: 01 Oct 2020 15:03


Tgt Ion:113 Resp: 274204

Ion Ratio Lower Upper

113 100

111 103.6 83.0 124.4



192 19.8 15.5 23.3

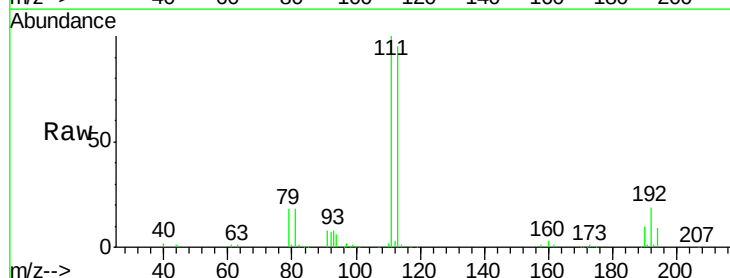


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



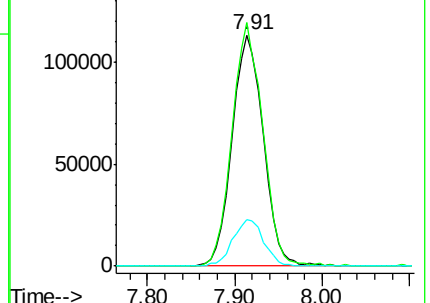
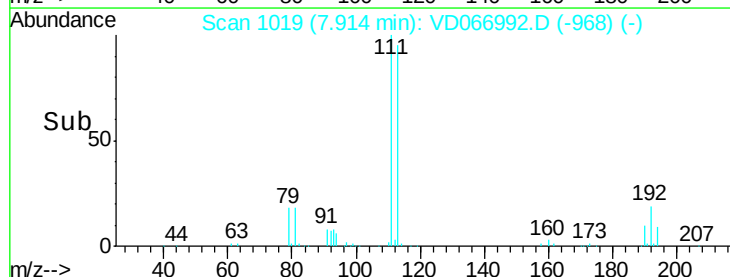


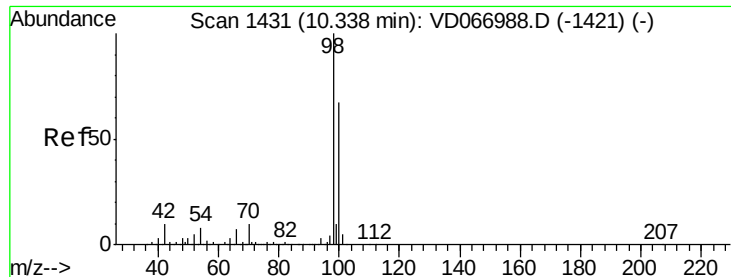

#50
Toluene-d8
Concen: 49.055 ug/l
RT: 10.34 min Scan# 1431
Delta R.T. 0.00 min
Lab File: VD066992.D
Acq: 01 Oct 2020 15:03




Instrument :
MSVOA_D
ClientSampleId :
VD1001SBL01


Tot Ion: 98 Resp: 1033664
Ion Ratio Lower Upper
98 100
100 65.6 52.8 79.2

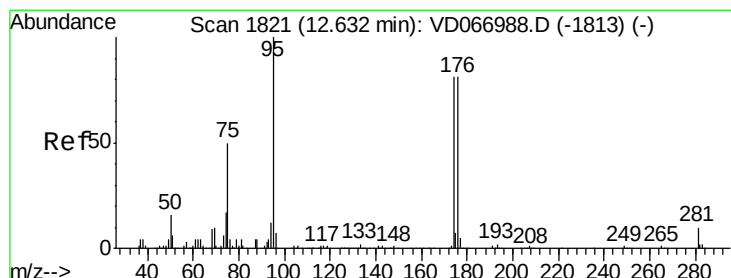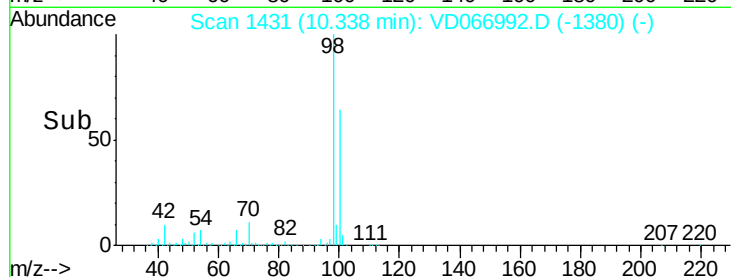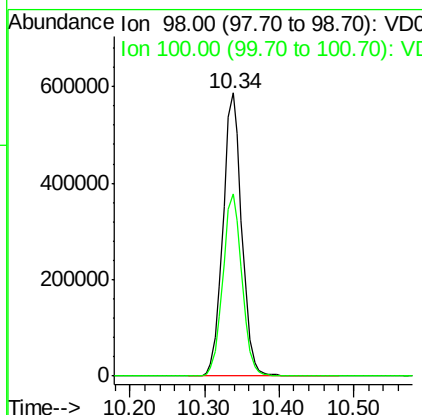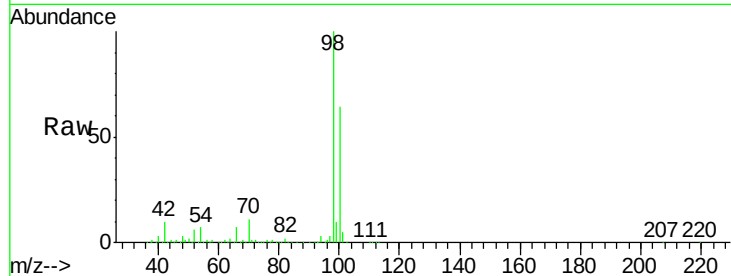

#62
4-Bromofluorobenzene
Concen: 51.100 ug/l
RT: 12.63 min Scan# 1821
Delta R.T. 0.00 min
Lab File: VD066992.D
Acq: 01 Oct 2020 15:03

Tgt Ion: 95 Resp: 365530
Ion Ratio Lower Upper
95 100
174 81.4 0.0 167.6
176 79.4 0.0 162.4


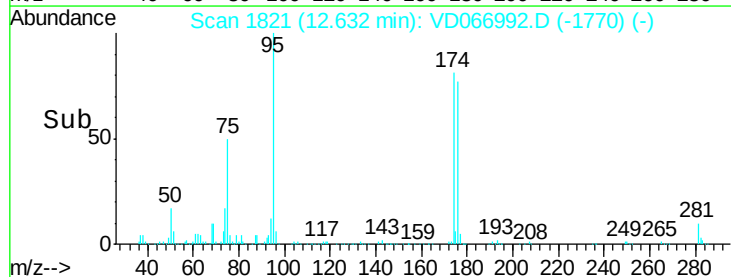
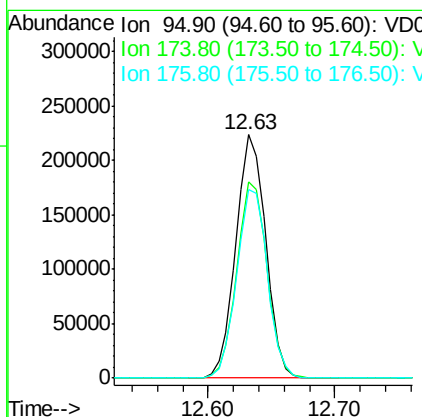
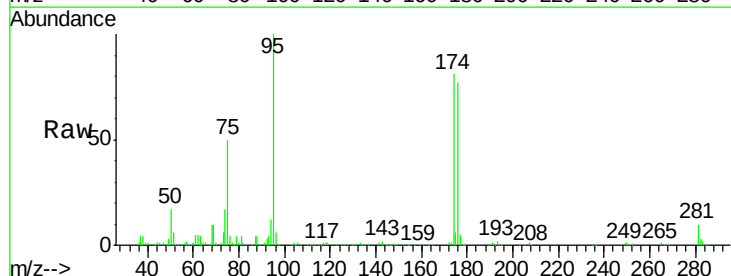


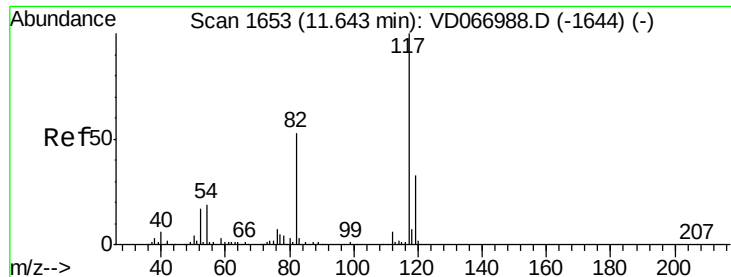

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.64 min Scan# 1653
Delta R.T. 0.00 min
Lab File: VD066992.D
Acq: 01 Oct 2020 15:03

Instrument :
MSVOA_D
ClientSampleId :
VD1001SBL01

Tot Ion:117 Resp: 845128
Ion Ratio Lower Upper
117 100
82 53.1 42.6 63.8
119 32.4 26.3 39.5

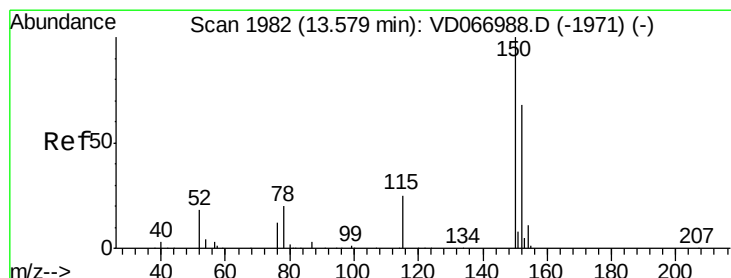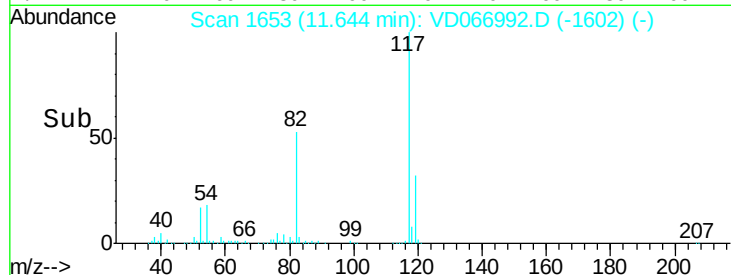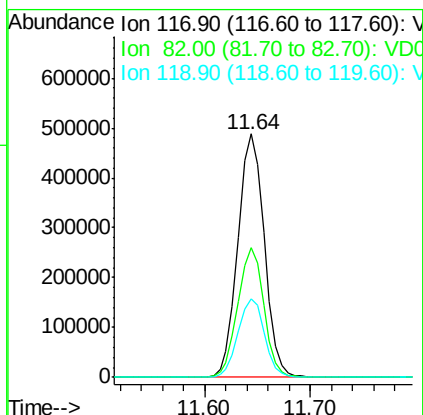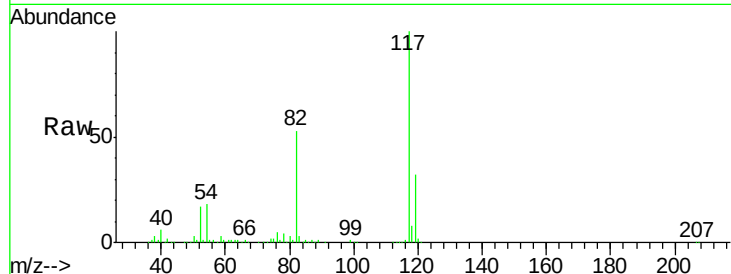

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. 0.00 min
Lab File: VD066992.D
Acq: 01 Oct 2020 15:03

Tgt Ion:152 Resp: 395308
Ion Ratio Lower Upper
152 100
115 59.5 29.6 88.8
150 157.1 0.0 344.8

