


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100120\
Data File : VD066983.D
Acq On : 01 Oct 2020 09:58
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
Title : SW846 8260
Last Update : Thu Oct 01 15:19:17 2020

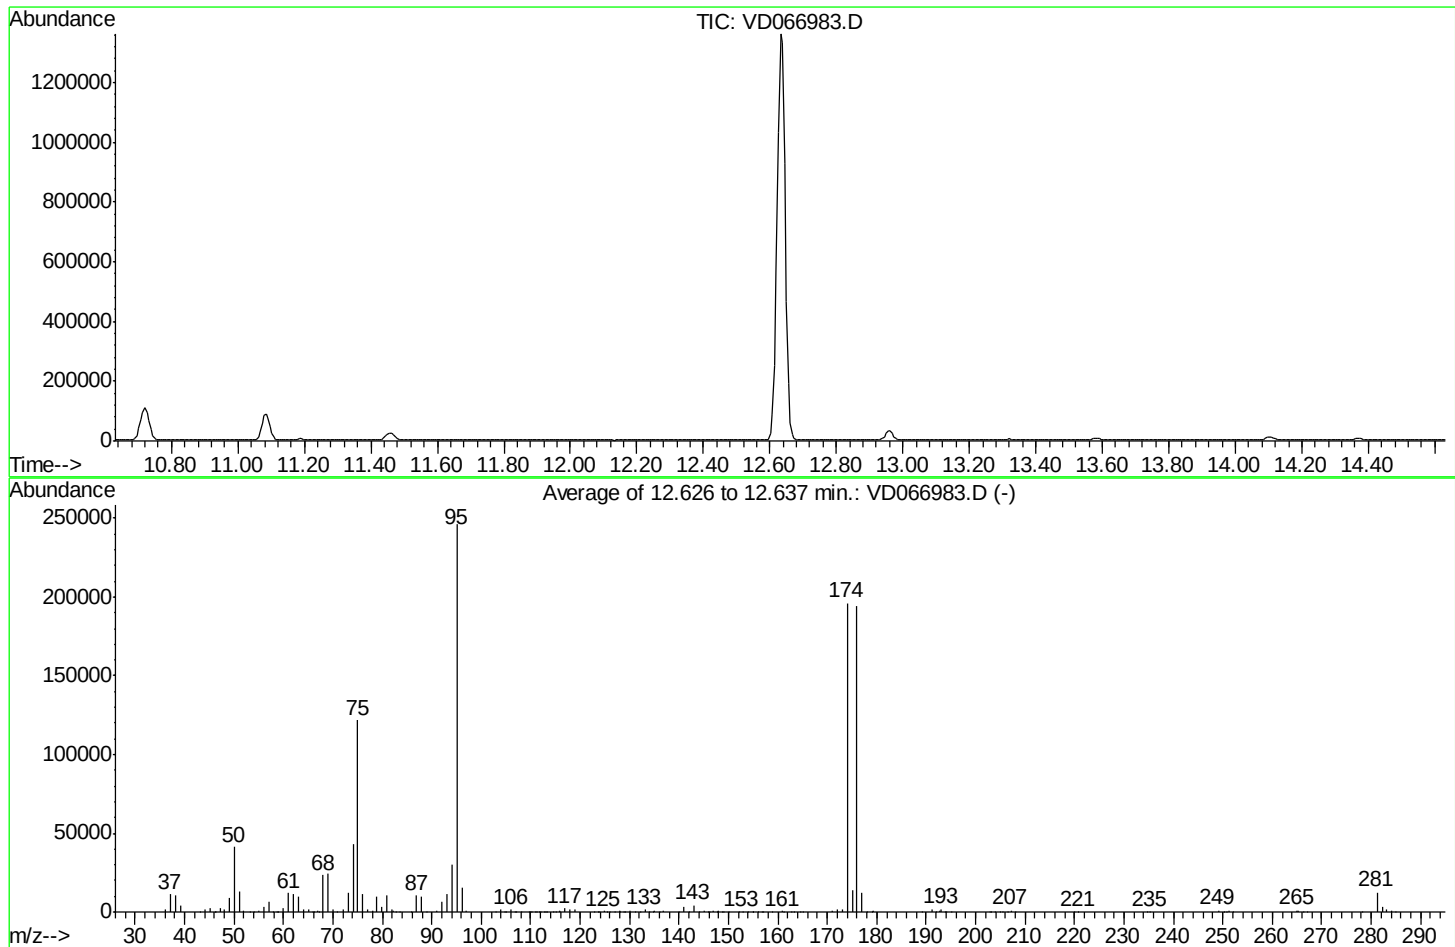

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	41338	PASS
75	95	30	60	49.4	121554	PASS
95	95	100	100	100.0	246144	PASS
96	95	5	9	6.3	15415	PASS
173	174	0.00	2	1.0	1881	PASS
174	95	50	100	79.6	195946	PASS
175	174	5	9	7.1	13977	PASS
176	174	95	101	99.1	194240	PASS
177	176	5	9	6.4	12356	PASS