


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100120\
 Data File : VD067006.D
 Acq On : 01 Oct 2020 21:52
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
 Title : SW846 8260
 Last Update : Thu Oct 01 15:19:17 2020

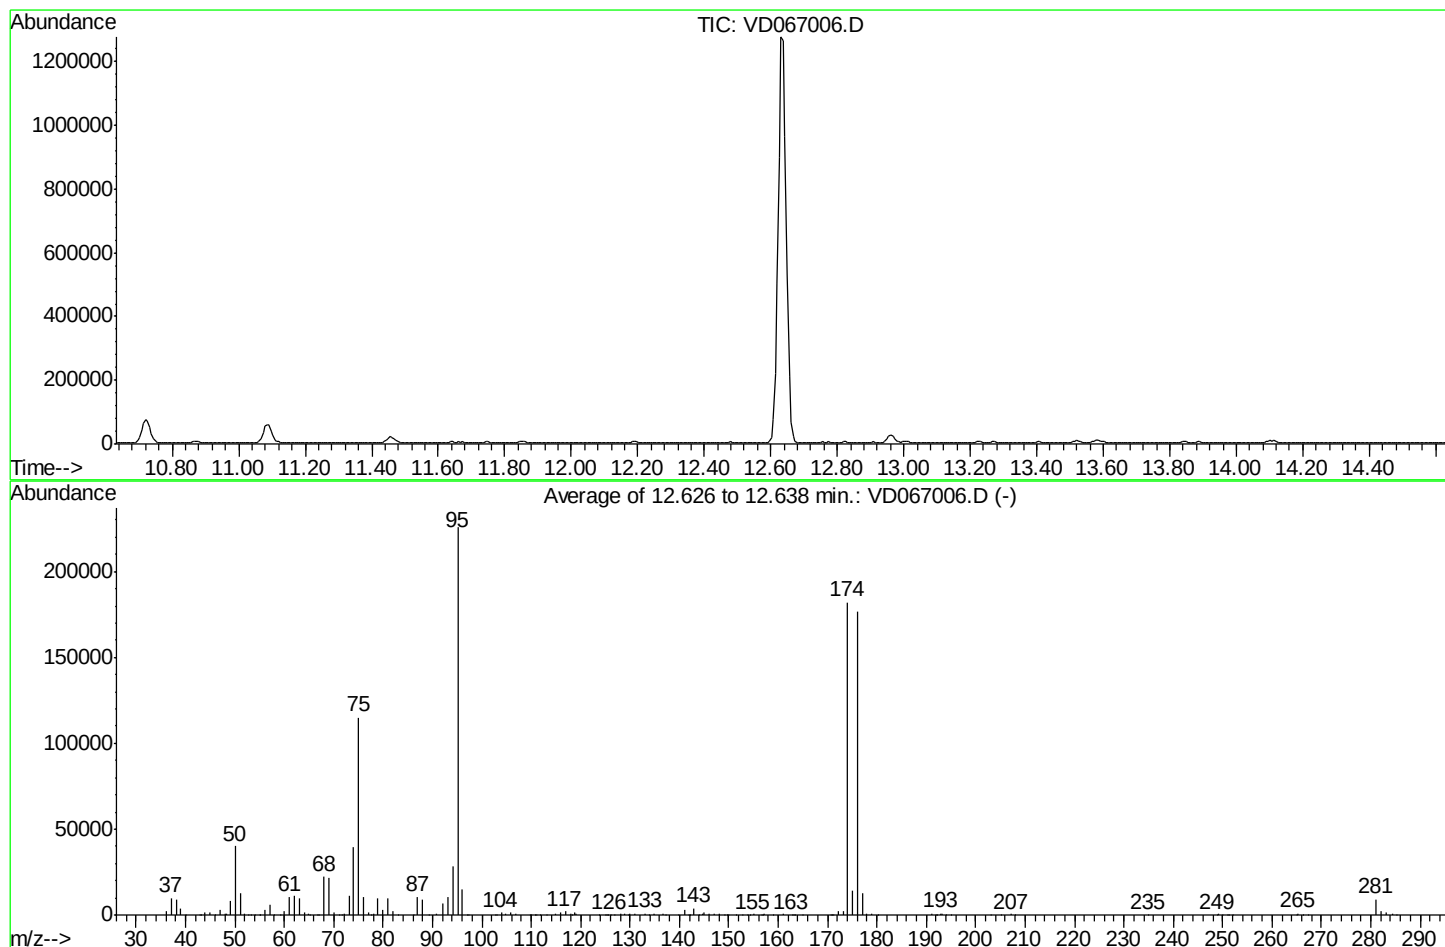

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	40205	PASS
75	95	30	60	50.9	114882	PASS
95	95	100	100	100.0	225728	PASS
96	95	5	9	6.8	15252	PASS
173	174	0.00	2	1.1	2086	PASS
174	95	50	100	80.6	181973	PASS
175	174	5	9	7.6	13880	PASS
176	174	95	101	97.1	176640	PASS
177	176	5	9	7.0	12388	PASS