


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100219\
 Data File : VD063860.D
 Acq On : 02 Oct 2019 13:40
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00µ/5.00mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100219S.M
 Title : SW846 8260
 Last Update : Fri Oct 04 01:55:35 2019

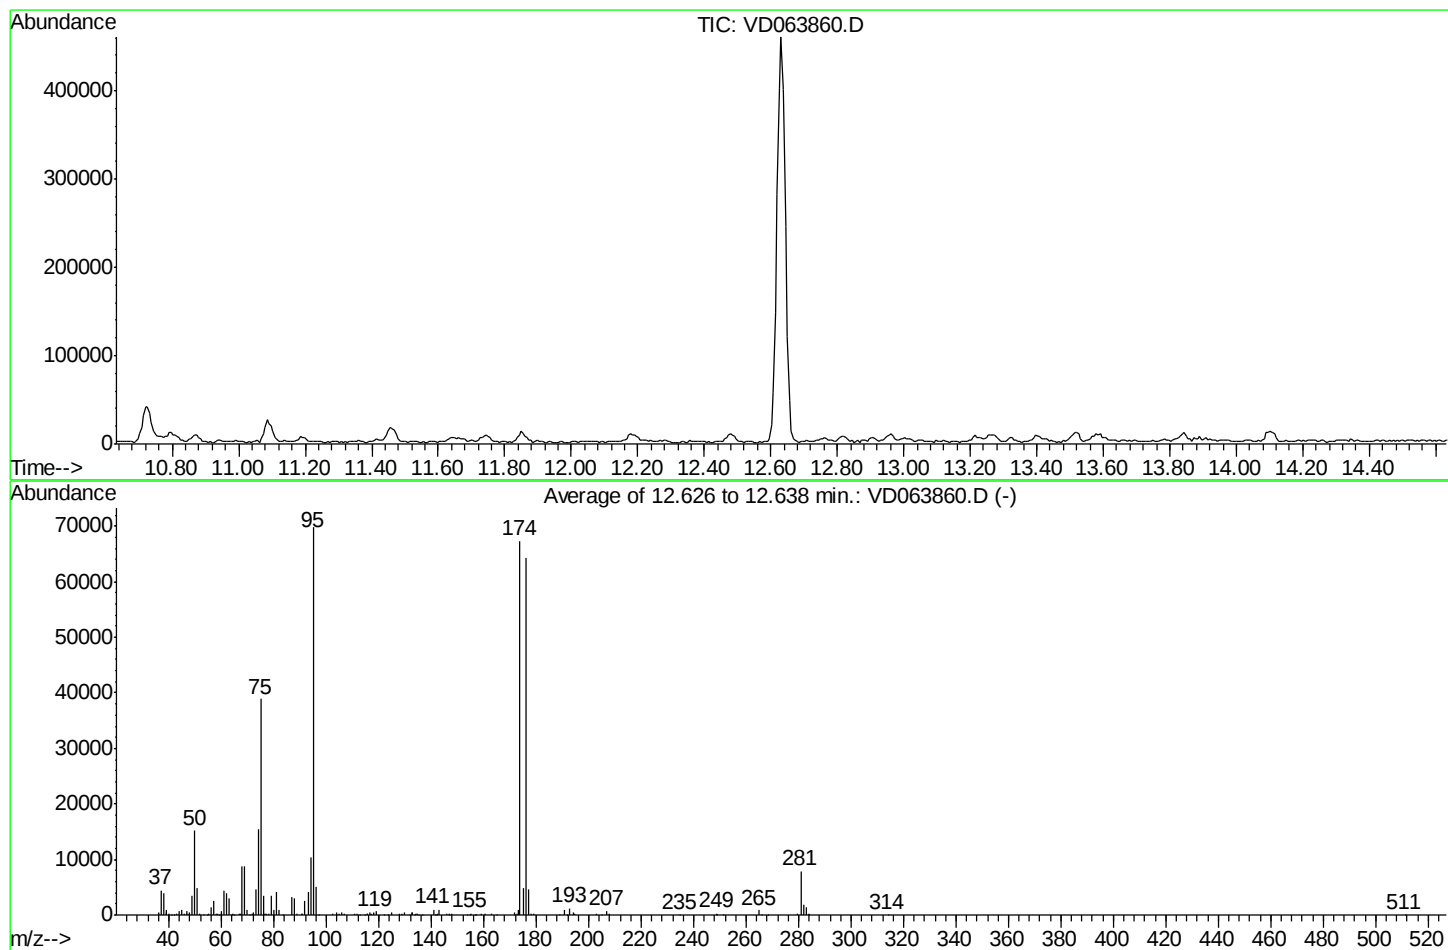

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	15212	PASS
75	95	30	60	55.7	38904	PASS
95	95	100	100	100.0	69810	PASS
96	95	5	9	7.3	5118	PASS
173	174	0.00	2	1.4	920	PASS
174	95	50	100	96.5	67357	PASS
175	174	5	9	7.1	4814	PASS
176	174	95	101	95.6	64384	PASS
177	176	5	9	7.1	4585	PASS