


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100318\  
Data File : VD060113.D  
Acq On : 3 Oct 2018 10:11  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µl/5ml/MSVOA D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D100118S.M  
Title : SW846 8260  
Last Update : Tue Oct 02 06:56:35 2018

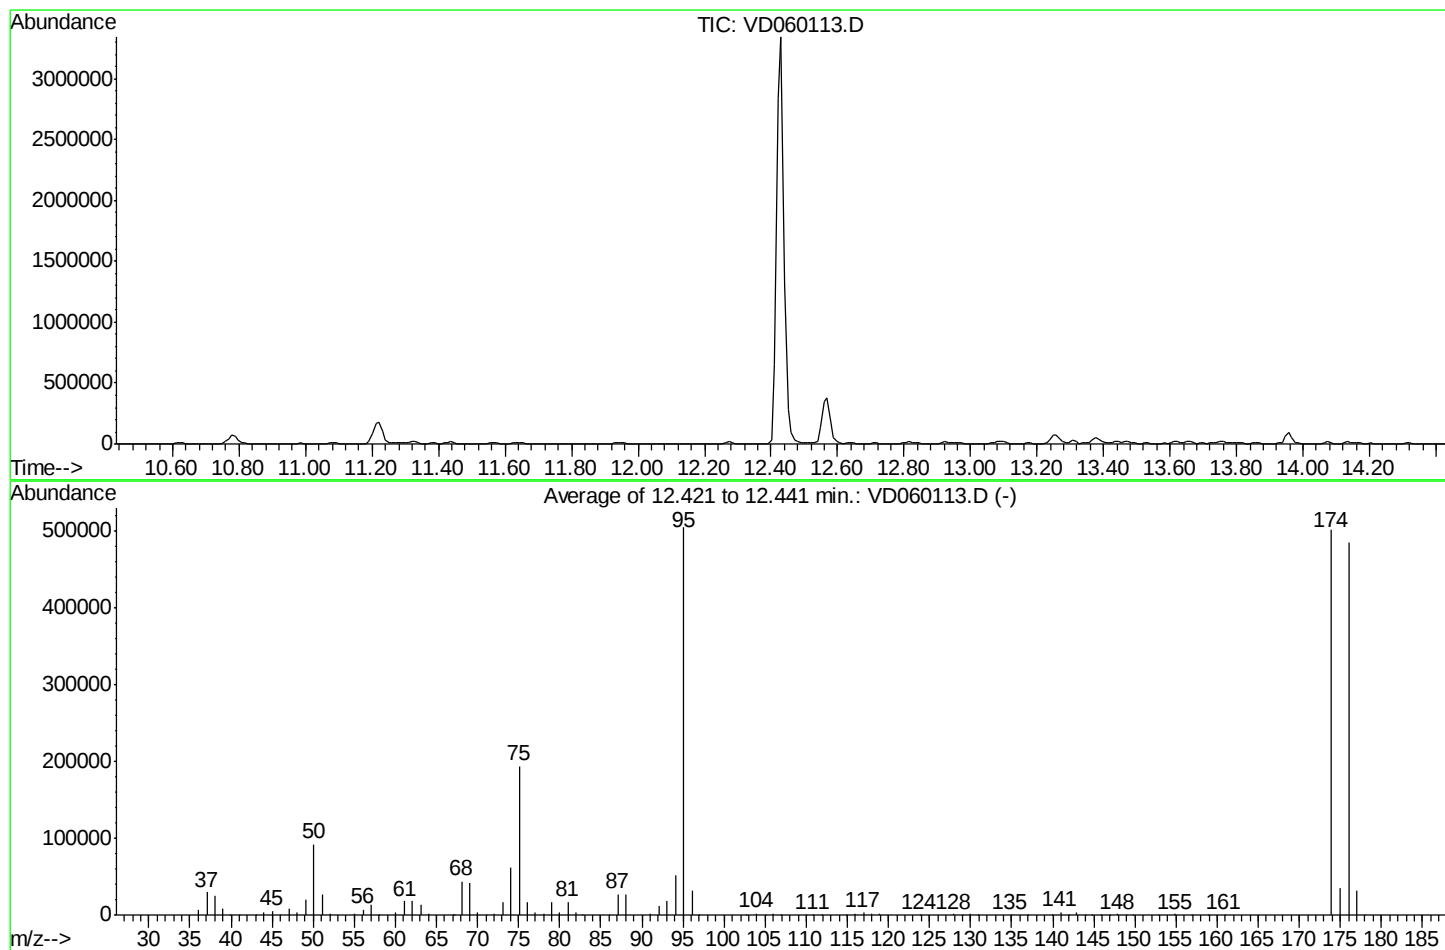

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1102

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.2      | 91925   | PASS             |
| 75          | 95           | 30           | 60           | 38.3      | 193528  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 505216  | PASS             |
| 96          | 95           | 5            | 9            | 6.4       | 32461   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 99.5      | 502656  | PASS             |
| 175         | 174          | 5            | 9            | 7.0       | 35085   | PASS             |
| 176         | 174          | 95           | 101          | 96.6      | 485760  | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 32029   | PASS             |