


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100319\
Data File : VD063874.D
Acq On : 03 Oct 2019 14:22
Operator : VA/SY
Sample : BFB
Misc : 5.00µ/5.00mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100219S.M
Title : SW846 8260
Last Update : Fri Oct 04 01:55:35 2019

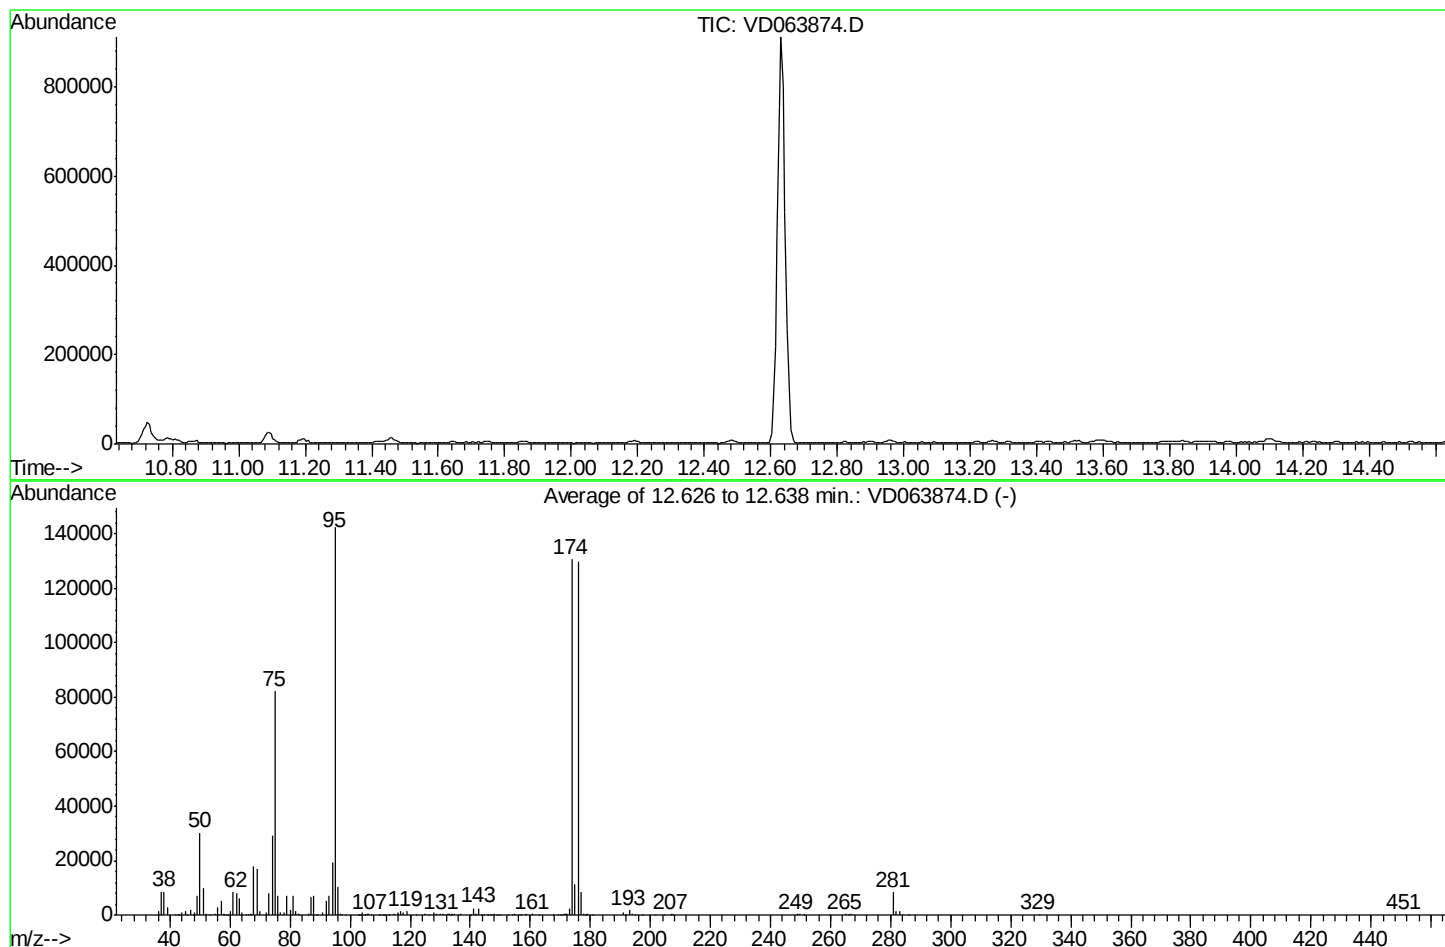

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	30302	PASS
75	95	30	60	57.7	82152	PASS
95	95	100	100	100.0	142461	PASS
96	95	5	9	7.2	10251	PASS
173	174	0.00	2	1.7	2246	PASS
174	95	50	100	91.8	130728	PASS
175	174	5	9	8.5	11094	PASS
176	174	95	101	99.3	129757	PASS
177	176	5	9	6.6	8562	PASS