


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100419\
 Data File : VD063883.D
 Acq On : 04 Oct 2019 09:44
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00µ/5.00mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100219S.M
 Title : SW846 8260
 Last Update : Sat Oct 05 03:51:17 2019

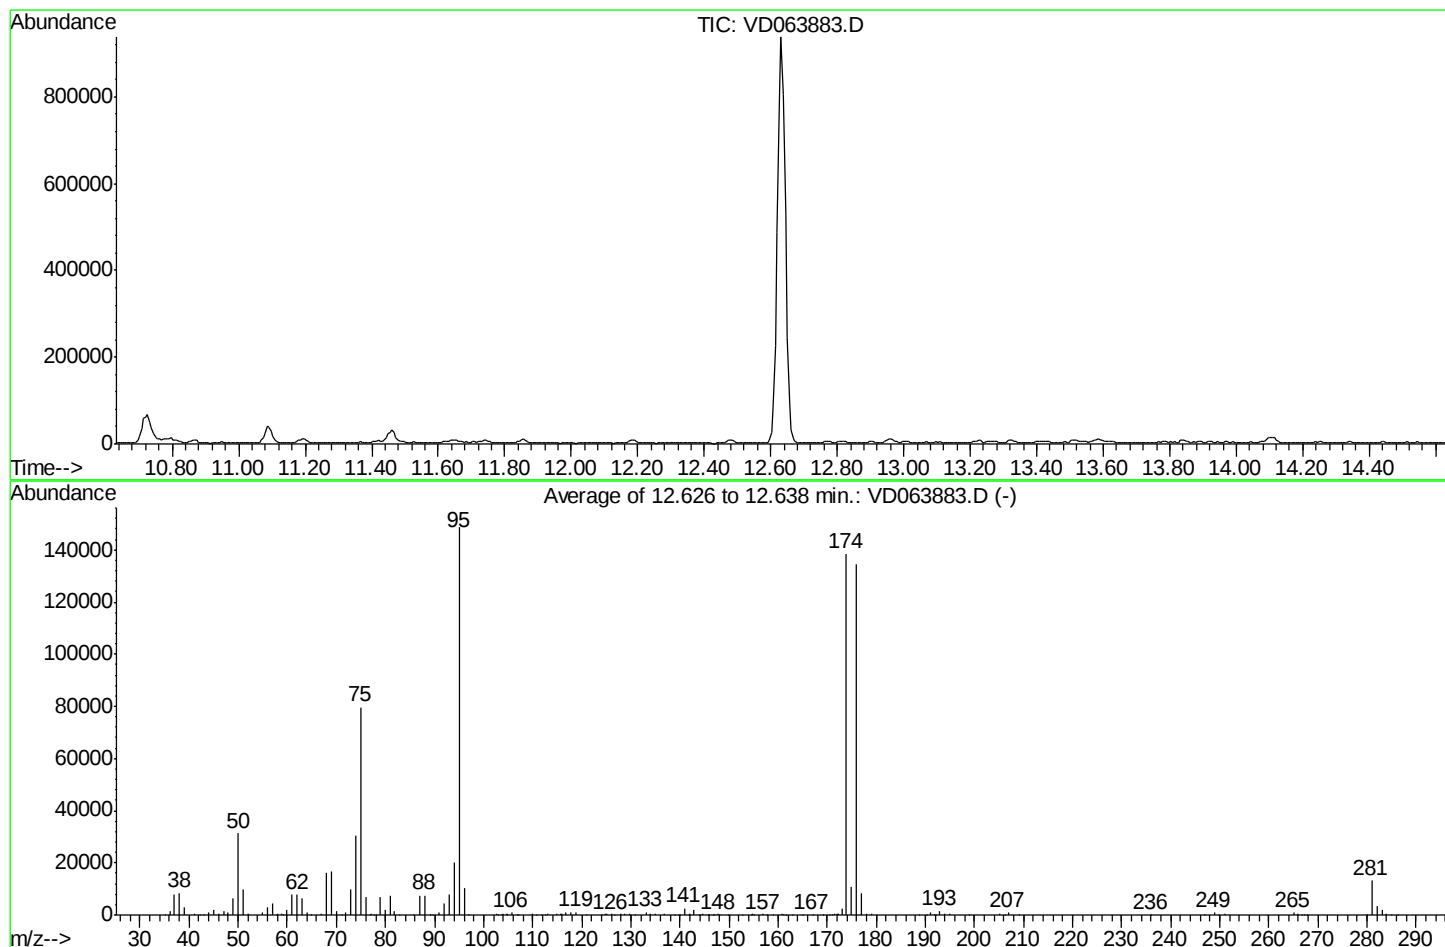

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	31362	PASS
75	95	30	60	53.6	79618	PASS
95	95	100	100	100.0	148629	PASS
96	95	5	9	6.9	10190	PASS
173	174	0.00	2	1.8	2520	PASS
174	95	50	100	93.3	138642	PASS
175	174	5	9	8.0	11031	PASS
176	174	95	101	96.8	134272	PASS
177	176	5	9	6.3	8447	PASS