

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100421\
 Data File : VD070554.D
 Acq On : 04 Oct 2021 16:41
 Operator : VA/SY
 Sample : M4032-01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 NB-08-100121

Quant Time: Oct 05 05:01:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 09 03:07:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.979	168	382303	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	813176	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	760264	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	328693	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	241535	49.204	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	98.400%		
35) Dibromofluoromethane	7.914	113	253337	43.767	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	87.540%		
50) Toluene-d8	10.338	98	1058584	50.371	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery =	100.740%		
62) 4-Bromofluorobenzene	12.626	95	348433	47.440	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery =	94.880%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.991	85	1127	Below Cal	#	70
3) Chloromethane	2.215	50	740	Below Cal		95
5) Bromomethane	2.750	94	58	Below Cal	#	4
6) Chloroethane	2.926	64	117	Below Cal	#	43
10) Methyl Iodide	4.303	142	220	1.074	ug/l #	39
16) Acetone	4.156	43	3201	3.652	ug/l #	64
20) Methylene Chloride	4.967	84	8817	Below Cal	#	94
31) Cyclohexane	7.961	56	31822	3.763	ug/l #	55
36) 1,1-Dichloropropene	7.973	75	33471	3.851	ug/l #	49
38) Carbon Tetrachloride	7.979	117	42954	4.997	ug/l #	17
39) Methylcyclohexane	9.350	83	64584	6.651	ug/l #	93
43) Isopropyl Acetate	8.450	43	6830	1.137	ug/l #	46
48) Methyl methacrylate	9.402	41	5665	2.042	ug/l #	10
51) 4-Methyl-2-Pentanone	10.332	43	9399	3.022	ug/l #	39
55) 1,1,2-Trichloroethane	10.773	97	19866	4.196	ug/l #	23
56) Ethyl methacrylate	10.685	69	5792	1.121	ug/l #	3
59) 2-Hexanone	10.938	43	8522	4.107	ug/l #	23
73) Isopropylbenzene	12.473	105	24271	1.053	ug/l	98
74) N-amyl acetate	12.255	43	8304	1.653	ug/l #	61
76) 1,2,3-Trichloropropane	12.626	75	164646	49.521	ug/l #	1
78) n-propylbenzene	12.808	91	86258	2.883	ug/l	95
80) 1,3,5-Trimethylbenzene	12.949	105	74842	3.762	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.626	75	164646	124.079	ug/l #	18
84) 1,2,4-Trimethylbenzene	13.261	105	221992	11.332	ug/l	100
85) sec-Butylbenzene	13.391	105	40696	1.605	ug/l #	40
86) p-Isopropyltoluene	13.502	119	54250	2.662	ug/l	98
89) n-Butylbenzene	13.832	91	155993	7.678	ug/l #	82
90) Hexachloroethane	14.102	117	152159	32.620	ug/l #	18
92) 1,2-Dibromo-3-Chloropr...	14.508	75	9625	13.018	ug/l #	5
95) Naphthalene	15.385	128	4065564	424.050	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100421\
Data File : VD070554.D
Acq On : 04 Oct 2021 16:41
Operator : VA/SY
Sample : M4032-01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121

Quant Time: Oct 05 05:01:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Quant Title : SW846 8260
QLast Update : Thu Sep 09 03:07:09 2021
Response via : Initial Calibration




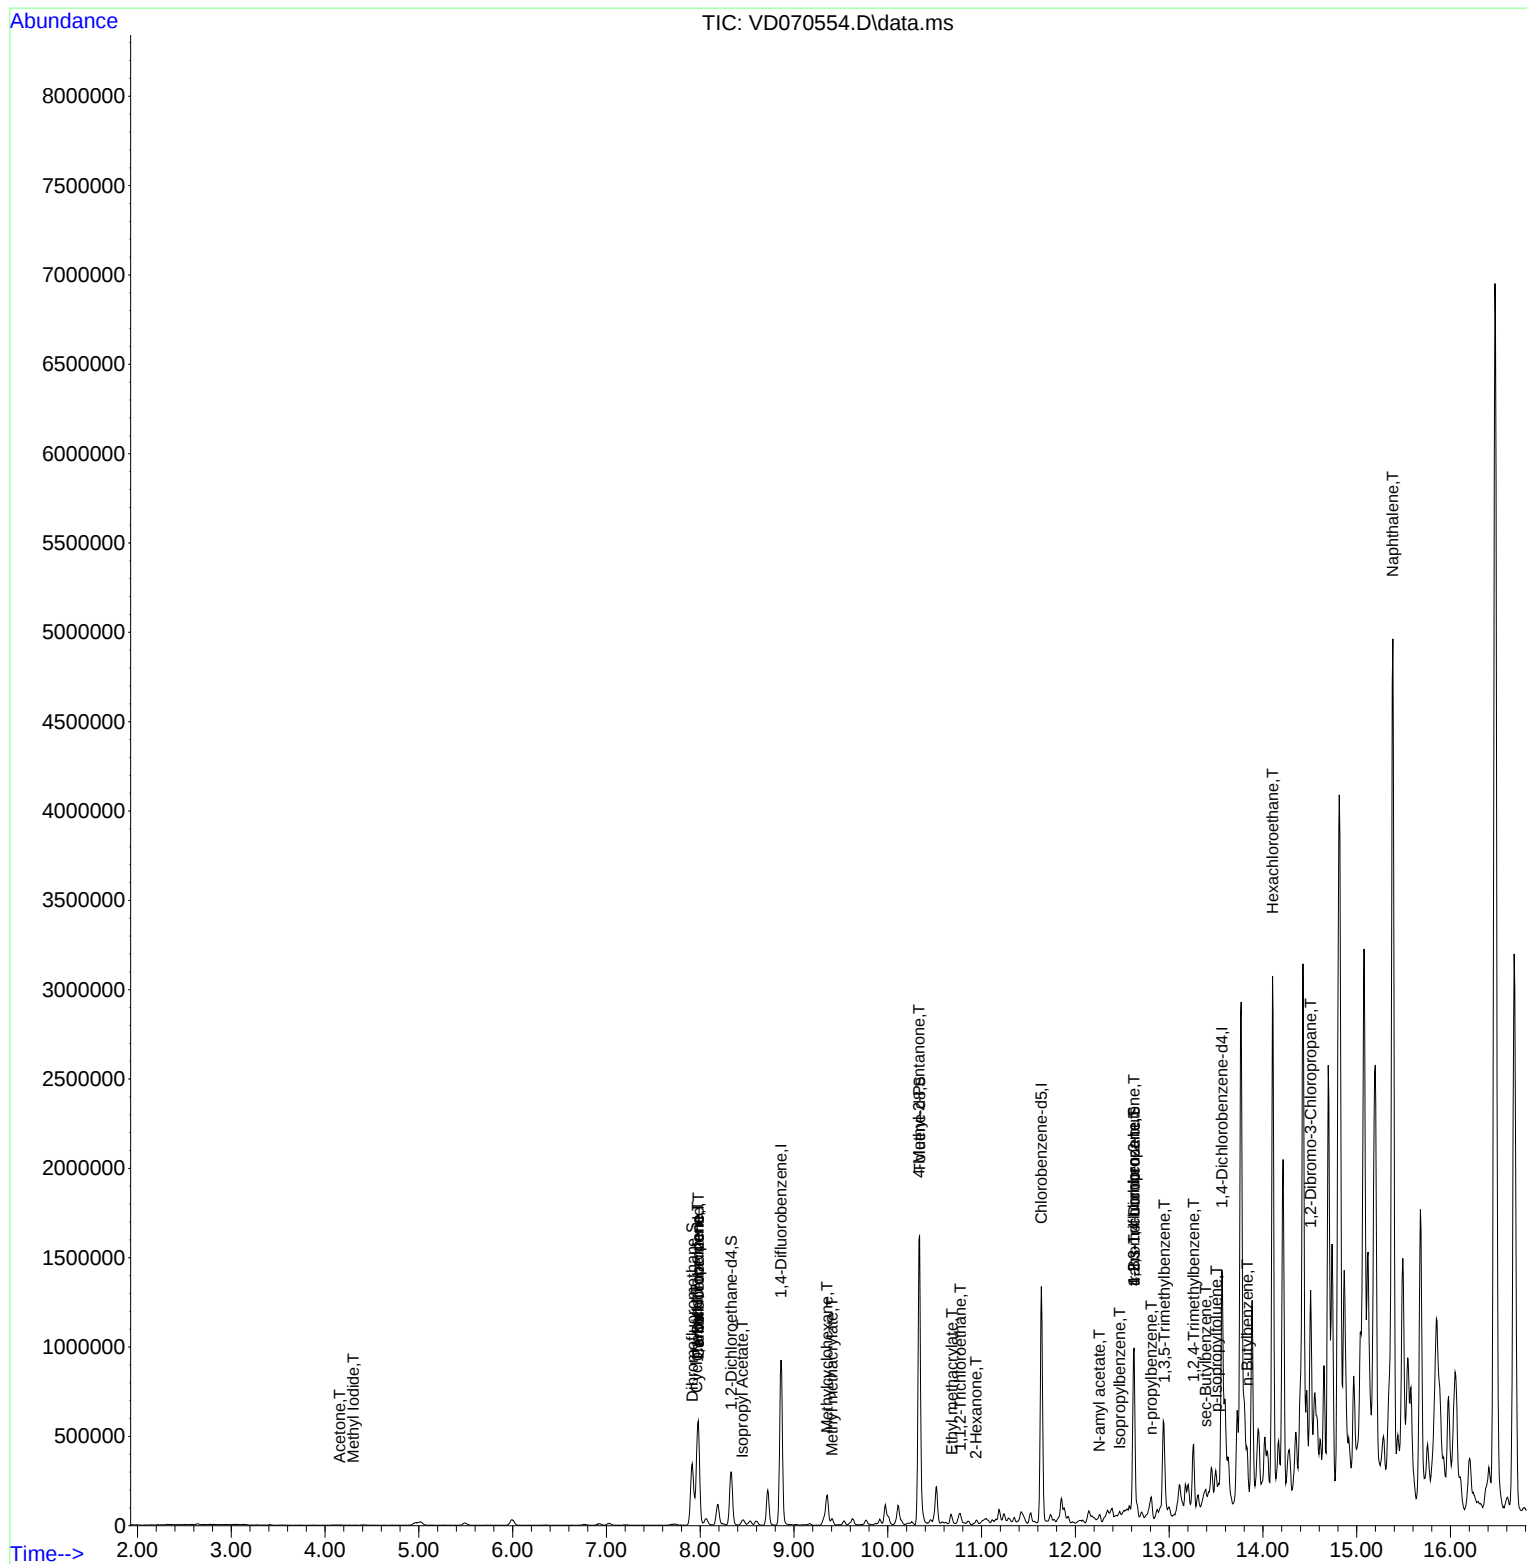




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion:168 Resp: 382303
Ion Ratio Lower Upper
168 100
99 65.7 50.8 76.2

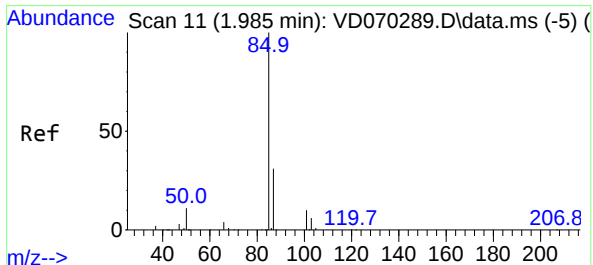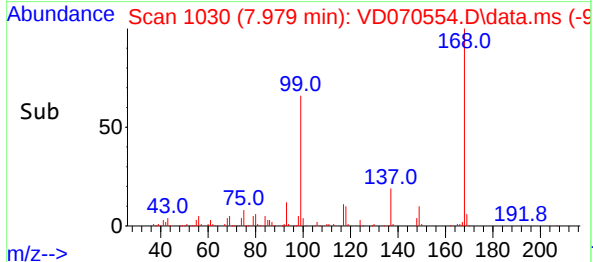

#2
Dichlorodifluoromethane
Concen: Below Cal
RT: 1.991 min Scan# 12
Delta R.T. 0.006 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 85 Resp: 1127
Ion Ratio Lower Upper
85 100
87 14.6 15.6 46.8#


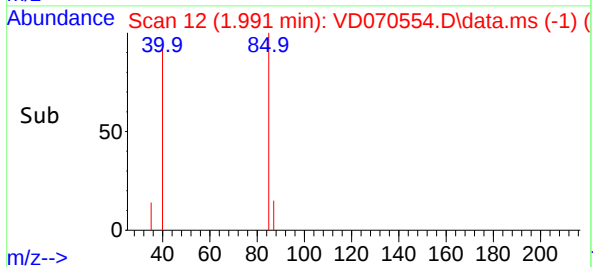

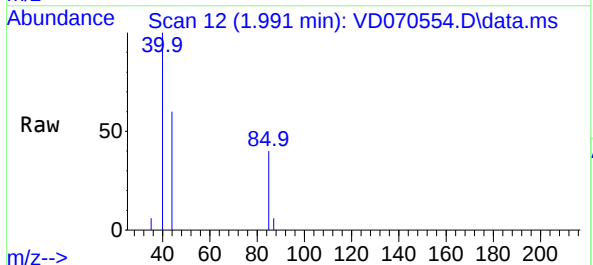




#3
Chloromethane
Concen: Below Cal
RT: 2.215 min Scan# 50
Delta R.T. 0.006 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 50 Resp: 740
Ion Ratio Lower Upper
50 100
52 35.2 26.2 39.2

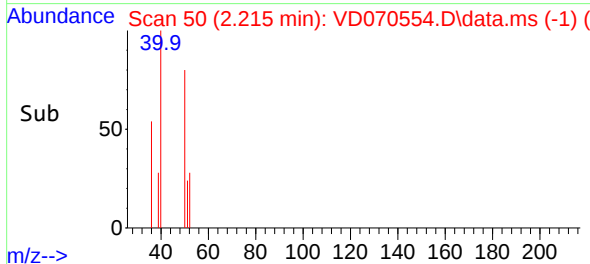

#5
Bromomethane
Concen: Below Cal
RT: 2.750 min Scan# 141
Delta R.T. -0.012 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 94 Resp: 58
Ion Ratio Lower Upper
94 100
96 0.0 73.0 109.6#


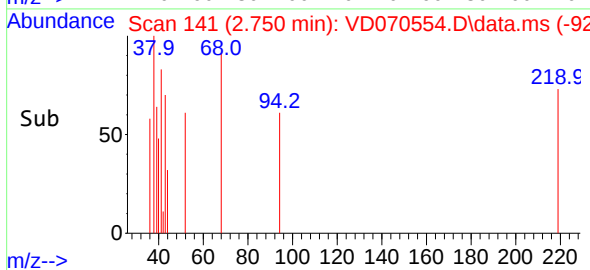

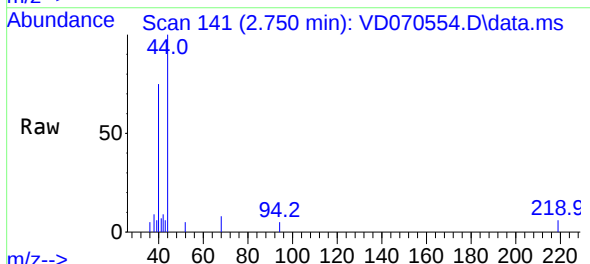




#6
Chloroethane
Concen: Below Cal
RT: 2.926 min Scan# 171
Delta R.T. 0.005 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 64 Resp: 117
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#



#10
Methyl Iodide
Concen: 1.074 ug/l
RT: 4.303 min Scan# 405
Delta R.T. 0.006 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 142 Resp: 220
Ion Ratio Lower Upper
142 100
127 0.0 36.9 55.3#
141 0.0 11.8 17.6#


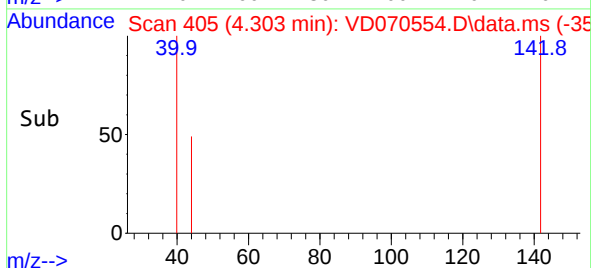
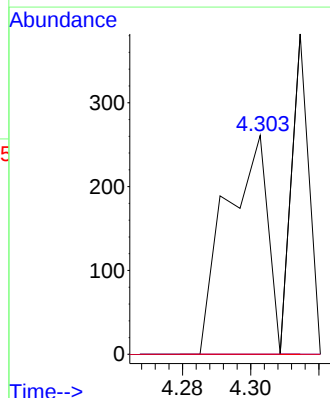





#16
Acetone
Concen: 3.652 ug/l
RT: 4.156 min Scan# 380
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 43 Resp: 3201
Ion Ratio Lower Upper
43 100
58 16.9 30.9 46.3#

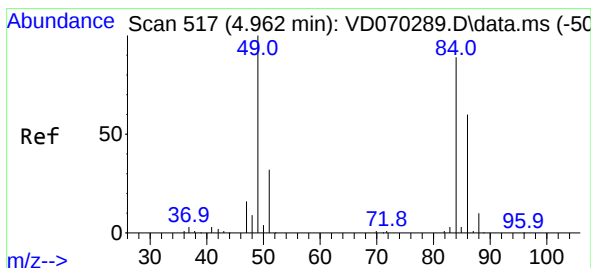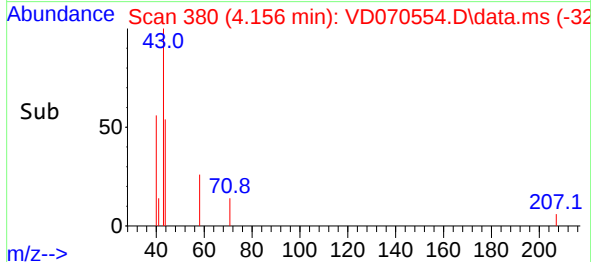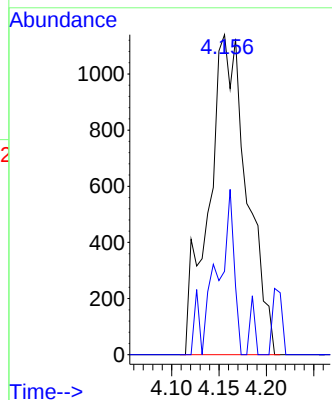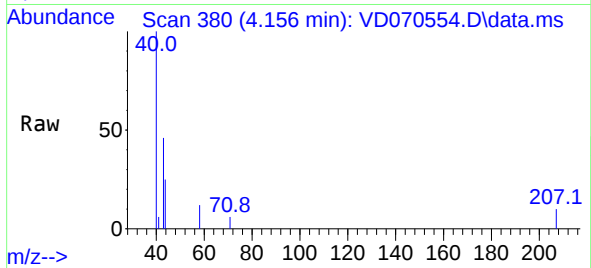

#20
Methylene Chloride
Concen: Below Cal
RT: 4.967 min Scan# 518
Delta R.T. 0.005 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 84 Resp: 8817
Ion Ratio Lower Upper
84 100
49 117.2 89.6 134.4
51 26.4 28.6 43.0#
86 64.0 53.5 80.3

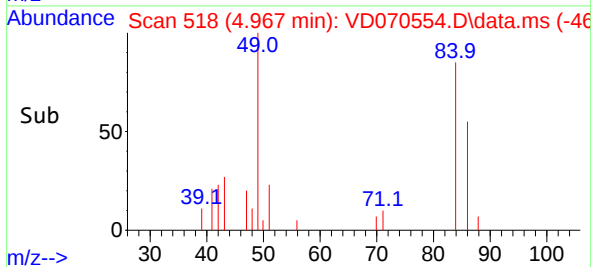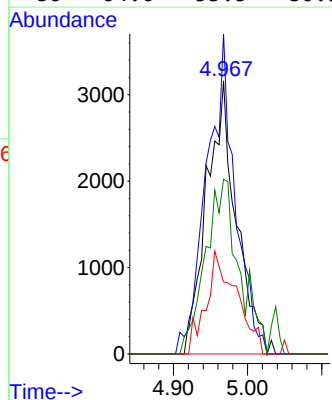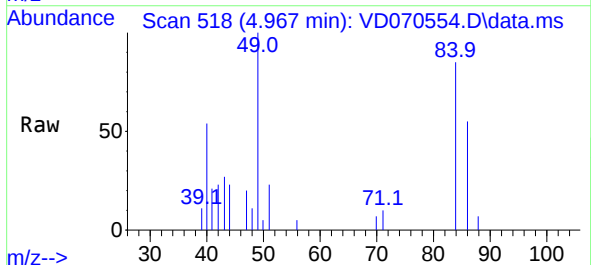



#31

Cyclohexane

Concen: 3.763 ug/l

RT: 7.961 min Scan# 1027

Delta R.T. -0.024 min

Lab File: VD070554.D

Acq: 04 Oct 2021 16:41

Tgt Ion: 56 Resp: 31822

Ion Ratio Lower Upper

56 100

69 63.1 26.9 40.3#





84 51.7 73.6 110.4#

Instrument :

MSVOA_D

ClientSampleId :

NB-08-100121



#33

1,2-Dichloroethane-d4

Concen: 49.204 ug/l

RT: 8.332 min Scan# 1090

Delta R.T. 0.006 min

Lab File: VD070554.D




Acq: 04 Oct 2021 16:41


Tgt Ion: 65 Resp: 241535

Ion Ratio Lower Upper

65 100

67 54.1 0.0 111.4

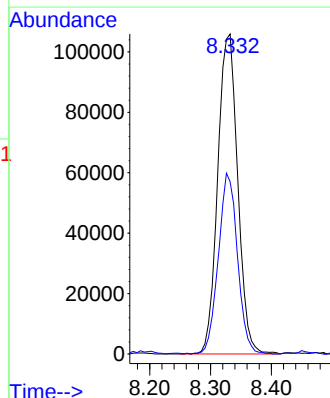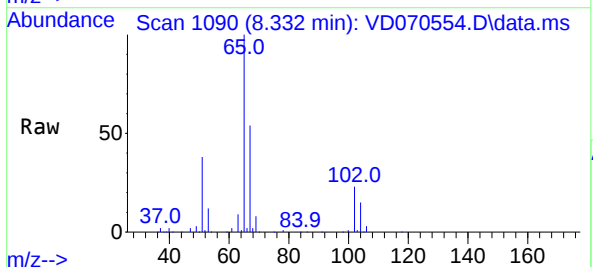




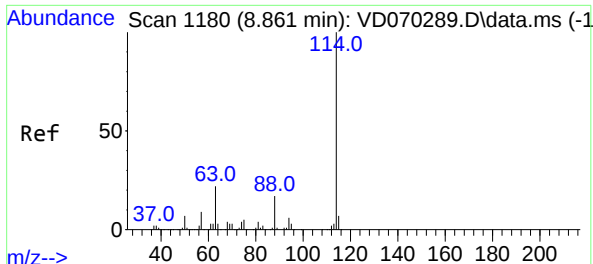


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121




Tgt Ion:	114	Resp:	813176
Ion	Ratio	Lower	Upper
114	100		
63	20.1	0.0	43.4
88	16.3	0.0	33.4

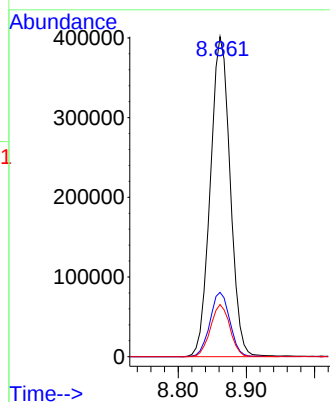


#35

Dibromofluoromethane
Concen: 43.767 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion:	113	Resp:	253337
Ion	Ratio	Lower	Upper
113	100		
111	104.6	81.4	122.2
192	16.1	13.0	19.6

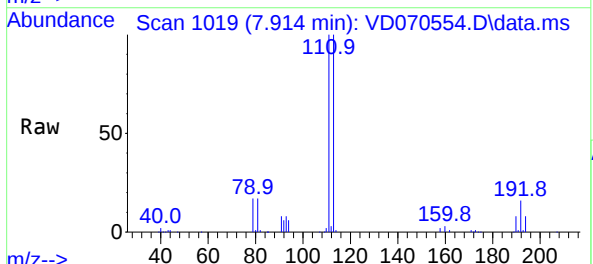







#36

1,1-Dichloropropene
Concen: 3.851 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.135 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121




Tgt Ion: 75 Resp: 33471
Ion Ratio Lower Upper
75 100
110 7.5 17.9 53.7#
77 1.4 25.3 37.9#

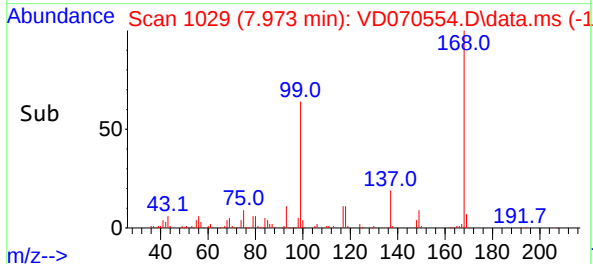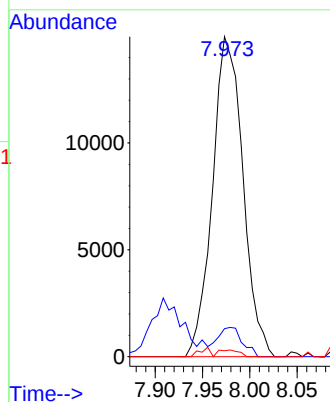


#38

Carbon Tetrachloride
Concen: 4.997 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.118 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 117 Resp: 42954
Ion Ratio Lower Upper
117 100
119 6.1 76.1 114.1#
121 0.0 23.8 35.6#

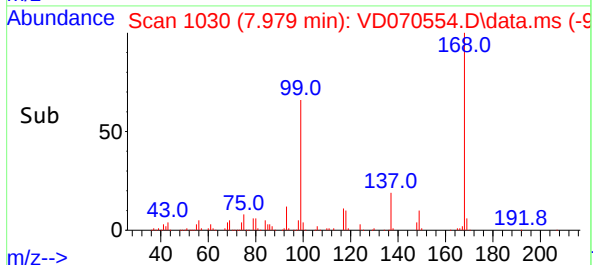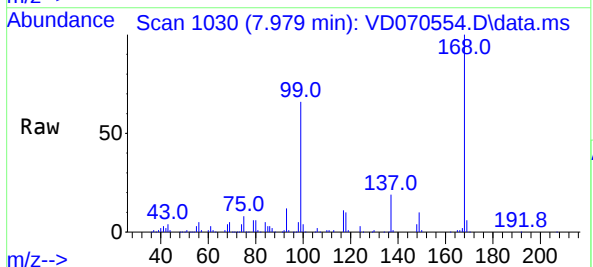



#39

Methylcyclohexane

Concen: 6.651 ug/l

RT: 9.350 min Scan# 1263





Delta R.T. -0.000 min

Lab File: VD070554.D

Acq: 04 Oct 2021 16:41

Tgt Ion:	83	Resp:	64584
Ion	Ratio	Lower	Upper
83	100		
55	70.9	58.5	87.7
98	38.0	38.4	57.6#

Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121

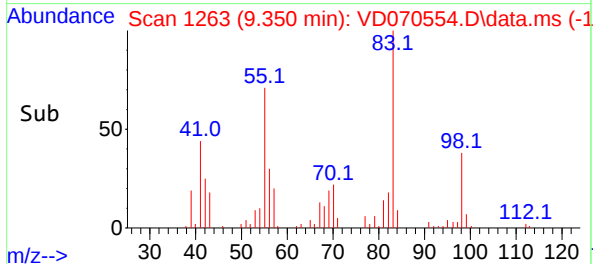

#43

Isopropyl Acetate

Concen: 1.137 ug/l




RT: 8.450 min Scan# 1110


Delta R.T. -0.000 min

Lab File: VD070554.D

Acq: 04 Oct 2021 16:41

Tgt Ion:	43	Resp:	6830
Ion	Ratio	Lower	Upper
43	100		
61	0.0	29.0	43.6#
87	0.0	12.8	19.2#

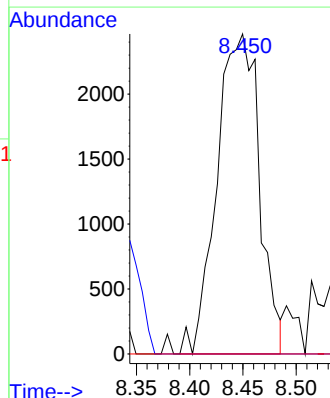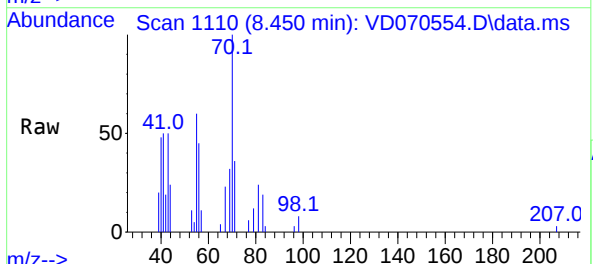







#48

Methyl methacrylate
Concen: 2.042 ug/l
RT: 9.402 min Scan# 1272
Delta R.T. -0.047 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121




Tgt Ion: 41 Resp: 5665
Ion Ratio Lower Upper
41 100
69 0.0 79.8 119.8#
39 0.0 34.4 51.6#

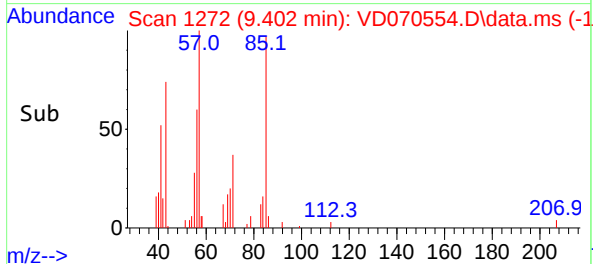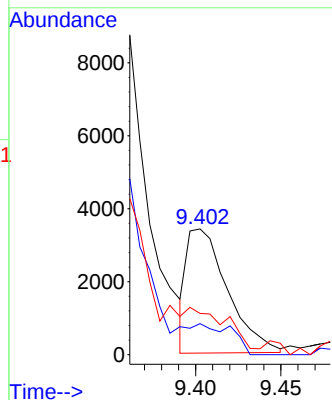


#50

Toluene-d8
Concen: 50.371 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 98 Resp: 1058584
Ion Ratio Lower Upper
98 100
100 65.0 52.0 78.0



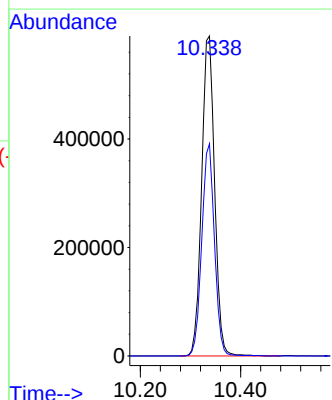
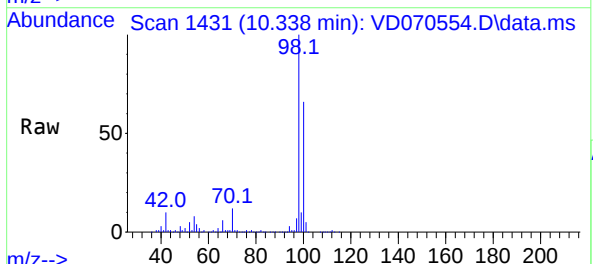




#51
4-Methyl-2-Pentanone
Concen: 3.022 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. 0.106 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 43 Resp: 9399
Ion Ratio Lower Upper
43 100
58 83.9 35.4 53.2#

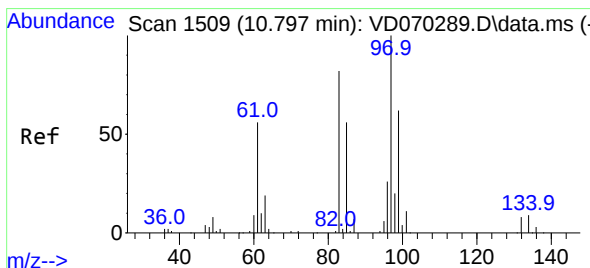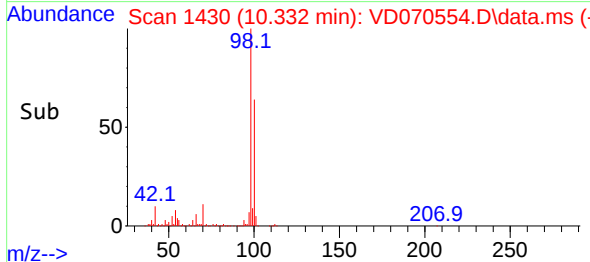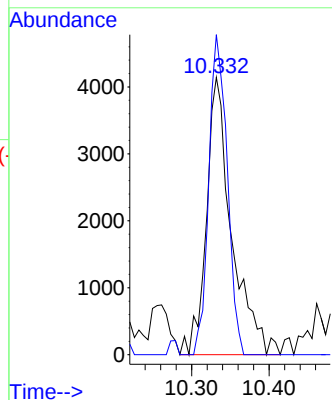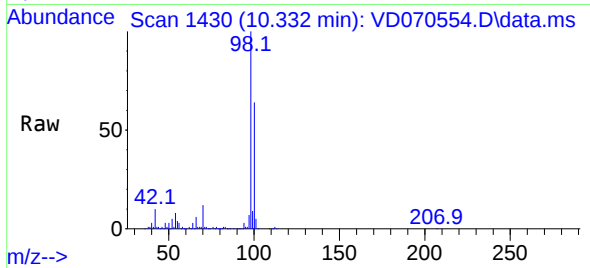

#55
1,1,2-Trichloroethane
Concen: 4.196 ug/l
RT: 10.773 min Scan# 1505
Delta R.T. -0.024 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 97 Resp: 19866
Ion Ratio Lower Upper
97 100
83 10.3 65.3 97.9#
85 5.8 44.8 67.2#
99 0.0 49.7 74.5#


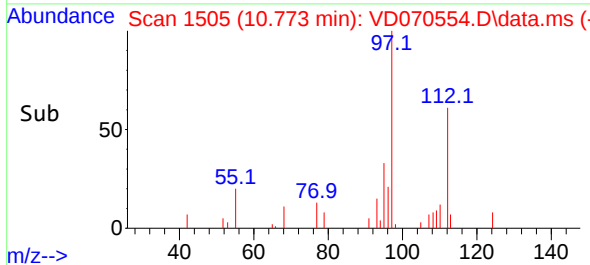
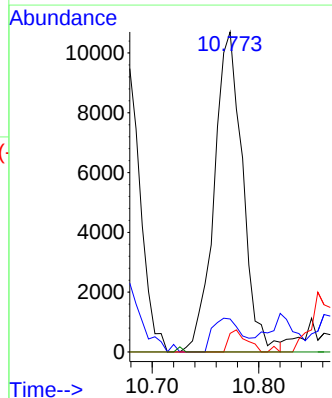
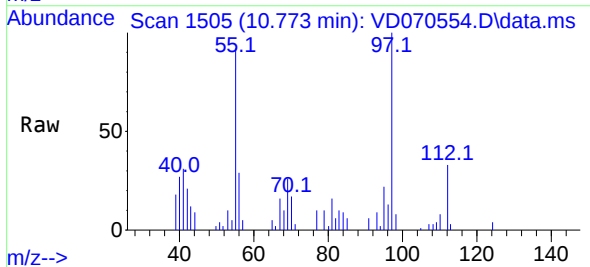




#56
Ethyl methacrylate
Concen: 1.121 ug/l
RT: 10.685 min Scan# 1490
Delta R.T. 0.029 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 69 Resp: 5792
Ion Ratio Lower Upper
69 100
41 129.3 43.6 65.4#
39 63.1 18.6 28.0#

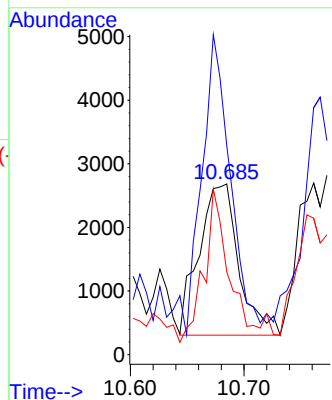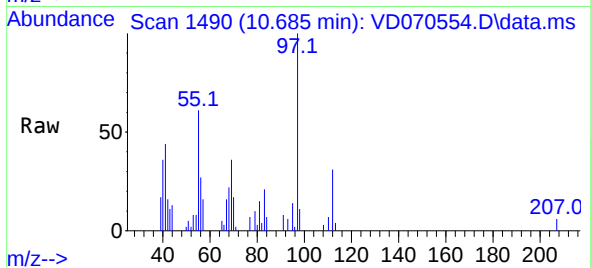

#59
2-Hexanone
Concen: 4.107 ug/l
RT: 10.938 min Scan# 1533
Delta R.T. -0.041 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 43 Resp: 8522
Ion Ratio Lower Upper
43 100
58 2.3 30.6 91.6#

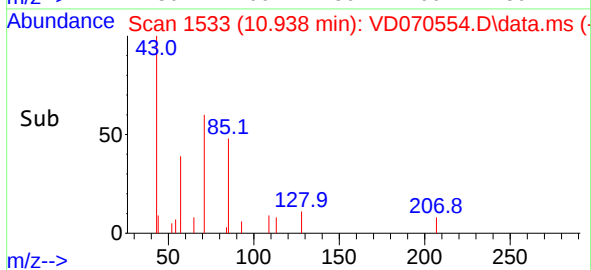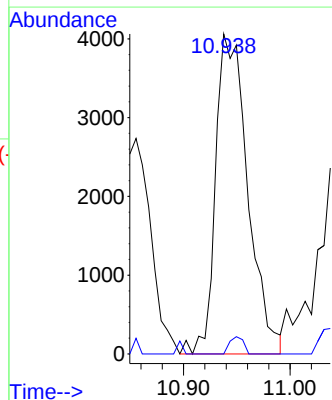







#62
4-Bromofluorobenzene
Concen: 47.440 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121

Tgt Ion: 95 Resp: 348433




Ion	Ratio	Lower	Upper
95	100		
174	69.1	0.0	140.6
176	66.2	0.0	137.4

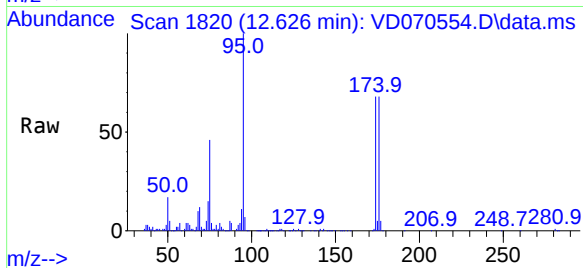


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 117 Resp: 760264


Ion	Ratio	Lower	Upper
117	100		
82	56.3	45.0	67.4
119	31.8	25.2	37.8

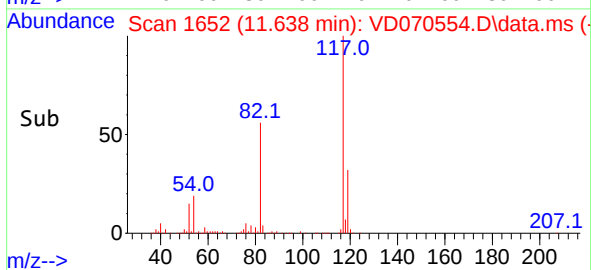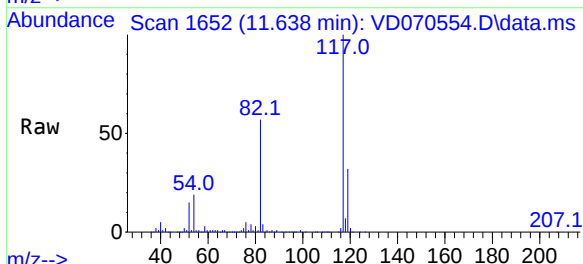






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.006 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41


Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121





Tgt Ion:152 Resp: 328693
Ion Ratio Lower Upper
152 100
115 66.8 32.1 96.3
150 156.1 0.0 350.6

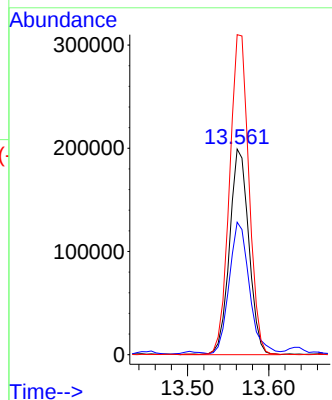


#73
Isopropylbenzene
Concen: 1.053 ug/l
RT: 12.473 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41



Tgt Ion:105 Resp: 24271
Ion Ratio Lower Upper
105 100
120 26.8 13.0 38.9



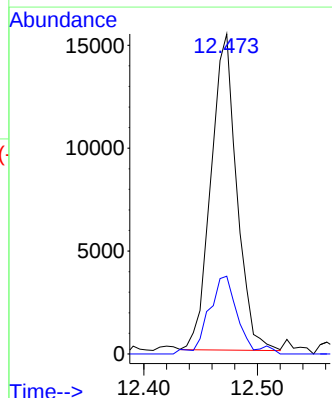
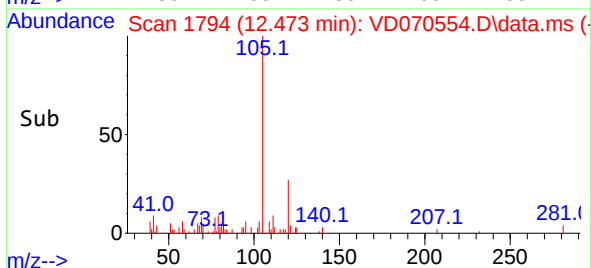




#74
N-amy1 acetate
Concen: 1.653 ug/l
RT: 12.255 min Scan# 1757
Delta R.T. -0.024 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion:	43	Resp:	8304
Ion	Ratio	Lower	Upper
43	100		
70	34.9	41.4	62.0#
55	0.0	22.8	34.2#
61	0.0	21.8	32.6#

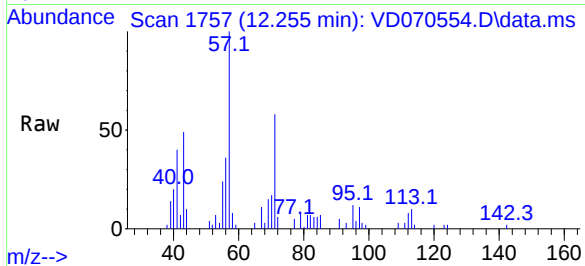

#76
1,2,3-Trichloropropane
Concen: 49.521 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.147 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion:	75	Resp:	164646
Ion	Ratio	Lower	Upper
75	100		
77	2.7	174.9	524.7#


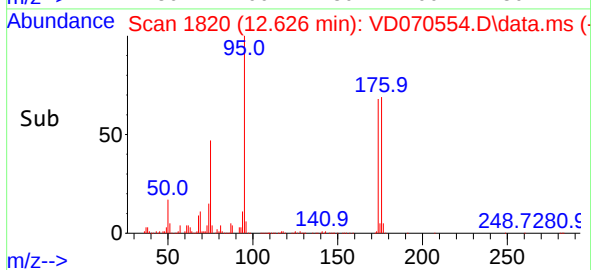

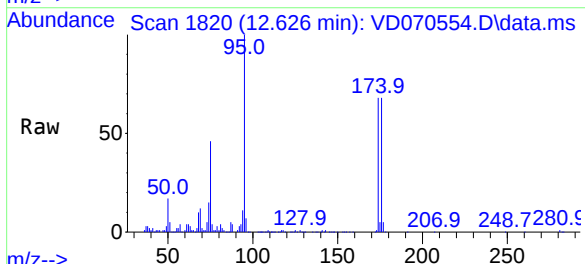




#78
n-propylbenzene
Concen: 2.883 ug/l
RT: 12.808 min Scan# 1851
Delta R.T. -0.006 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 91 Resp: 86258
Ion Ratio Lower Upper
91 100
120 24.4 11.0 33.0

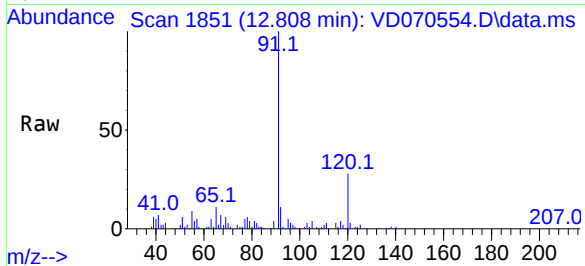

#80
1,3,5-Trimethylbenzene
Concen: 3.762 ug/l
RT: 12.949 min Scan# 1875
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion:105 Resp: 74842
Ion Ratio Lower Upper
105 100
120 46.4 24.1 72.2


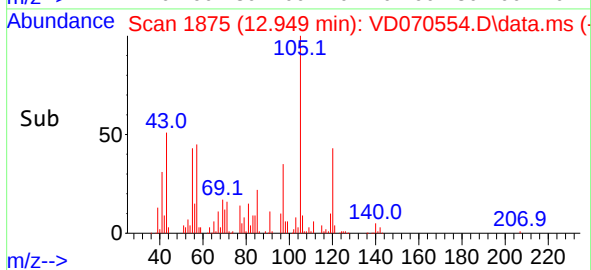

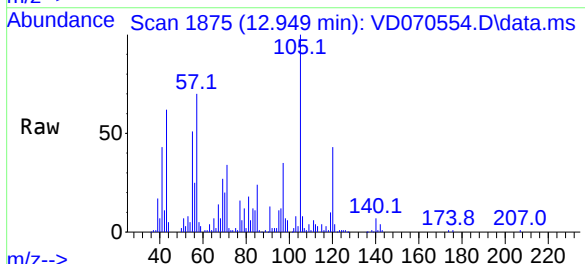


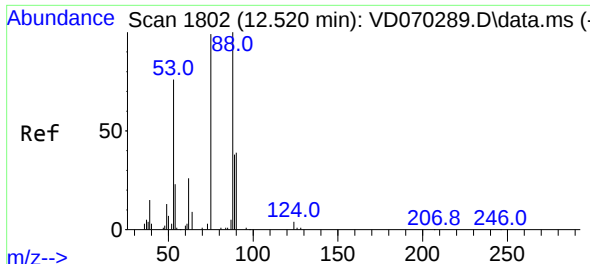

#81
trans-1,4-Dichloro-2-butene
Concen: 124.079 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.106 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 75 Resp: 164646
Ion Ratio Lower Upper
75 100
53 0.4 64.2 96.2#
89 0.0 35.6 53.4#



#84
1,2,4-Trimethylbenzene
Concen: 11.332 ug/l
RT: 13.261 min Scan# 1928
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 105 Resp: 221992
Ion Ratio Lower Upper
105 100
120 44.2 22.3 66.8


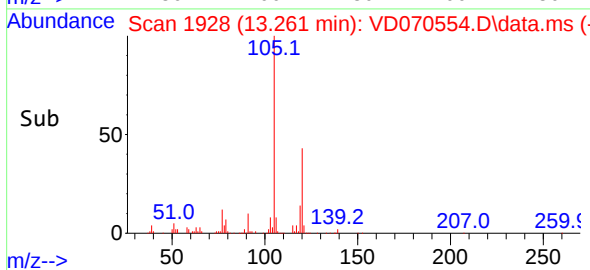

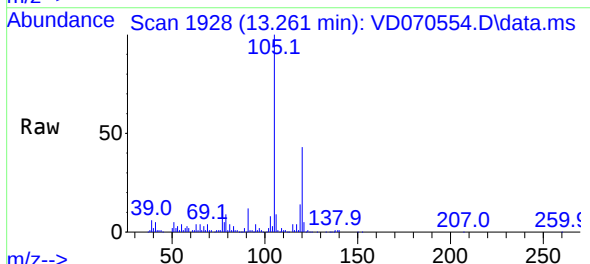




#85
sec-Butylbenzene
Concen: 1.605 ug/l
RT: 13.391 min Scan# 1950
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion:105 Resp: 40696
Ion Ratio Lower Upper
105 100
134 46.9 9.8 29.3#

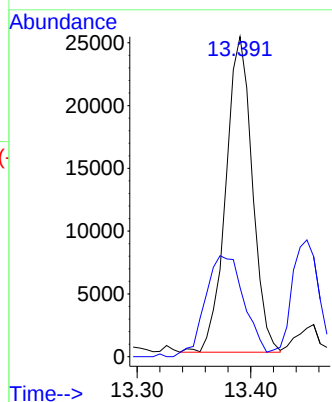

#86
p-Isopropyltoluene
Concen: 2.662 ug/l
RT: 13.502 min Scan# 1969
Delta R.T. -0.006 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion:119 Resp: 54250
Ion Ratio Lower Upper
119 100
134 25.8 12.7 38.0
91 25.4 11.8 35.3


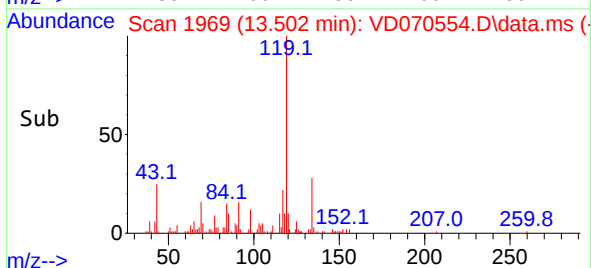
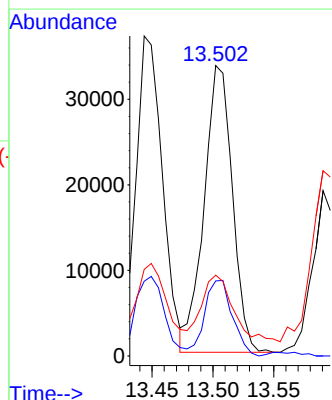





#89
n-Butylbenzene
Concen: 7.678 ug/l
RT: 13.832 min Scan# 2025
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41




Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121


Tgt Ion: 91 Resp: 155993
Ion Ratio Lower Upper
91 100
92 56.3 26.8 80.4
134 0.0 12.1 36.3#

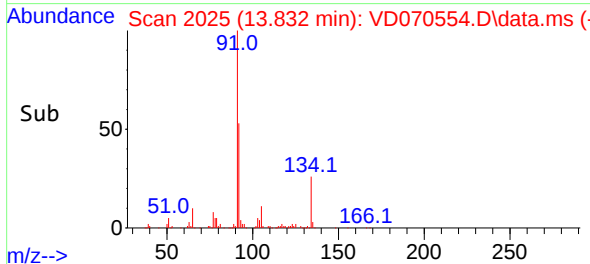

#90
Hexachloroethane
Concen: 32.620 ug/l
RT: 14.102 min Scan# 2071
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion: 117 Resp: 152159
Ion Ratio Lower Upper
117 100
201 0.2 31.9 95.9#


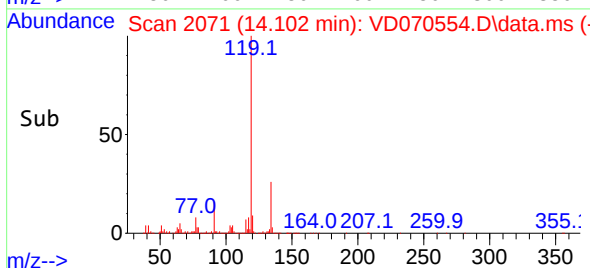
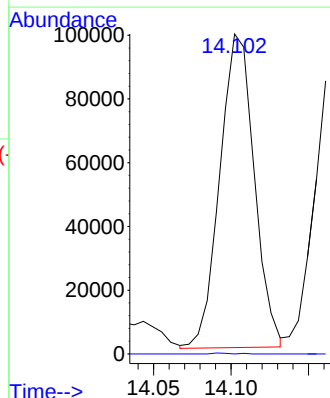
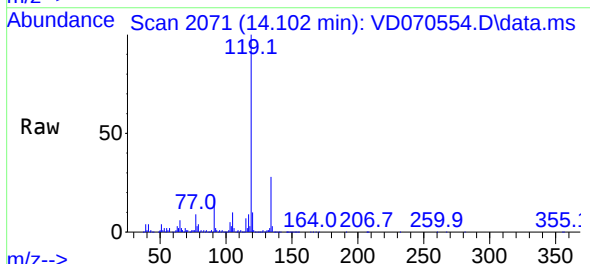




#92
1,2-Dibromo-3-Chloropropane
Concen: 13.018 ug/l
RT: 14.508 min Scan# 2140
Delta R.T. 0.018 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Instrument :
MSVOA_D
ClientSampleId :
NB-08-100121

Tgt Ion: 75 Resp: 9625
Ion Ratio Lower Upper
75 100
155 0.0 40.3 120.9#
157 0.0 48.9 146.6#

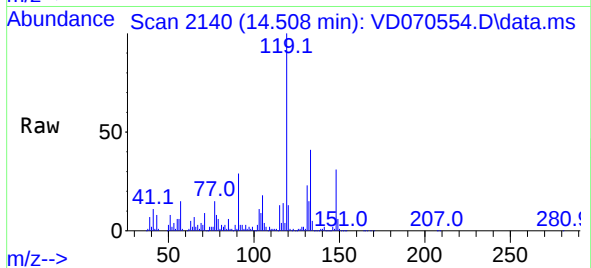

#95
Naphthalene
Concen: 424.050 ug/l
RT: 15.385 min Scan# 2289
Delta R.T. -0.000 min
Lab File: VD070554.D
Acq: 04 Oct 2021 16:41

Tgt Ion:128 Resp: 4065564
Ion Ratio Lower Upper
128 100
127 13.2 10.5 15.7
129 11.0 9.0 13.4

