


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100421\
Data File : VD070544.D
Acq On : 04 Oct 2021 09:55
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Title : SW846 8260
Last Update : Thu Sep 09 03:07:09 2021

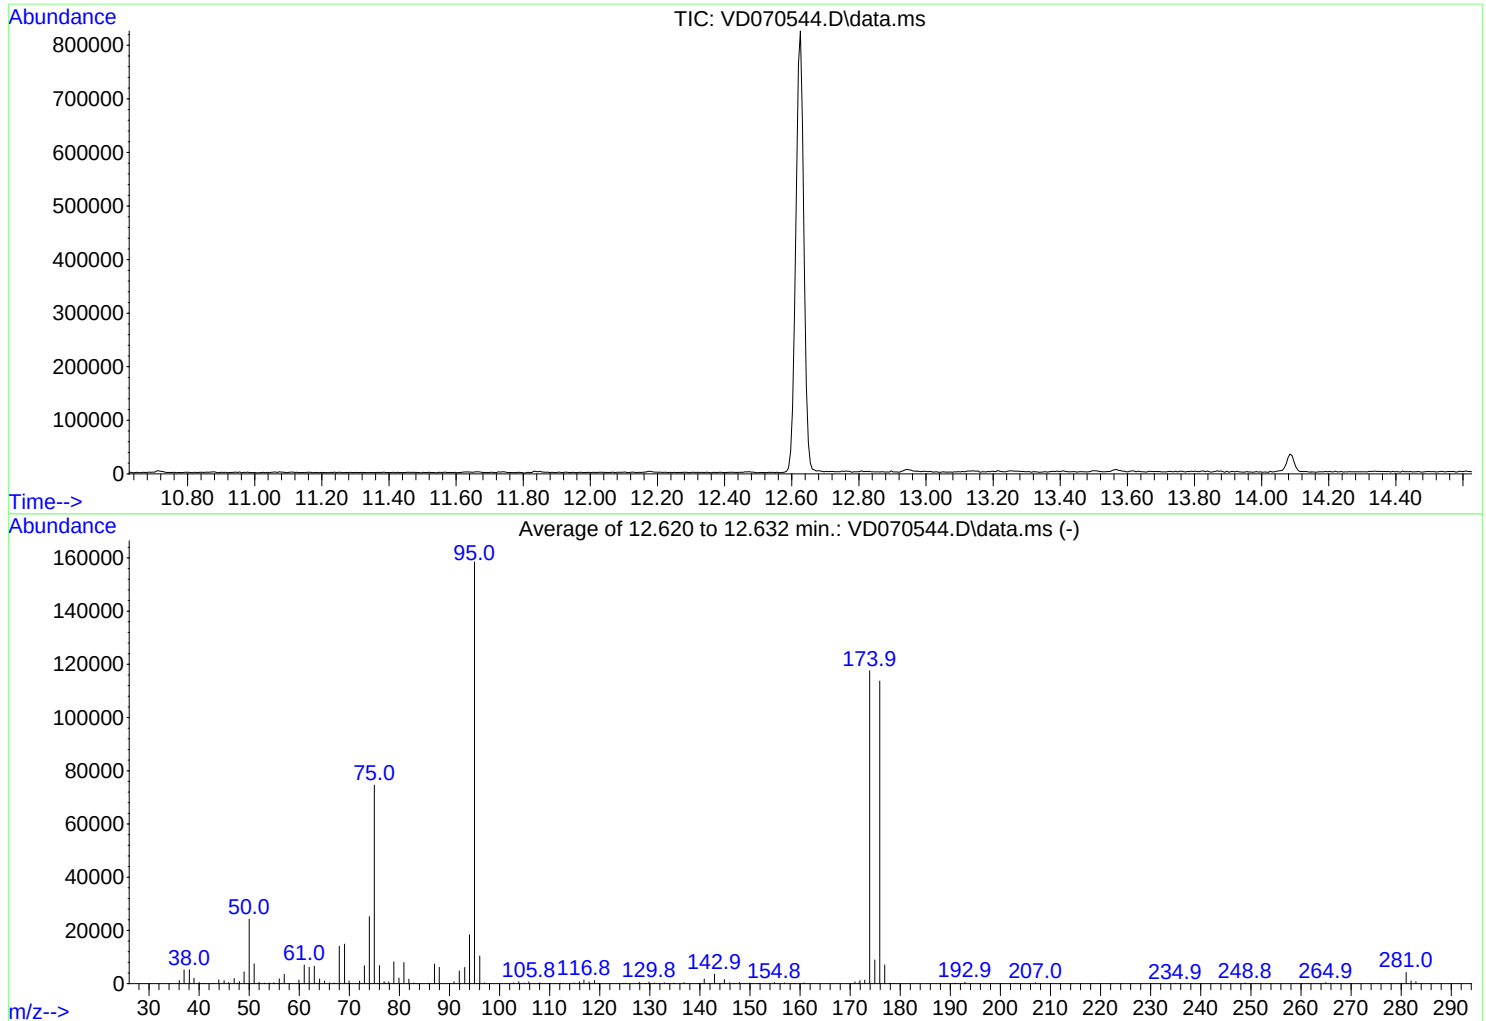

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	24256	PASS
75	95	30	60	47.1	74619	PASS
95	95	100	100	100.0	158528	PASS
96	95	5	9	6.6	10407	PASS
173	174	0.00	2	1.1	1309	PASS
174	95	50	100	74.2	117568	PASS
175	174	5	9	7.5	8876	PASS
176	174	95	101	96.7	113715	PASS
177	176	5	9	6.2	7036	PASS